

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122220\
 Data File : PO074074.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Dec 2020 4:57
 Operator : DD\AJ
 Sample : L5168-03
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S13-03-C

Manual Integrations
 APPROVED

Ankita
 12/23/2020 2:55:24 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 23 10:18:14 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121020.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 11 03:58:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.934	3.992	1777177	1063350	19.438	19.825
2) SA Decachlor...	10.954	9.251	1133511	631703	13.716	13.501m
Target Compounds						
41) L9 AR-1268-1	9.450	8.178	991681	605424	69.625	62.911
42) L9 AR-1268-2	9.546	8.242	593800	370620	48.171	44.986
43) L9 AR-1268-3	9.772	8.449	617520	435547	56.898	61.685
44) L9 AR-1268-4	10.208	8.735	133543	105849	28.507m	35.760 #
45) L9 AR-1268-5	10.621	9.013	1719691	957967	52.548	47.684

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122220\
Data File : PO074074.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Dec 2020 4:57
Operator : DD\AJ
Sample : L5168-03
Misc :
ALS Vial : 58 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
S13-03-C


Manual Integrations
APPROVED

Ankita
12/23/2020 2:55:24 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 23 10:18:14 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121020.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 11 03:58:06 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

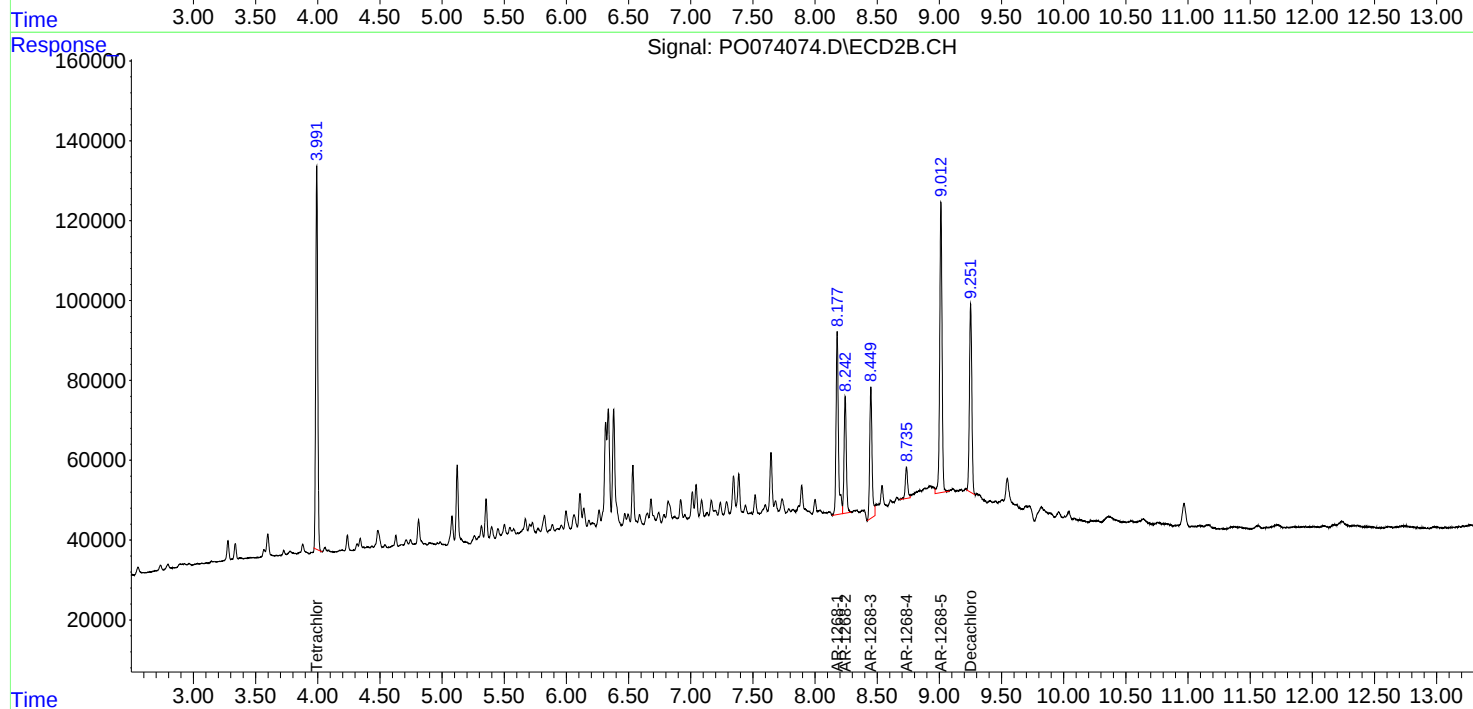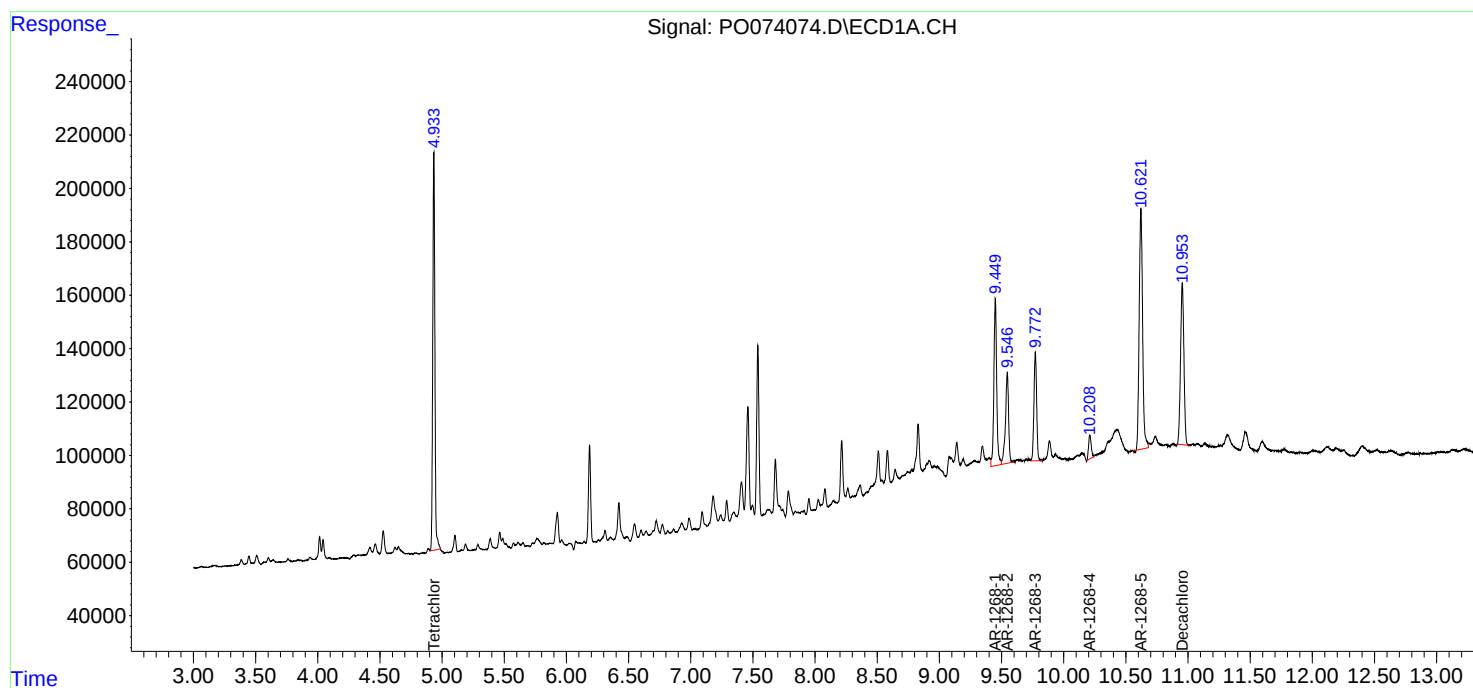

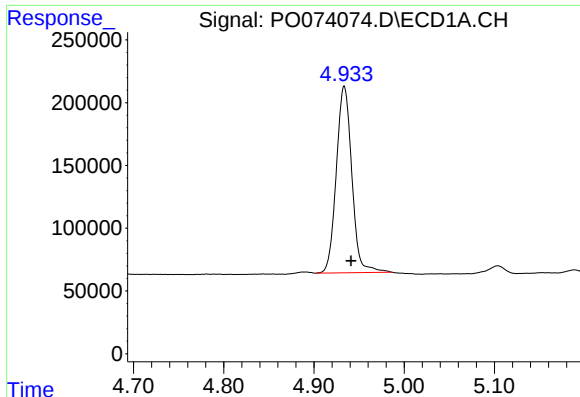


#1 Tetrachloro-m-xylene

R.T.: 4.934 min
Delta R.T.: -0.007 min
Response: 1777177
Conc: 19.44 ng/ml

Instrument :
ECD_O
ClientSampleId :
S13-03-C


Manual Integrations
APPROVED

Ankita
12/23/2020 2:55:24 PM

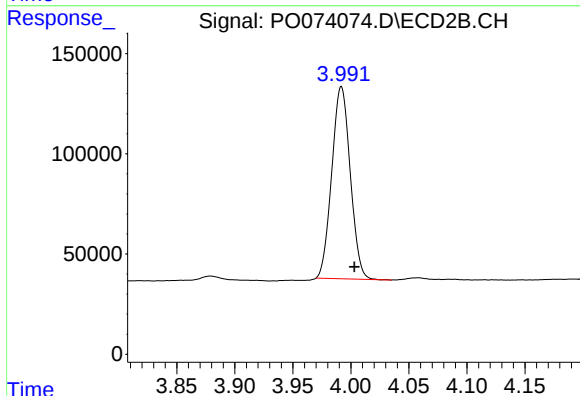


#1 Tetrachloro-m-xylene

R.T.: 3.992 min
Delta R.T.: -0.011 min
Response: 1063350
Conc: 19.83 ng/ml

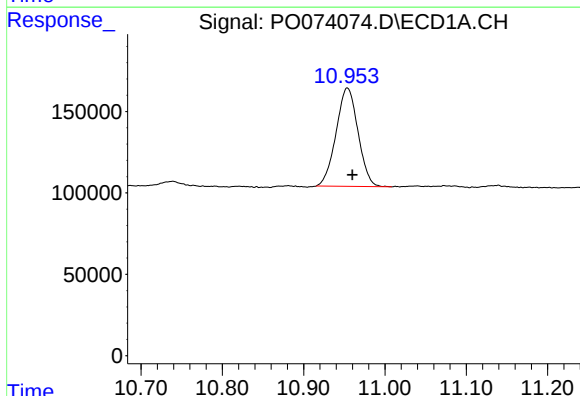


#2 Decachlorobiphenyl

R.T.: 10.954 min
Delta R.T.: -0.006 min
Response: 1133511
Conc: 13.72 ng/ml

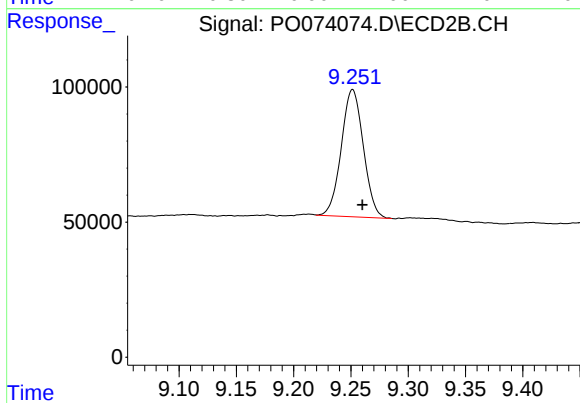

#2 Decachlorobiphenyl

R.T.: 9.251 min
Delta R.T.: -0.009 min
Response: 631703
Conc: 13.50 ng/ml m

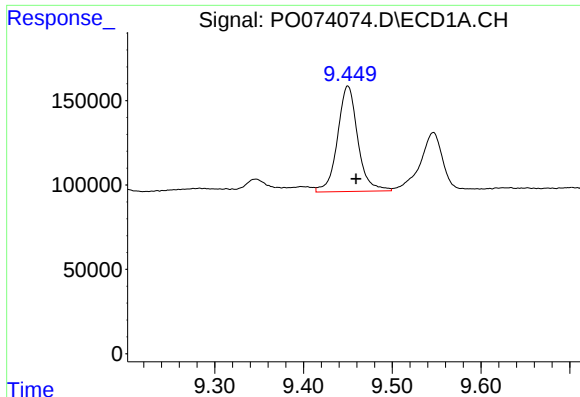


#41 AR-1268-1

R.T.: 9.450 min
Delta R.T.: -0.009 min
Response: 991681
Conc: 69.63 ng/ml

Instrument :
ECD_O
ClientSampleId :
S13-03-C


Manual Integrations
APPROVED

Ankita
12/23/2020 2:55:24 PM

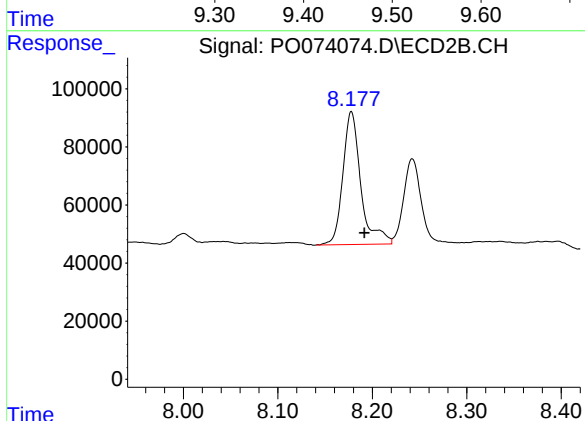


#41 AR-1268-1

R.T.: 8.178 min
Delta R.T.: -0.014 min
Response: 605424
Conc: 62.91 ng/ml

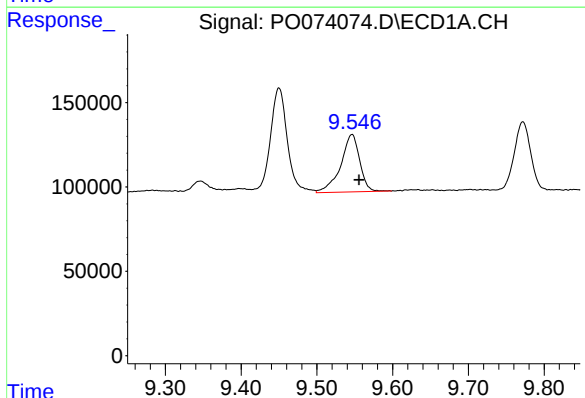


#42 AR-1268-2

R.T.: 9.546 min
Delta R.T.: -0.009 min
Response: 593800
Conc: 48.17 ng/ml

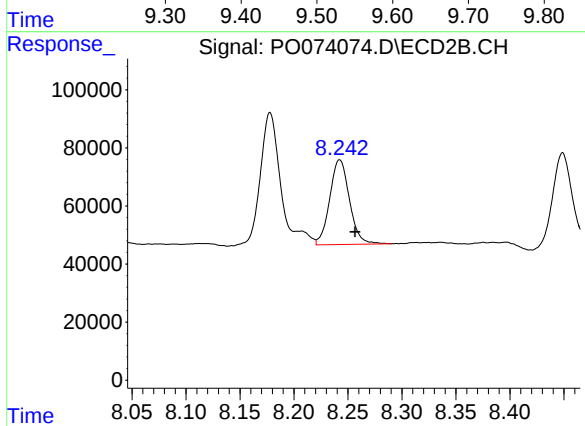

#42 AR-1268-2

R.T.: 8.242 min
Delta R.T.: -0.014 min
Response: 370620
Conc: 44.99 ng/ml

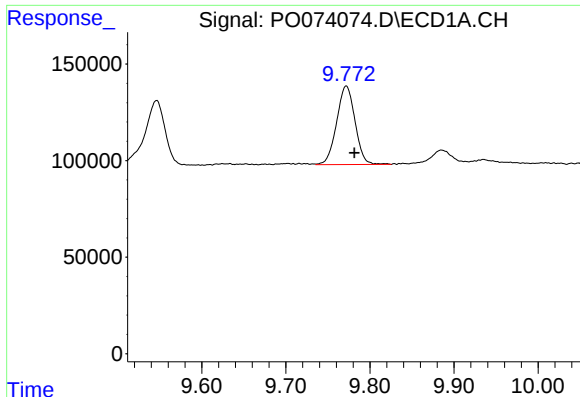


#43 AR-1268-3

R.T.: 9.772 min
Delta R.T.: -0.010 min
Response: 617520
Conc: 56.90 ng/ml

Instrument :
ECD_O
ClientSampleId :
S13-03-C


Manual Integrations
APPROVED

Ankita
12/23/2020 2:55:24 PM

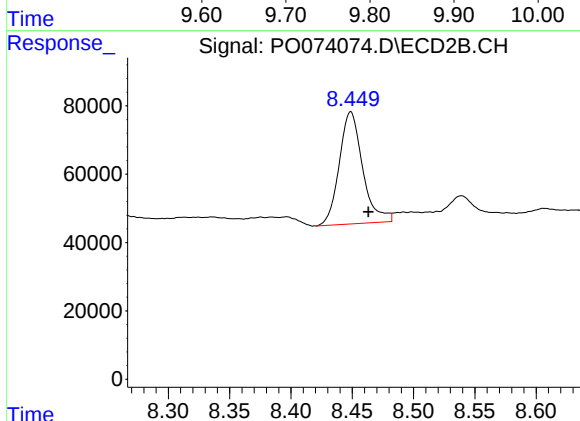


#43 AR-1268-3

R.T.: 8.449 min
Delta R.T.: -0.014 min
Response: 435547
Conc: 61.68 ng/ml

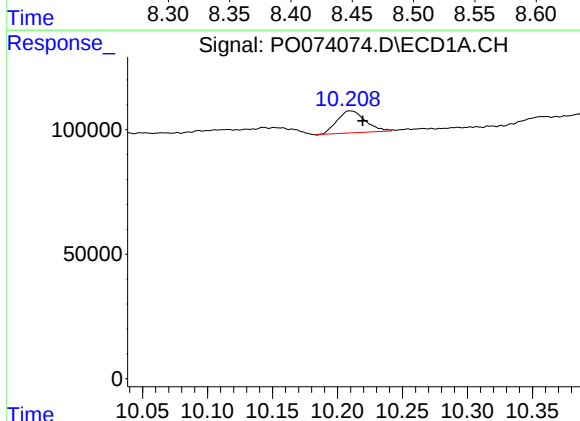


#44 AR-1268-4

R.T.: 10.208 min
Delta R.T.: -0.011 min
Response: 133543
Conc: 28.51 ng/ml m

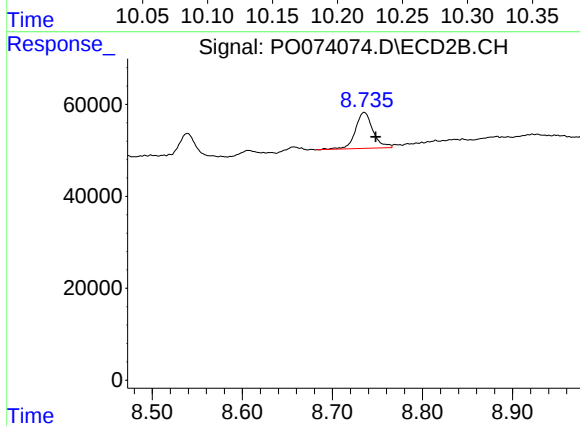

#44 AR-1268-4

R.T.: 8.735 min
Delta R.T.: -0.013 min
Response: 105849
Conc: 35.76 ng/ml

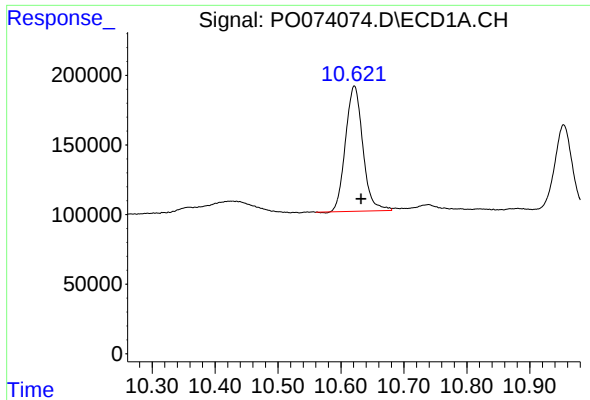


#45 AR-1268-5

R.T.: 10.621 min
Delta R.T.: -0.011 min
Response: 1719691
Conc: 52.55 ng/ml

Instrument :
ECD_O
ClientSampleId :
S13-03-C

Manual Integrations
APPROVED

Ankita
12/23/2020 2:55:24 PM

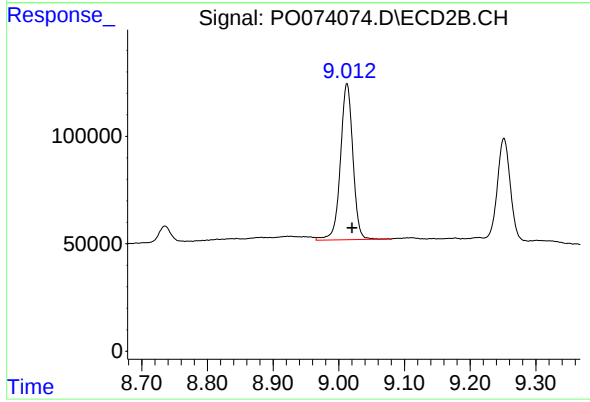

#45 AR-1268-5

R.T.: 9.013 min
Delta R.T.: -0.007 min
Response: 957967
Conc: 47.68 ng/ml