

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122223\
 Data File : PO100709.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Dec 2023 17:23
 Operator : YP/AJ
 Sample : 05991-01 10X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BC122669LOK-END-1-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/26/2023
 Supervised By :Ankita Jodhani 12/26/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 22 22:22:37 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO122023.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Dec 21 04:28:19 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.347	3.643	5971957	3829431	1.914	1.874m
2) SA Decachlor...	10.089	8.704	4874723	3102243	2.333	2.055m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122223\
Data File : PO100709.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Dec 2023 17:23
Operator : YP/AJ
Sample : 05991-01 10X
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
BC122669LOK-END-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/26/2023
Supervised By :Ankita Jodhani 12/26/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 22 22:22:37 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO122023.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Dec 21 04:28:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

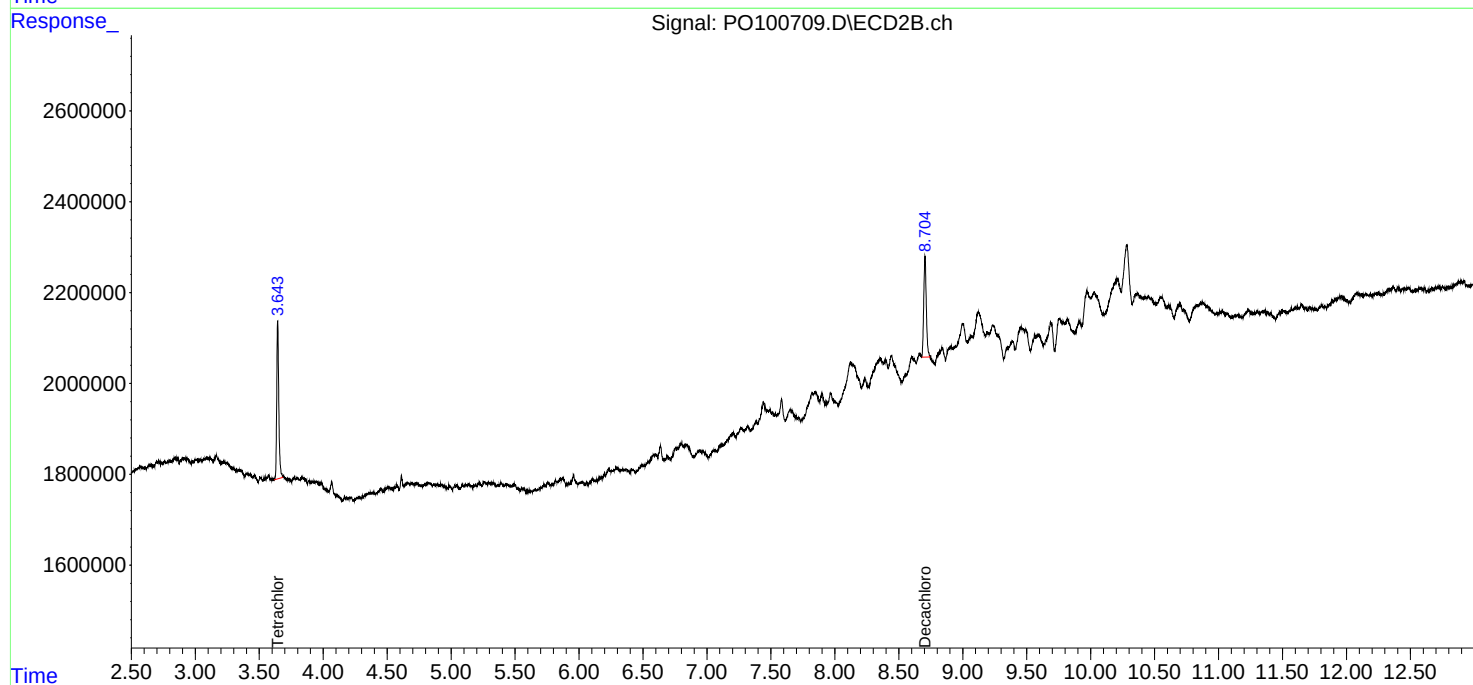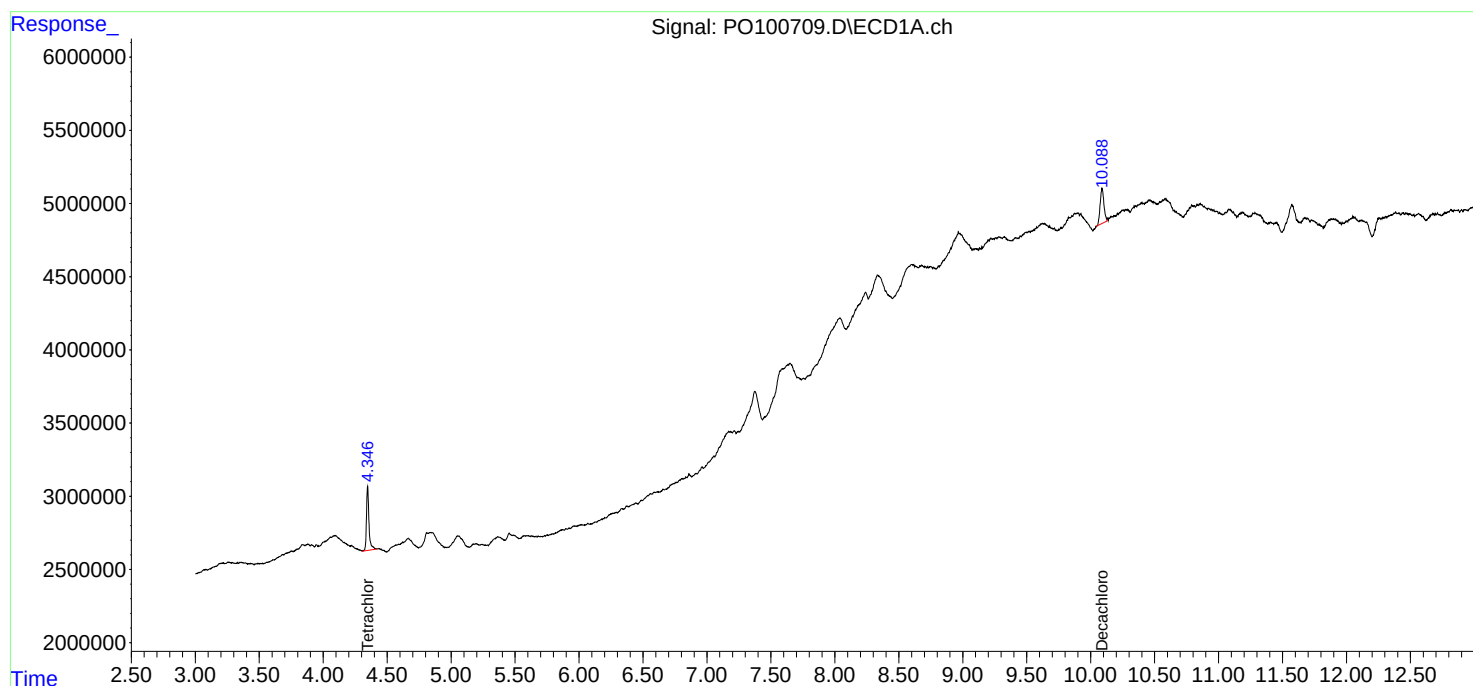

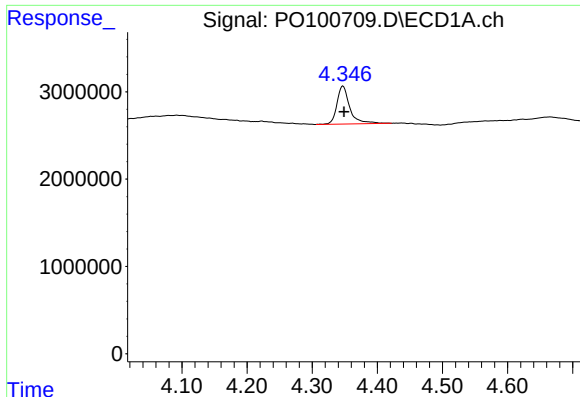


#1 Tetrachloro-m-xylene

R.T.: 4.347 min
Delta R.T.: -0.002 min
Response: 5971957
Conc: 1.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
BC122669LOK-END-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/26/2023
Supervised By :Ankita Jodhani 12/26/2023

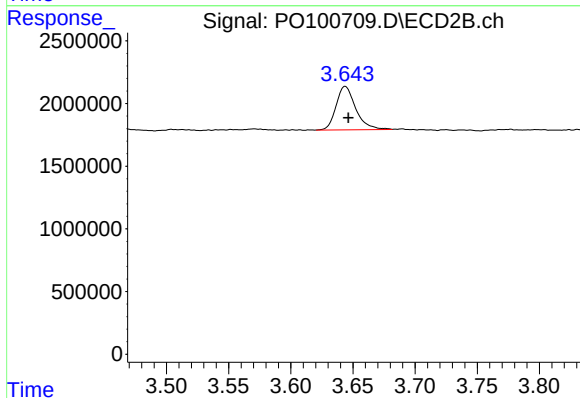


#1 Tetrachloro-m-xylene

R.T.: 3.643 min
Delta R.T.: -0.003 min
Response: 3829431
Conc: 1.87 ng/ml m

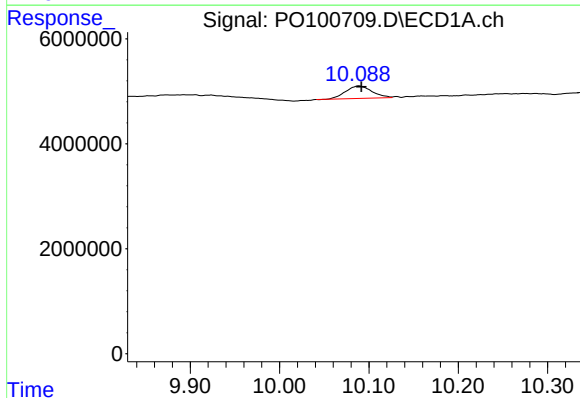

#2 Decachlorobiphenyl

R.T.: 10.089 min
Delta R.T.: -0.003 min
Response: 4874723
Conc: 2.33 ng/ml

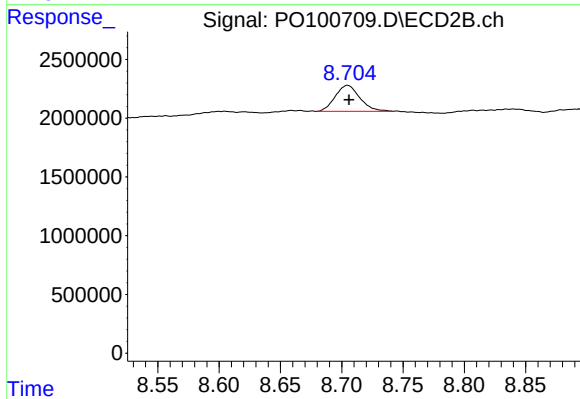

#2 Decachlorobiphenyl

R.T.: 8.704 min
Delta R.T.: -0.002 min
Response: 3102243
Conc: 2.06 ng/ml m