

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122223\
 Data File : PO100712.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Dec 2023 18:13
 Operator : YP/AJ
 Sample : 05991-04 10X
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BC226734LOK-END-1-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/26/2023
 Supervised By :Ankita Jodhani 12/26/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 22 22:23:54 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO122023.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Dec 21 04:28:19 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.368	3.644	4221362	3800012	1.353m	1.860 #
2) SA Decachlor...	10.108	8.704	2877305	2750277	1.377	1.822 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122223\
Data File : PO100712.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Dec 2023 18:13
Operator : YP/AJ
Sample : 05991-04 10X
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
BC226734LOK-END-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/26/2023
Supervised By :Ankita Jodhani 12/26/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 22 22:23:54 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO122023.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Dec 21 04:28:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

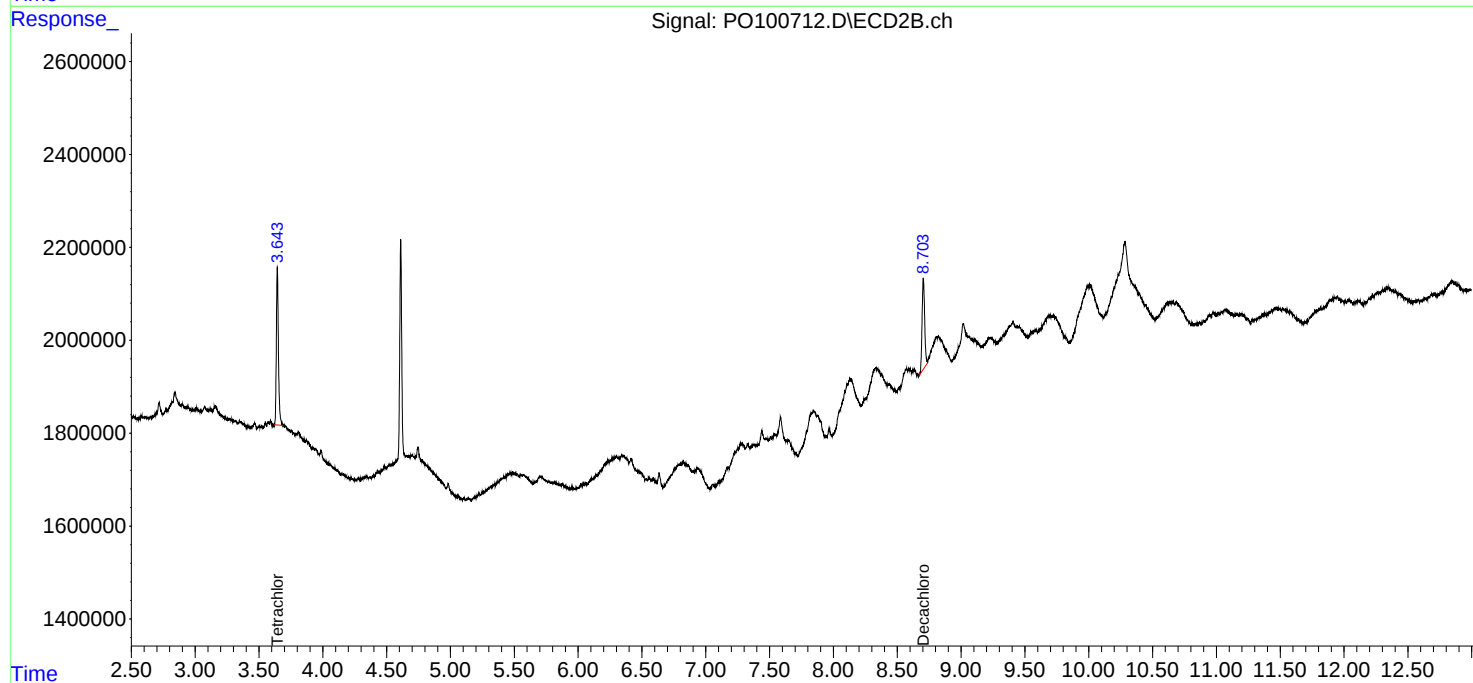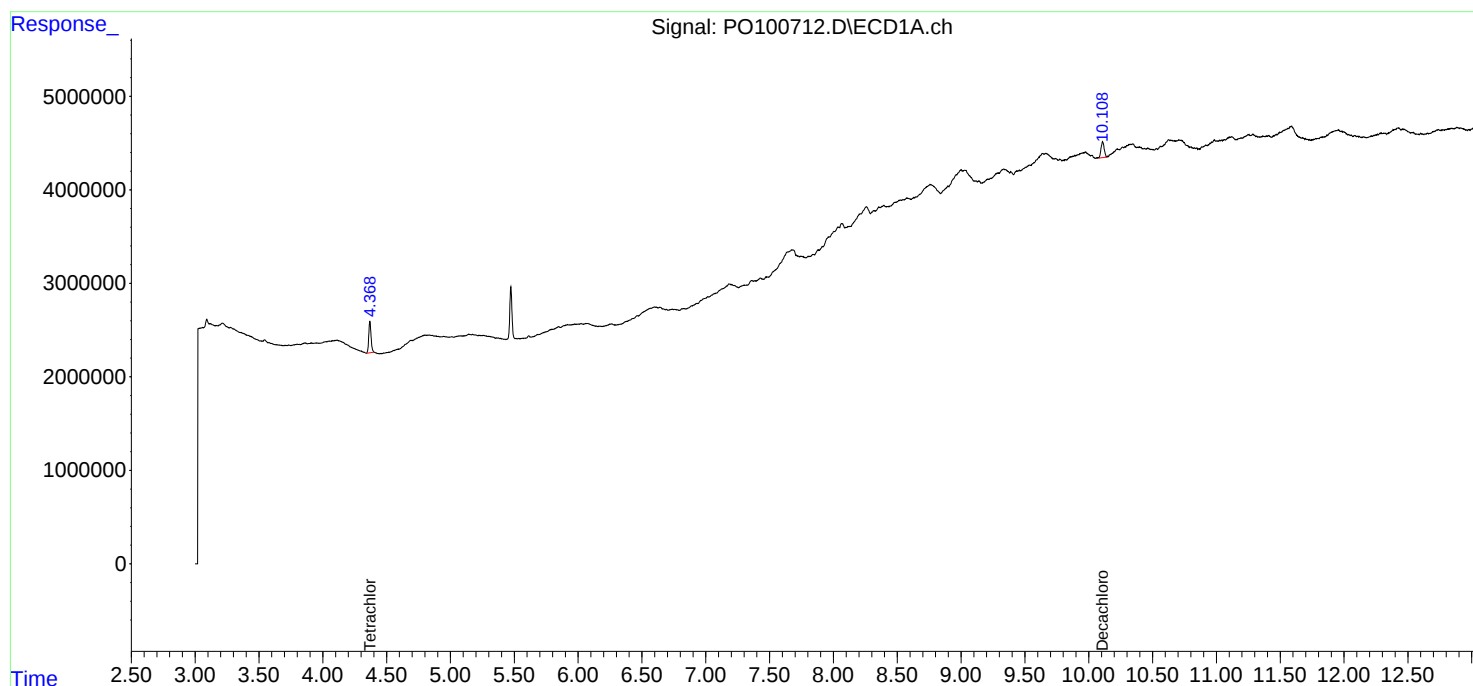

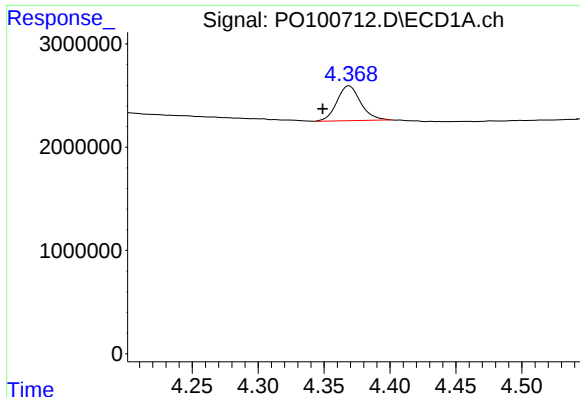


#1 Tetrachloro-m-xylene

R.T.: 4.368 min
Delta R.T.: 0.019 min
Response: 4221362
Conc: 1.35 ng/ml

Instrument :
ECD_O
ClientSampleId :
BC226734LOK-END-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/26/2023
Supervised By :Ankita Jodhani 12/26/2023

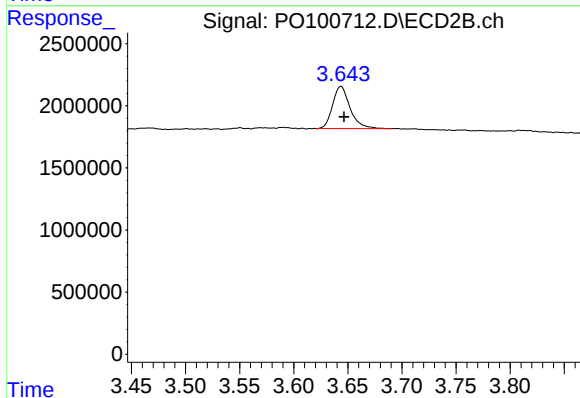


#1 Tetrachloro-m-xylene

R.T.: 3.644 min
Delta R.T.: -0.003 min
Response: 3800012
Conc: 1.86 ng/ml

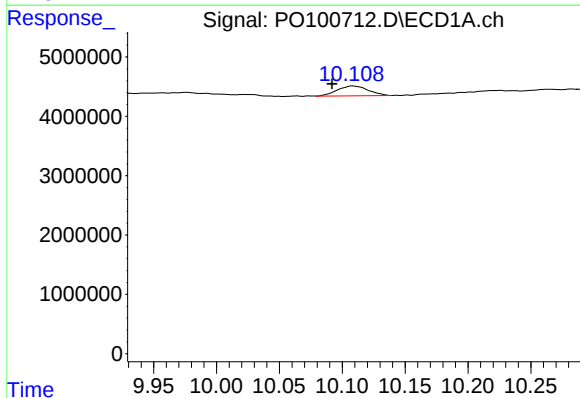

#2 Decachlorobiphenyl

R.T.: 10.108 min
Delta R.T.: 0.017 min
Response: 2877305
Conc: 1.38 ng/ml

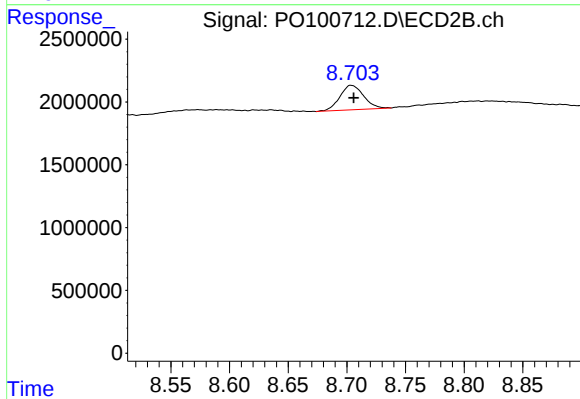

#2 Decachlorobiphenyl

R.T.: 8.704 min
Delta R.T.: -0.002 min
Response: 2750277
Conc: 1.82 ng/ml