

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122223\
 Data File : PO100720.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Dec 2023 21:01
 Operator : YP/AJ
 Sample : 05991-05 10X
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BC260098LOK-END-1-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/26/2023
 Supervised By :Ankita Jodhani 12/26/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 22 22:27:29 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO122023.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Dec 21 04:28:19 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.348	3.644	7343627	4289527	2.354	2.099m
2) SA Decachlor...	10.086	8.705	5536182	3837483	2.650m	2.542m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122223\
Data File : PO100720.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Dec 2023 21:01
Operator : YP/AJ
Sample : 05991-05 10X
Misc :
ALS Vial : 29 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
BC260098LOK-END-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/26/2023
Supervised By :Ankita Jodhani 12/26/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 22 22:27:29 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO122023.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Dec 21 04:28:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

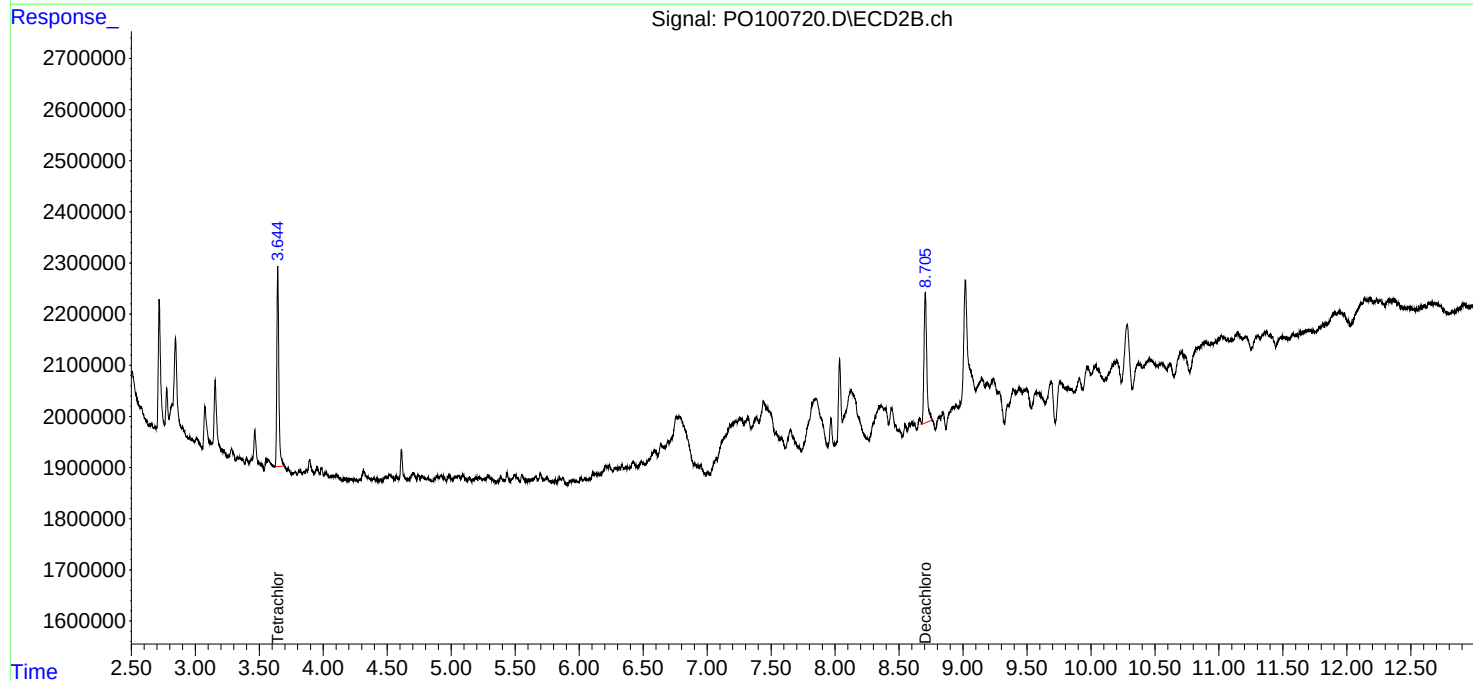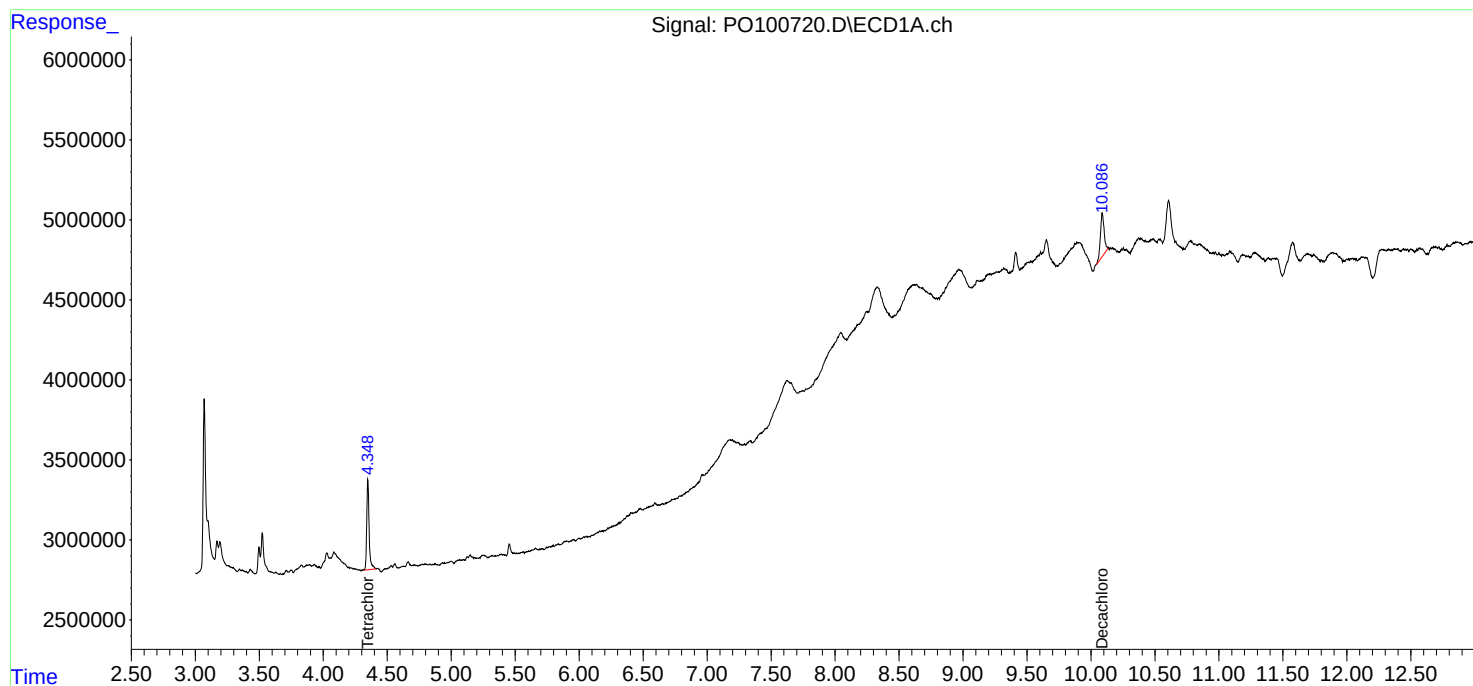

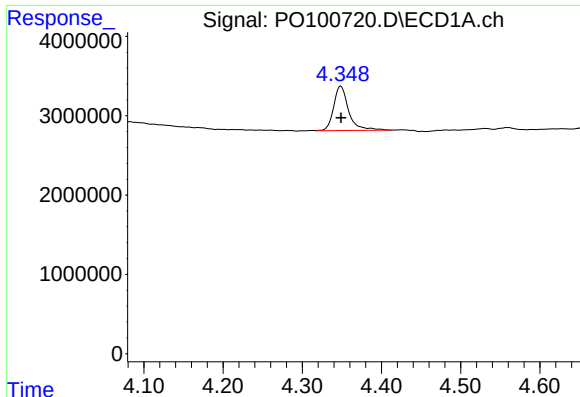


#1 Tetrachloro-m-xylene

R.T.: 4.348 min
Delta R.T.: 0.000 min
Response: 7343627
Conc: 2.35 ng/ml

Instrument :
ECD_O
ClientSampleId :
BC260098LOK-END-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/26/2023
Supervised By :Ankita Jodhani 12/26/2023

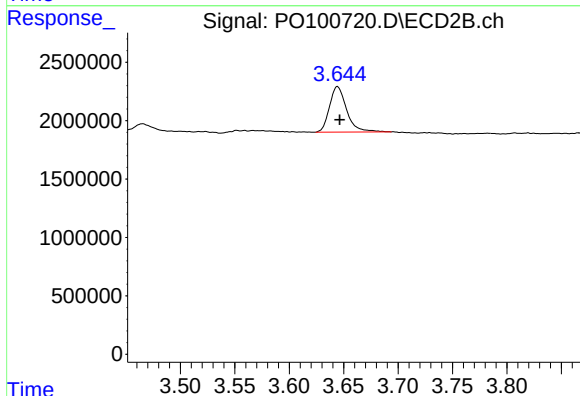


#1 Tetrachloro-m-xylene

R.T.: 3.644 min
Delta R.T.: -0.003 min
Response: 4289527
Conc: 2.10 ng/ml m

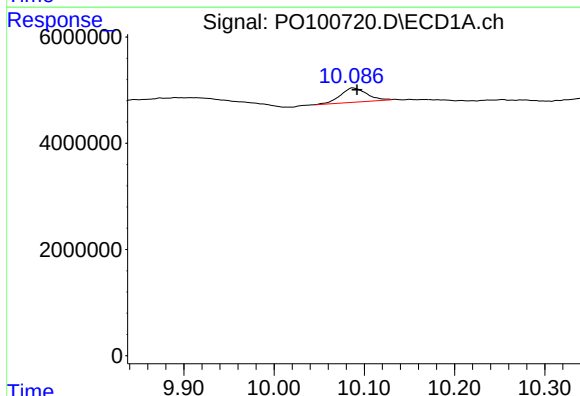

#2 Decachlorobiphenyl

R.T.: 10.086 min
Delta R.T.: -0.006 min
Response: 5536182
Conc: 2.65 ng/ml m

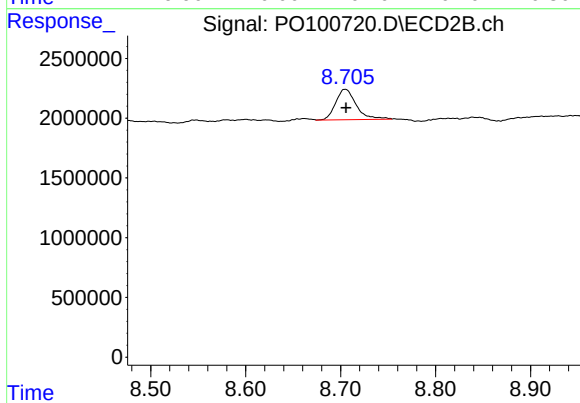

#2 Decachlorobiphenyl

R.T.: 8.705 min
Delta R.T.: -0.001 min
Response: 3837483
Conc: 2.54 ng/ml m