

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0122319\
 Data File : P0064870.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Dec 2019 13:45
 Operator : SM/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 24 05:46:04 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0121319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 13 08:19:24 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.179	3.450	547443	682997	22.487	26.943
2) SA Decachlor...	9.698	8.368	669304	855493	21.808	24.634
Target Compounds						
30) L6 AR-1254-5	7.450	0.000	29130	0	13.845	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122319\
Data File : PO064870.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Dec 2019 13:45
Operator : SM/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 24 05:46:04 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 13 08:19:24 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

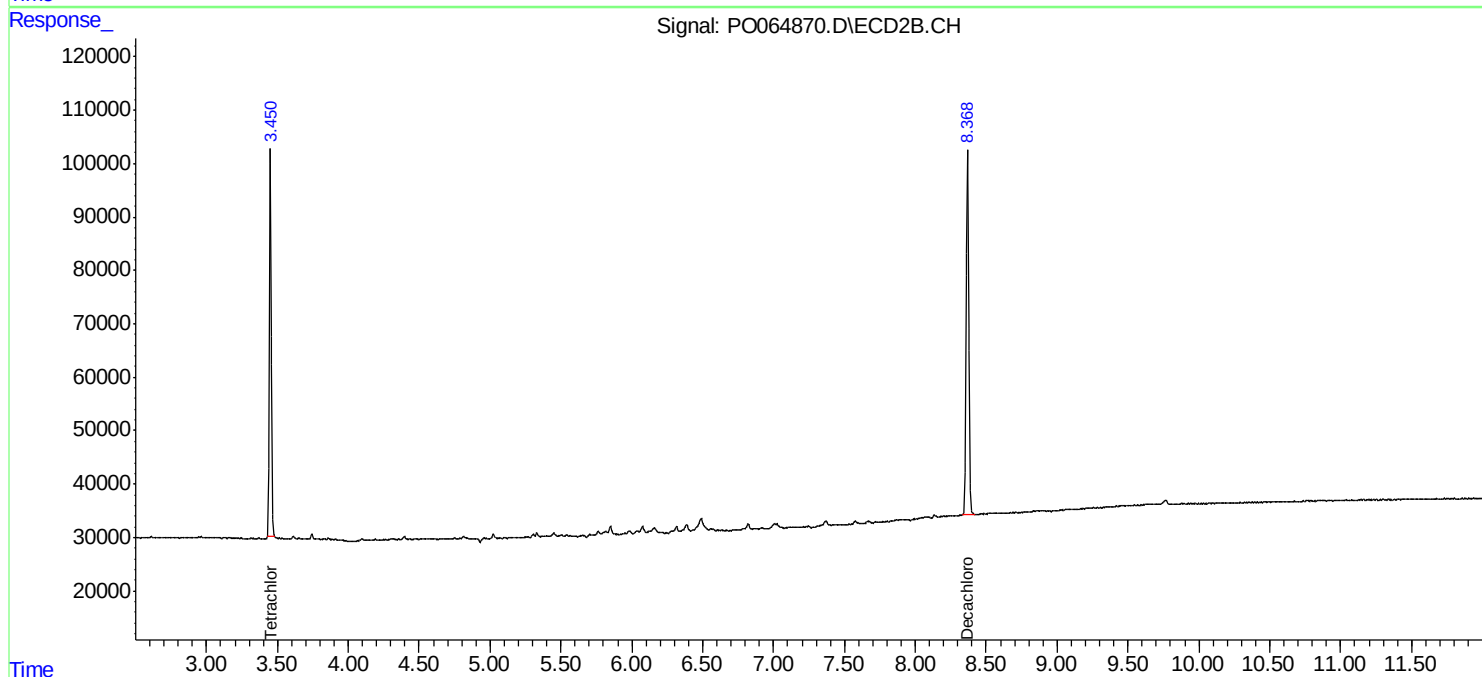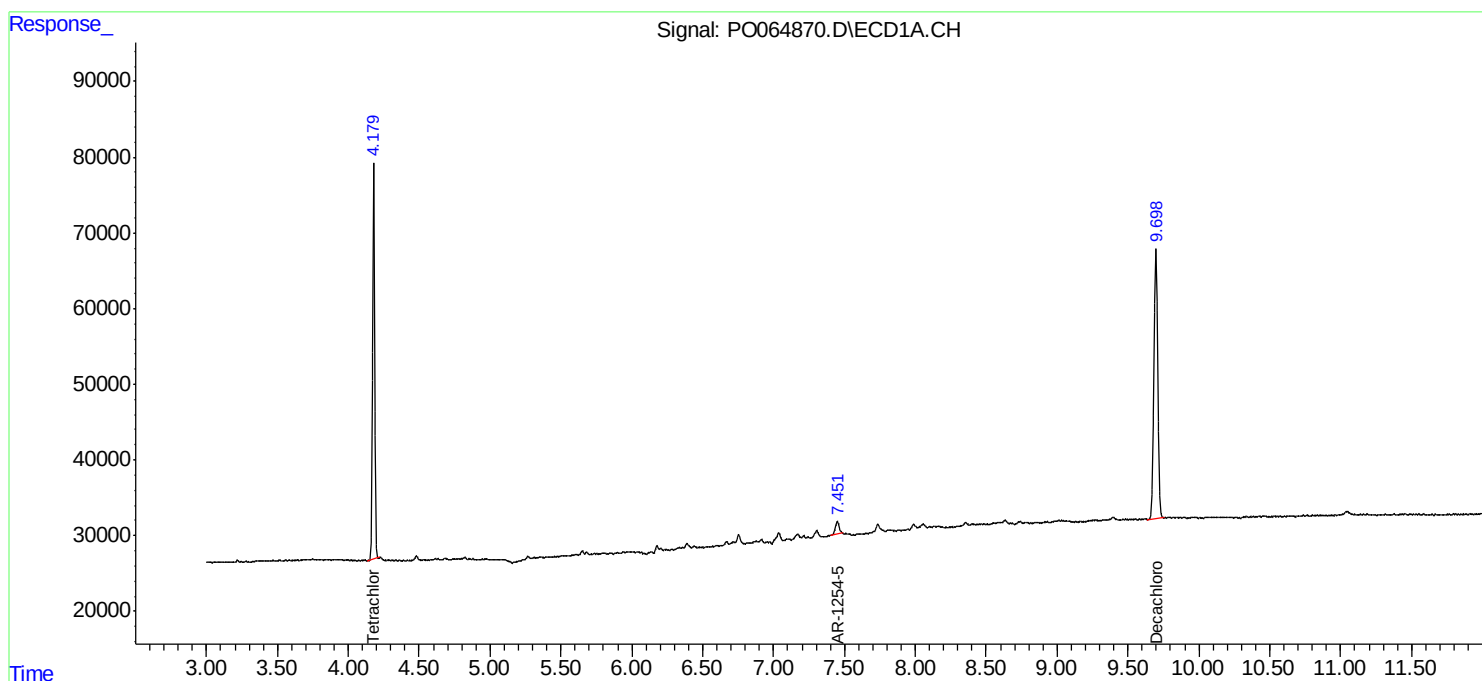


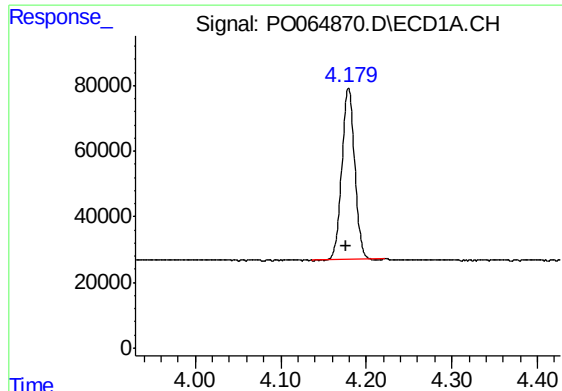

#1 Tetrachloro-m-xylene


R.T.: 4.179 min
Delta R.T.: 0.002 min
Response: 547443
Conc: 22.49 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

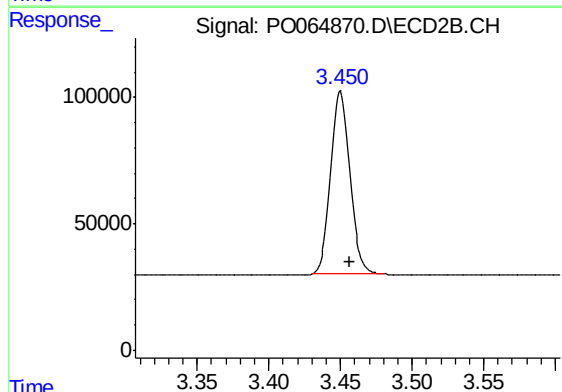


#1 Tetrachloro-m-xylene

R.T.: 3.450 min
Delta R.T.: -0.007 min
Response: 682997
Conc: 26.94 ng/ml

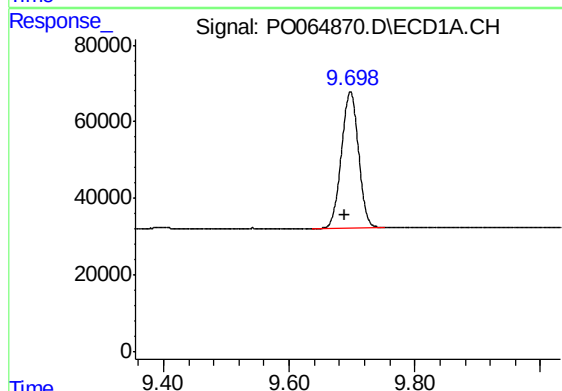


#2 Decachlorobiphenyl

R.T.: 9.698 min
Delta R.T.: 0.010 min
Response: 669304
Conc: 21.81 ng/ml

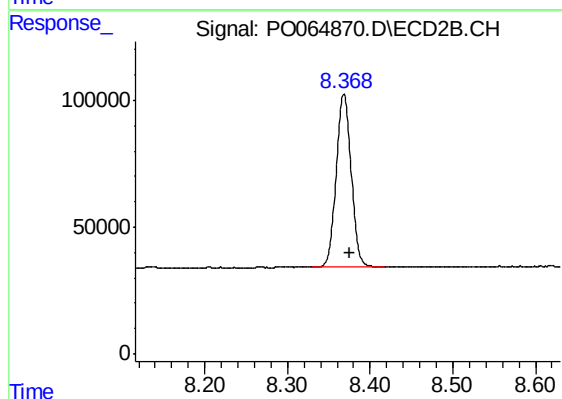

#2 Decachlorobiphenyl


R.T.: 8.368 min
Delta R.T.: -0.008 min
Response: 855493
Conc: 24.63 ng/ml

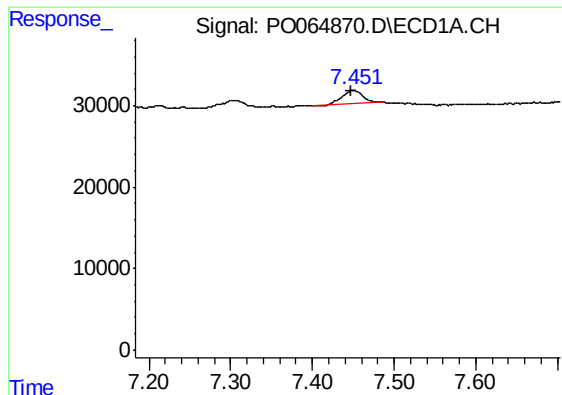

#30 AR-1254-5

R.T.: 7.450 min
Delta R.T.: 0.003 min
Response: 29130
Conc: 13.84 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

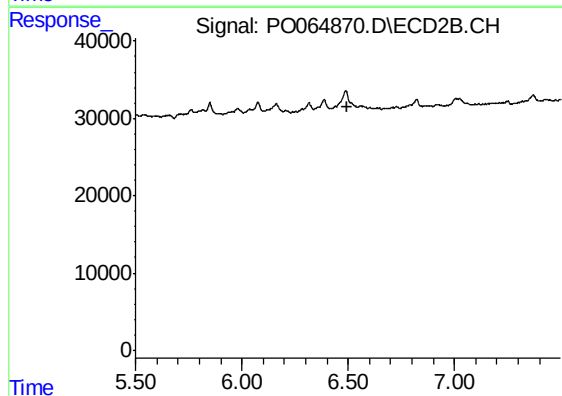

#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 6.499 min
Response: 0
Conc: N.D.