Quantitation Report (QT Reviewed)

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122319\
Data File : PO064884.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Dec 2019 20:03
Operator : SM/AJ
Sample : K6297-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SIMW-02-20191218-A

Manual Integrations APPROVED
Ankita
12/24/2019 2:08:55 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 24 05:52:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 13 08:19:24 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
	System Monitoring Compounds						
1)	SA Tetrachlo...	4.174	3.448	697210	884364	28.639	34.887m
2)	SA Decachlor...	9.690	8.364	574356	740538	18.715	21.324
	Target Compounds						

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122319\
Data File : PO064884.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Dec 2019 20:03
Operator : SM/AJ
Sample : K6297-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SIMW-02-20191218-A

Manual Integrations APPROVED
Ankita
12/24/2019 2:08:55 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 24 05:52:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 13 08:19:24 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

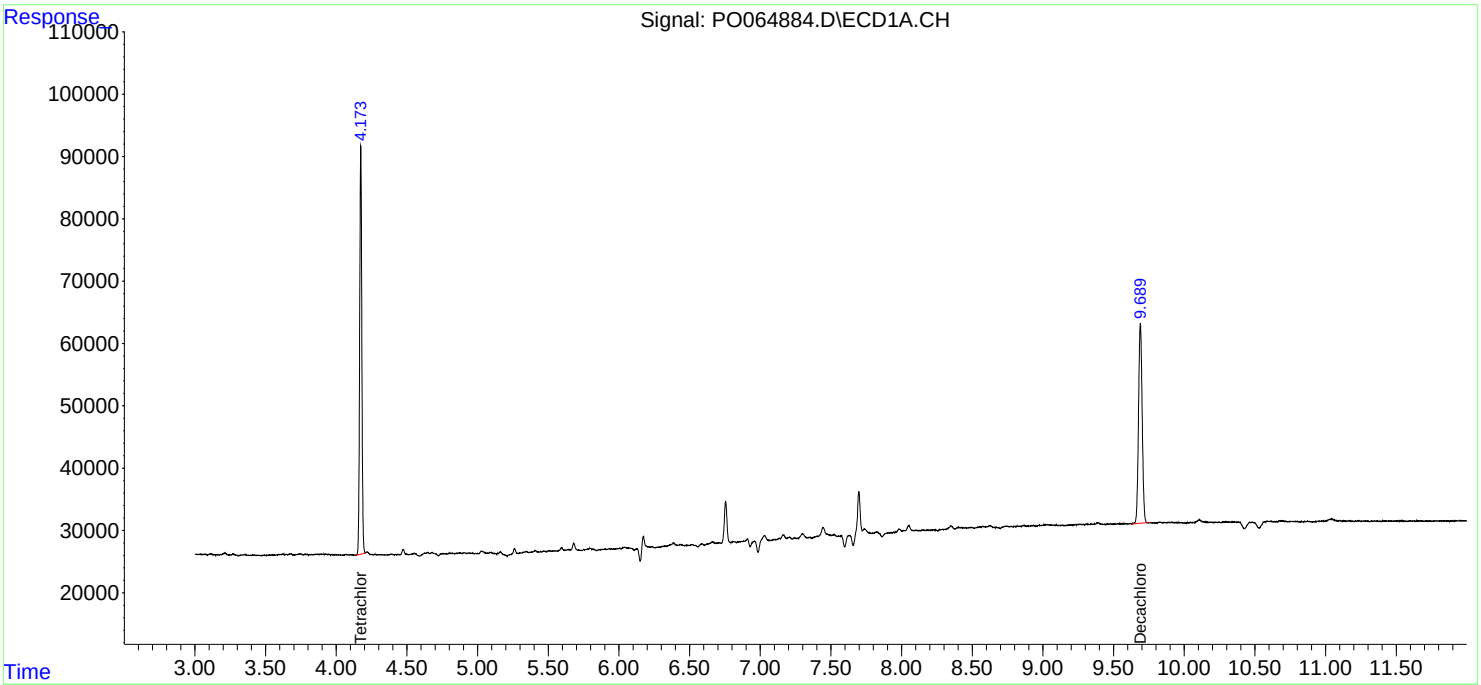

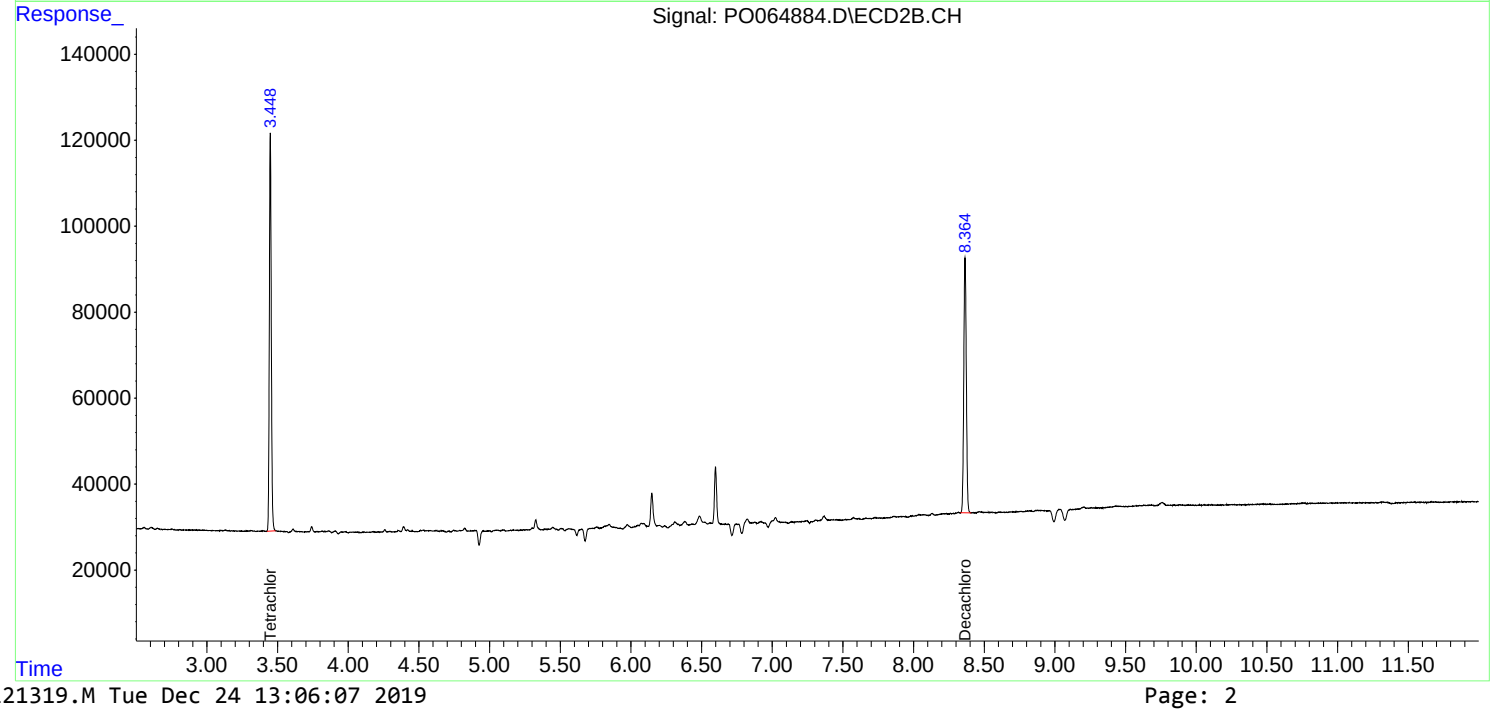

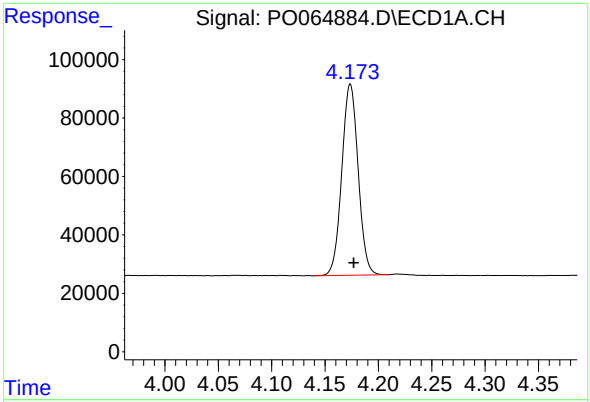

#1 Tetrachloro-m-xylene

R.T.: 4.174 min
Delta R.T.: -0.003 min
Response: 697210
Conc: 28.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
SIMW-02-20191218-A

Manual Integrations APPROVED
Ankita
12/24/2019 2:08:55 PM

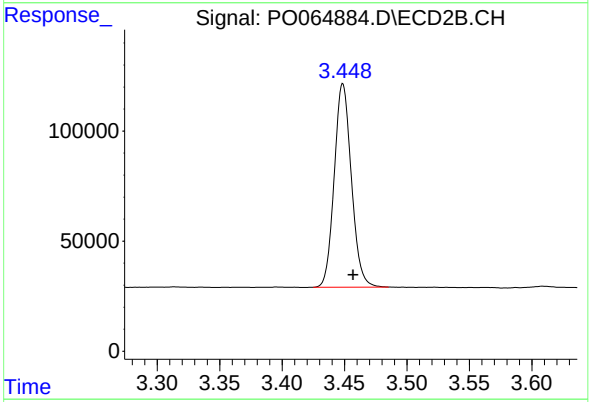

#1 Tetrachloro-m-xylene

R.T.: 3.448 min
Delta R.T.: -0.008 min
Response: 884364
Conc: 34.89 ng/ml m

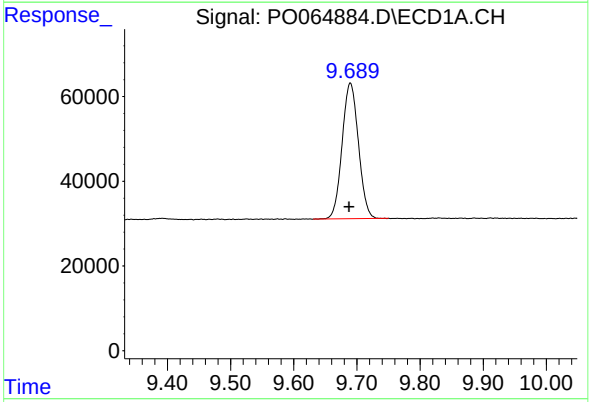

#2 Decachlorobiphenyl

R.T.: 9.690 min
Delta R.T.: 0.002 min
Response: 574356
Conc: 18.71 ng/ml

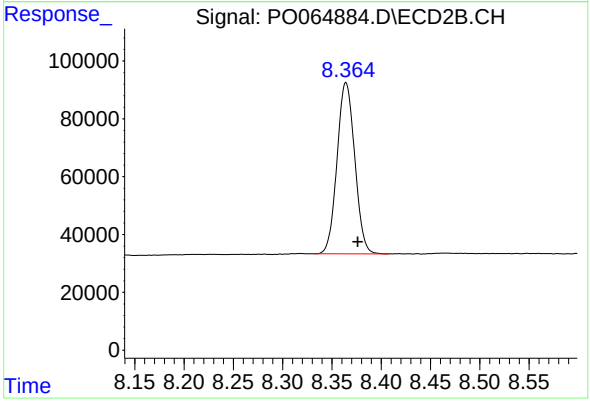

#2 Decachlorobiphenyl

R.T.: 8.364 min
Delta R.T.: -0.012 min
Response: 740538
Conc: 21.32 ng/ml