

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0122319\
 Data File : P0064885.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Dec 2019 20:19
 Operator : SM/AJ
 Sample : K6297-05
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MW-3-20191218

Manual Integrations
 APPROVED

Ankita
 12/24/2019 2:08:58 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 24 05:52:46 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0121319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 13 08:19:24 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.174	3.449	673659	856827	27.671	33.801m
2) SA Decachlor...	9.690	8.366	474925	608955	15.475	17.535

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122319\
Data File : P0064885.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Dec 2019 20:19
Operator : SM/AJ
Sample : K6297-05
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
MW-3-20191218


Manual Integrations
APPROVED

Ankita
12/24/2019 2:08:58 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 24 05:52:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 13 08:19:24 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

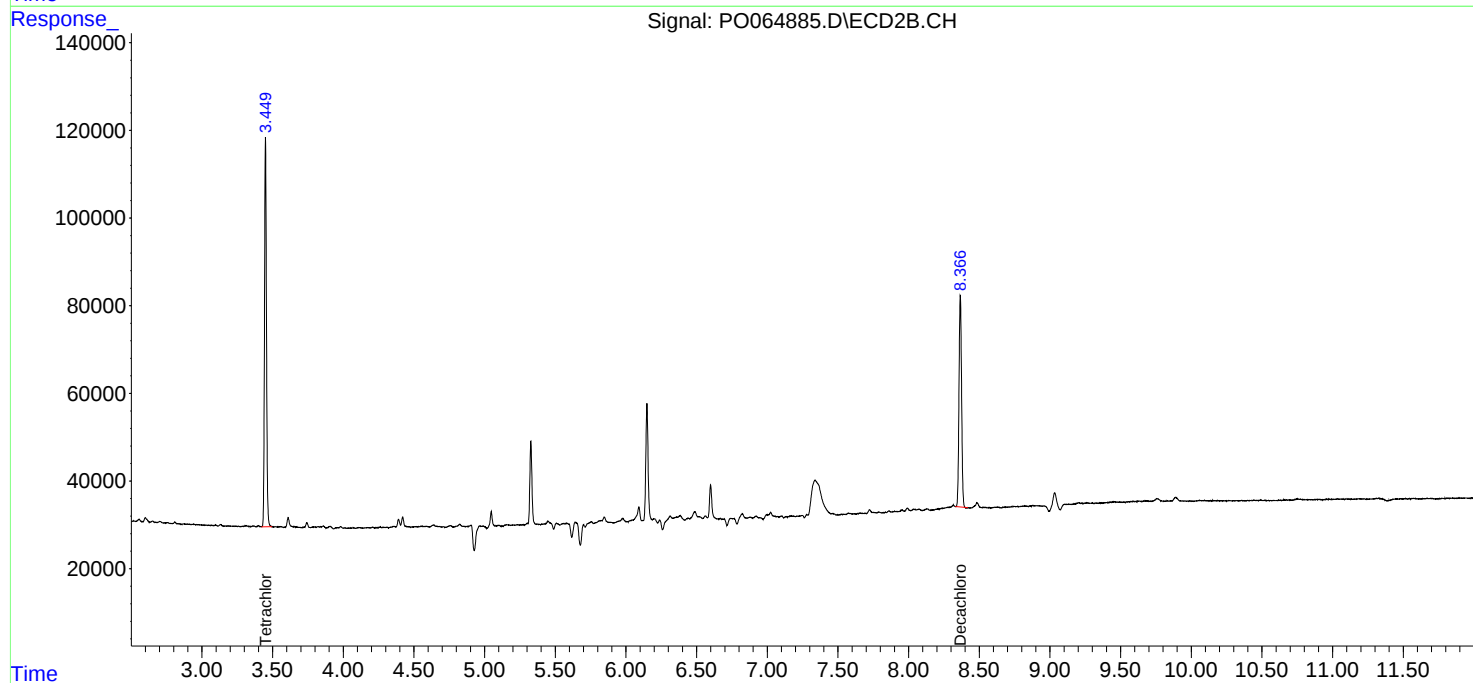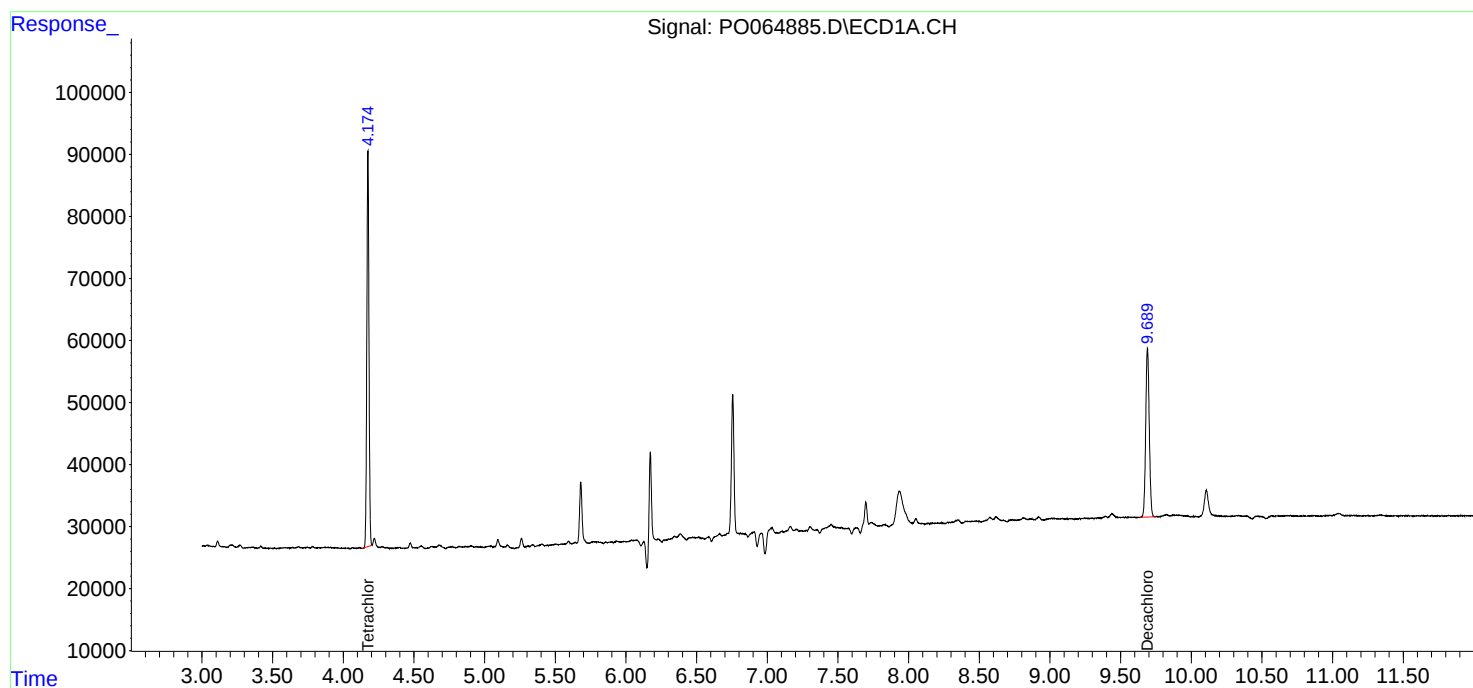

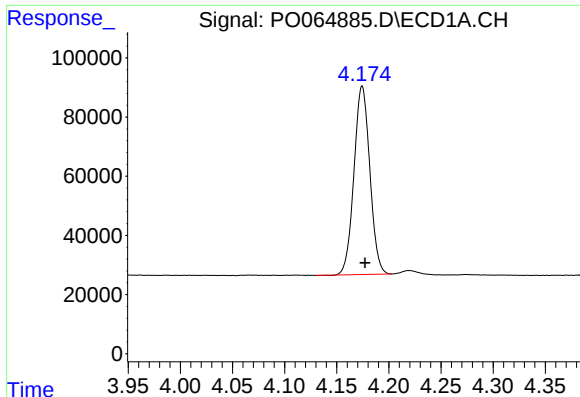


#1 Tetrachloro-m-xylene

R.T.: 4.174 min
Delta R.T.: -0.003 min
Response: 673659
Conc: 27.67 ng/ml

Instrument :
ECD_O
ClientSampleId :
MW-3-20191218


Manual Integrations
APPROVED

Ankita
12/24/2019 2:08:58 PM

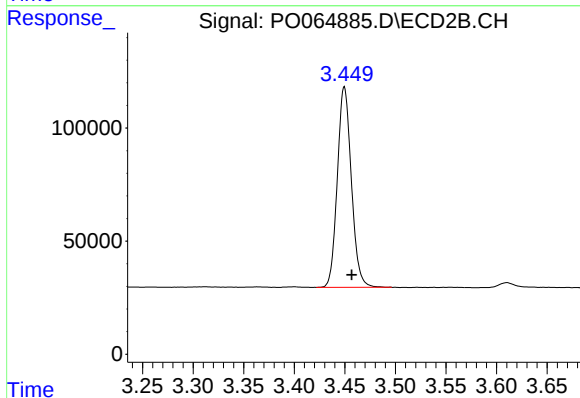


#1 Tetrachloro-m-xylene

R.T.: 3.449 min
Delta R.T.: -0.008 min
Response: 856827
Conc: 33.80 ng/ml m

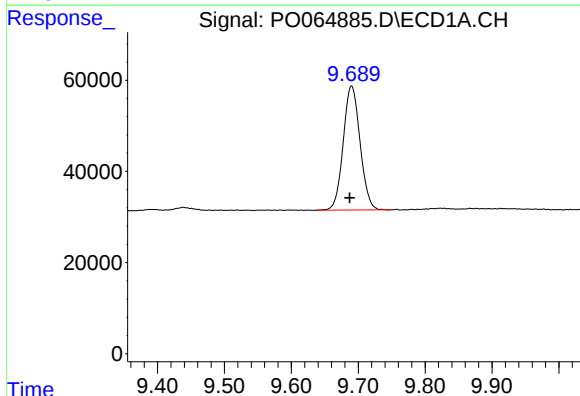

#2 Decachlorobiphenyl

R.T.: 9.690 min
Delta R.T.: 0.002 min
Response: 474925
Conc: 15.47 ng/ml

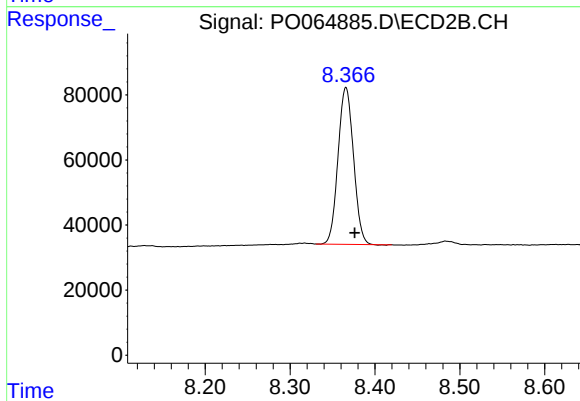

#2 Decachlorobiphenyl

R.T.: 8.366 min
Delta R.T.: -0.010 min
Response: 608955
Conc: 17.53 ng/ml