

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122319\
 Data File : P0064904.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Dec 2019 2:10
 Operator : SM/AJ
 Sample : K6395-02
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 24 07:29:03 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 13 08:19:24 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.174	3.449	723046	951072	29.700	37.519 #
2) SA Decachlor...	9.689	8.365	667615	799749	21.753	23.029

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122319\
Data File : P0064904.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Dec 2019 2:10
Operator : SM/AJ
Sample : K6395-02
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 24 07:29:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 13 08:19:24 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

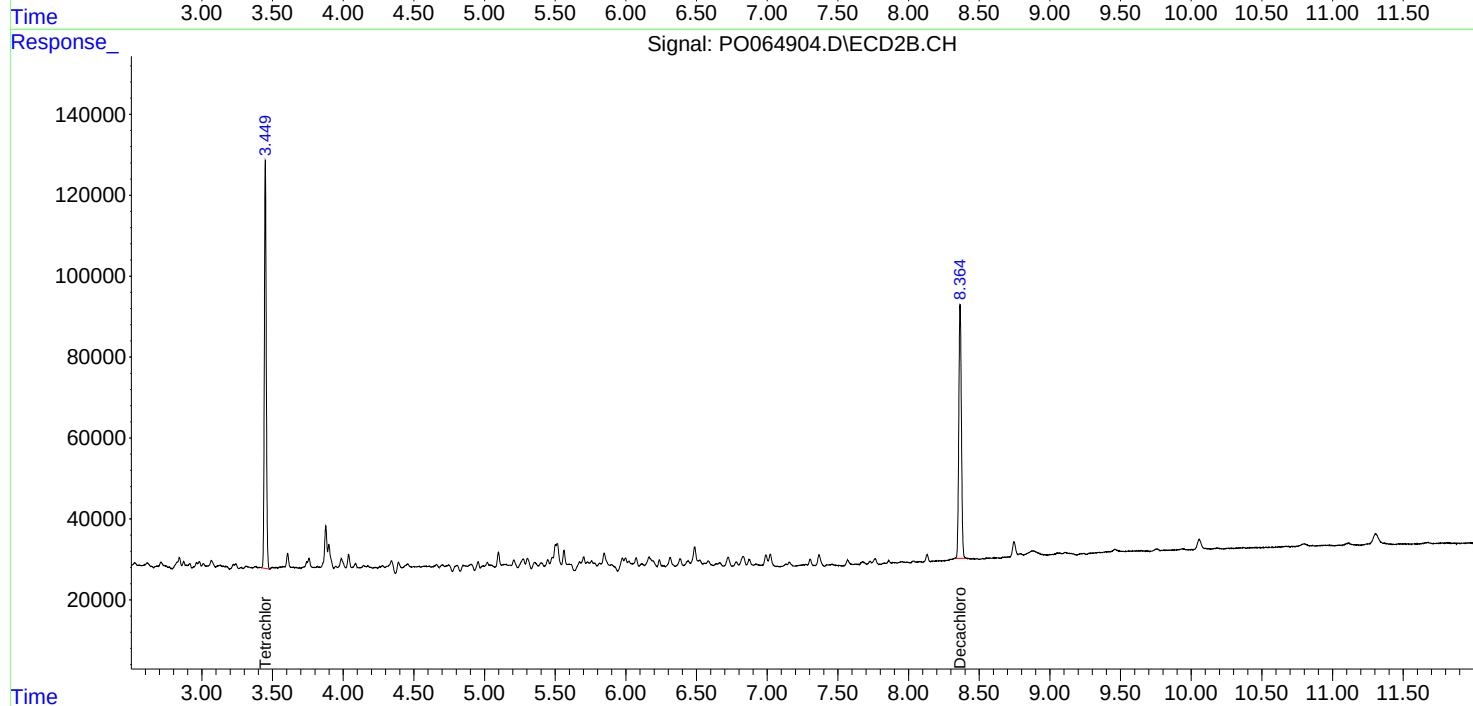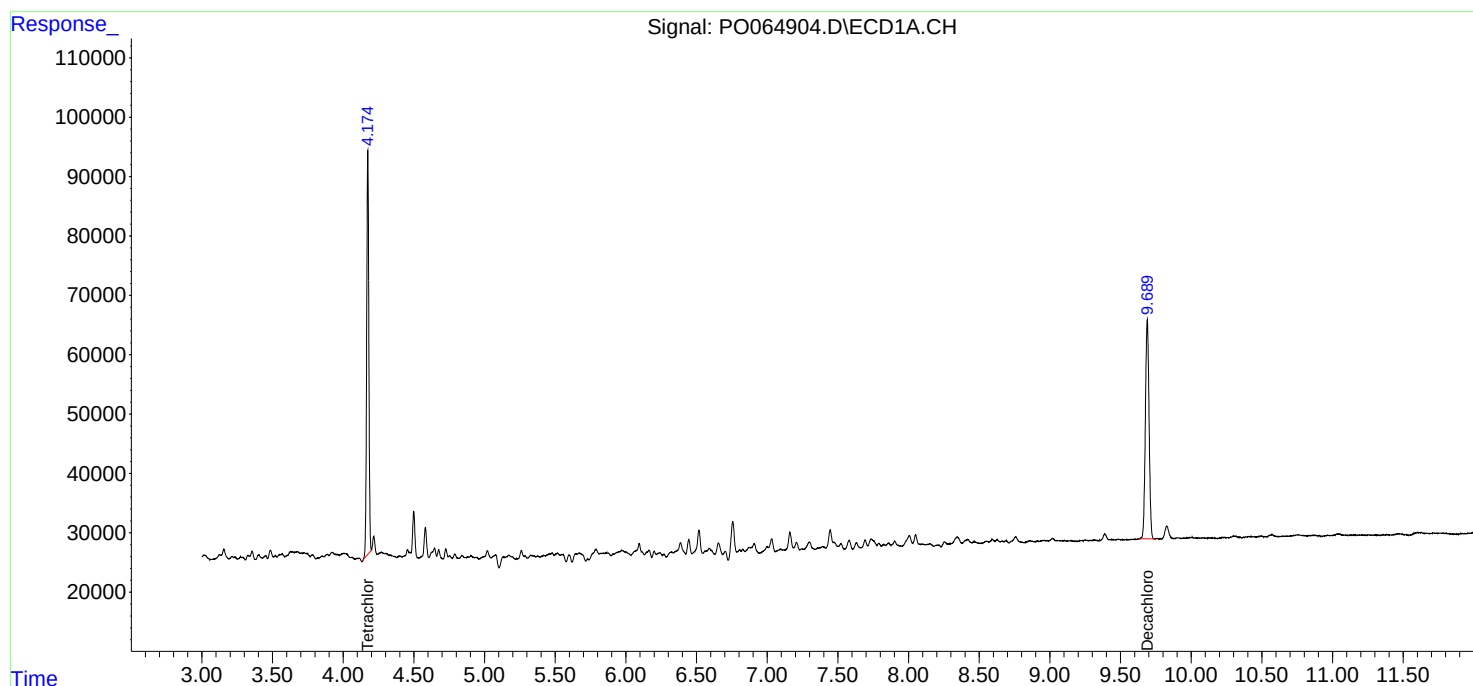


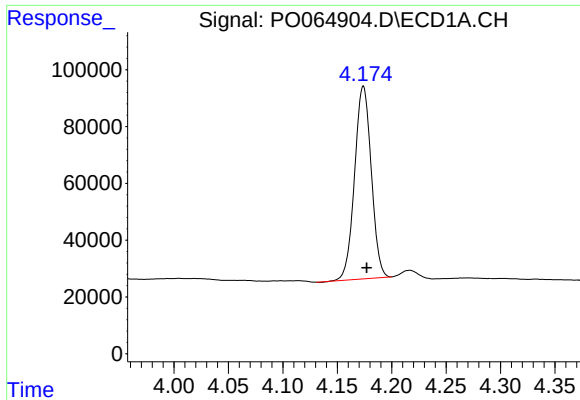

#1 Tetrachloro-m-xylene


R.T.: 4.174 min
Delta R.T.: -0.003 min
Response: 723046
Conc: 29.70 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-3

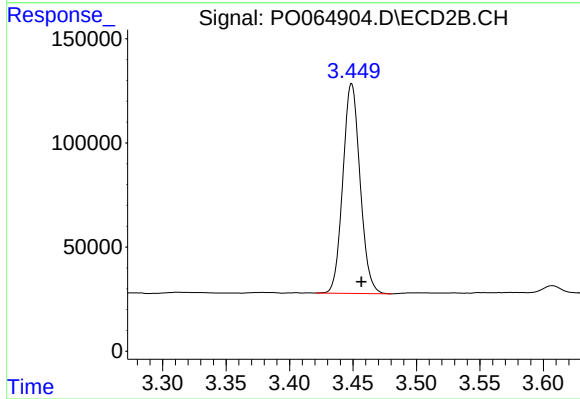


#1 Tetrachloro-m-xylene

R.T.: 3.449 min
Delta R.T.: -0.008 min
Response: 951072
Conc: 37.52 ng/ml

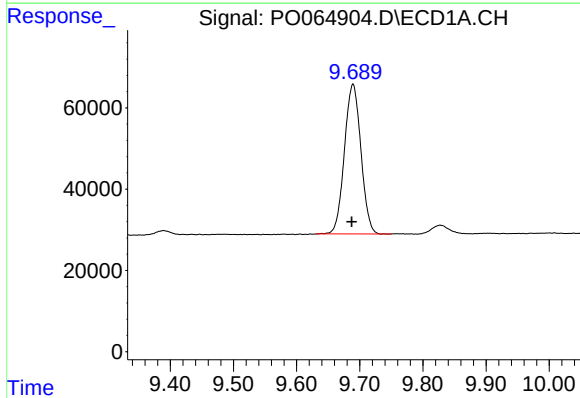

#2 Decachlorobiphenyl

R.T.: 9.689 min
Delta R.T.: 0.002 min
Response: 667615
Conc: 21.75 ng/ml

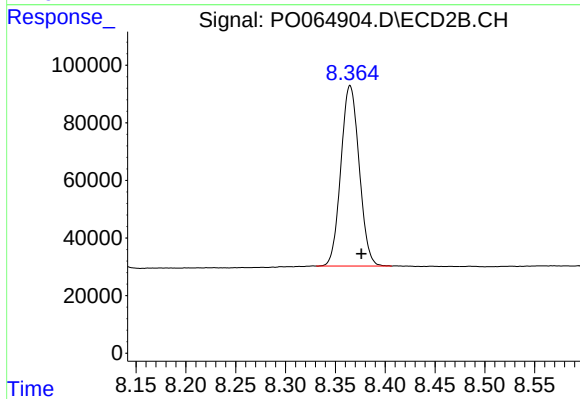

#2 Decachlorobiphenyl

R.T.: 8.365 min
Delta R.T.: -0.011 min
Response: 799749
Conc: 23.03 ng/ml