

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0122319\
Data File : P0064907.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Dec 2019 3:01
Operator : SM/AJ
Sample : K6400-01
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
115-MAIDEN-LANE-BERGENFIELD

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 24 07:36:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0121319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 13 08:19:24 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.175	3.450	762078	949504	31.303	37.457
2) SA Decachlor...	9.692	8.366	600826	707194	19.577	20.364

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122319\
Data File : PO064907.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Dec 2019 3:01
Operator : SM/AJ
Sample : K6400-01
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
115-MAIDEN-LANE-BERGENFIELD

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 24 07:36:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 13 08:19:24 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

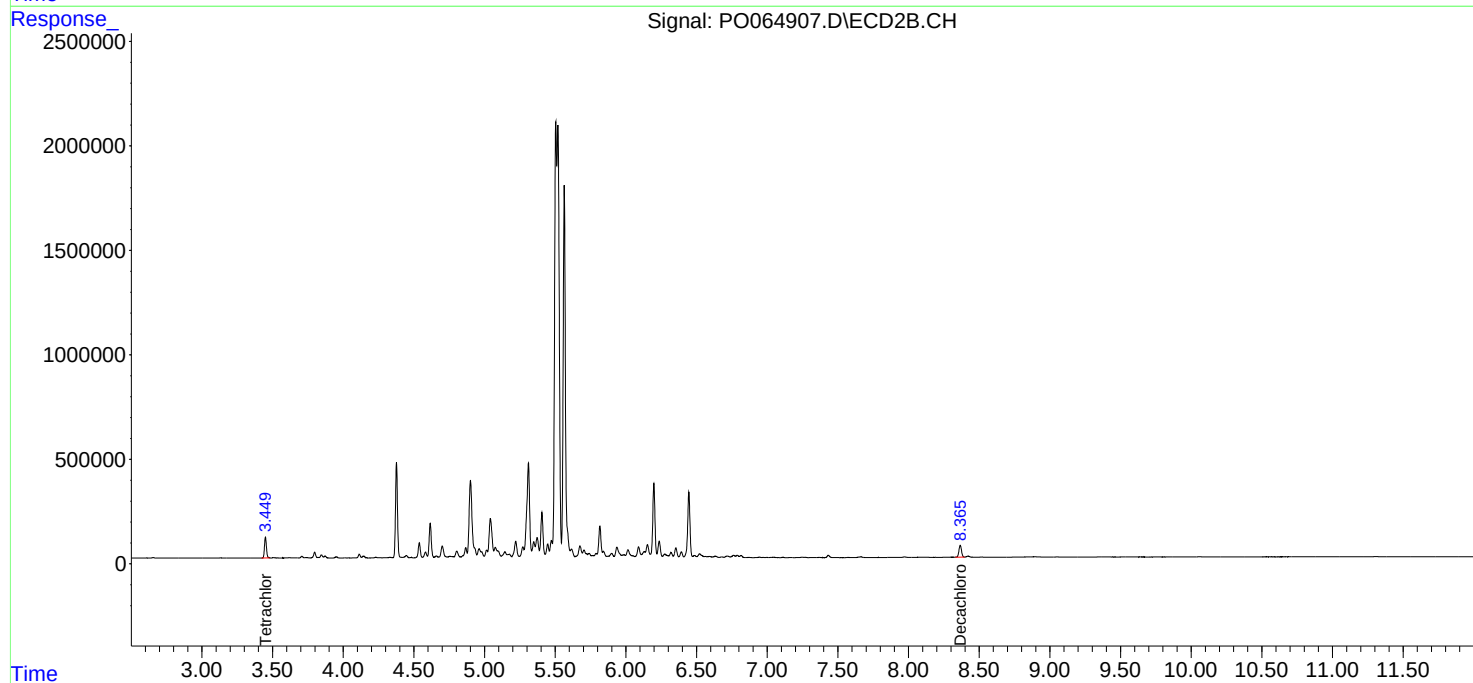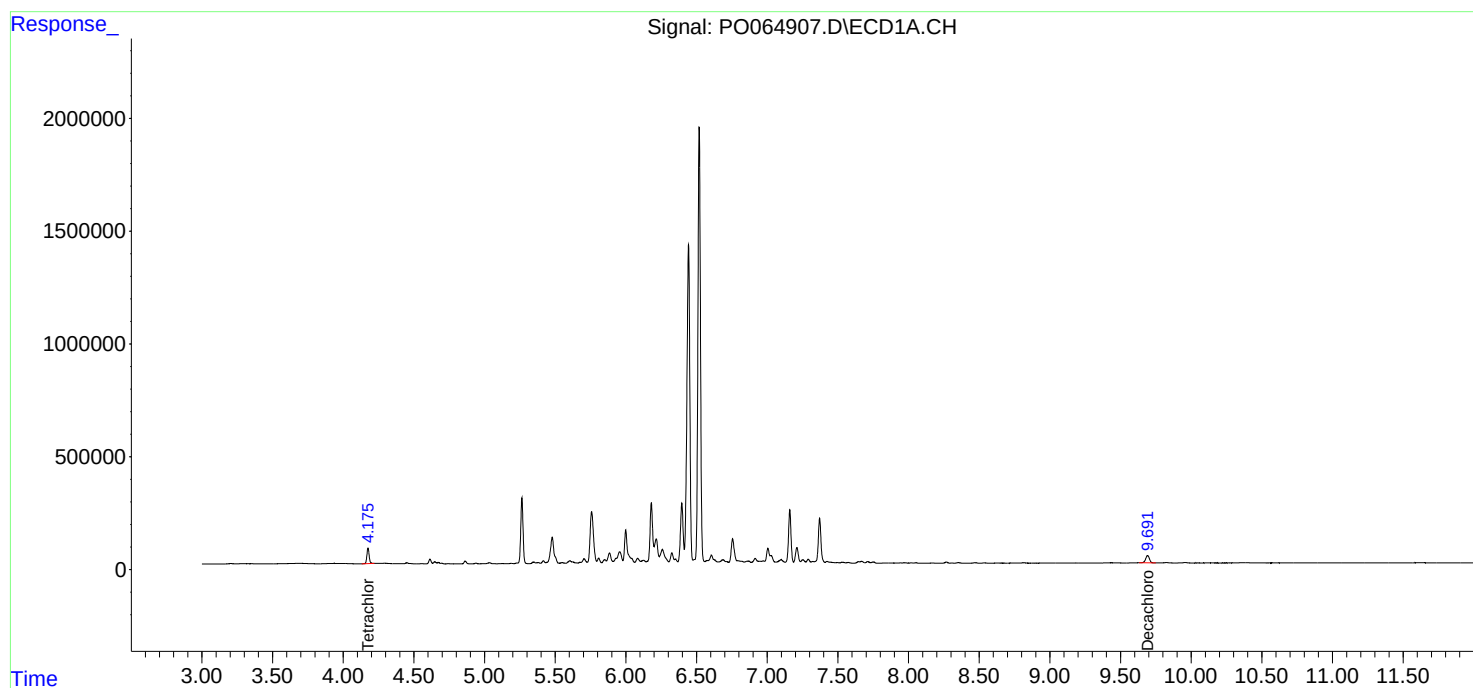


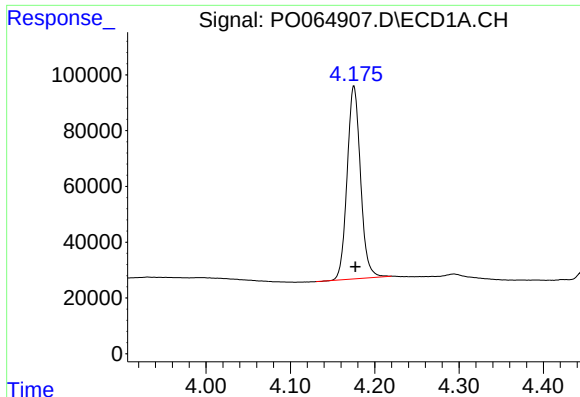

#1 Tetrachloro-m-xylene


R.T.: 4.175 min
Delta R.T.: -0.002 min
Response: 762078
Conc: 31.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
115-MAIDEN-LANE-BERGENFIELD

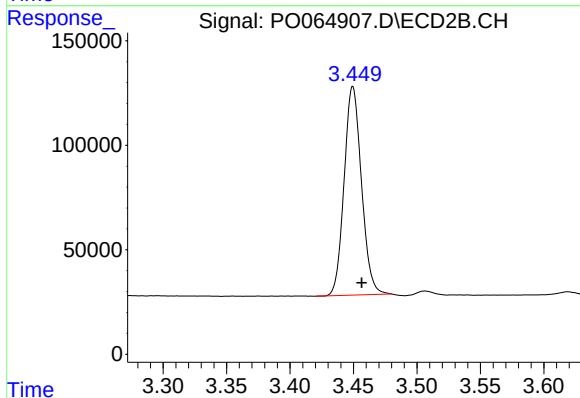


#1 Tetrachloro-m-xylene

R.T.: 3.450 min
Delta R.T.: -0.007 min
Response: 949504
Conc: 37.46 ng/ml

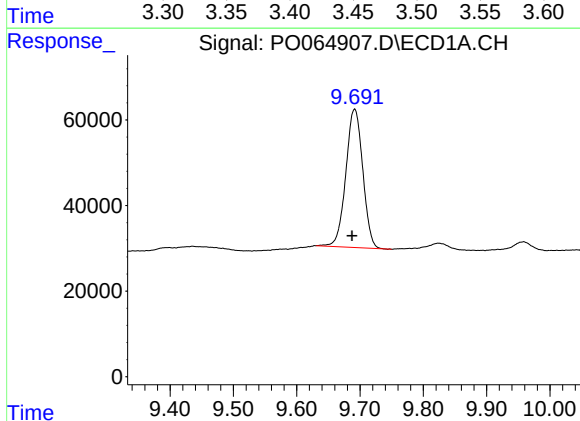

#2 Decachlorobiphenyl

R.T.: 9.692 min
Delta R.T.: 0.004 min
Response: 600826
Conc: 19.58 ng/ml

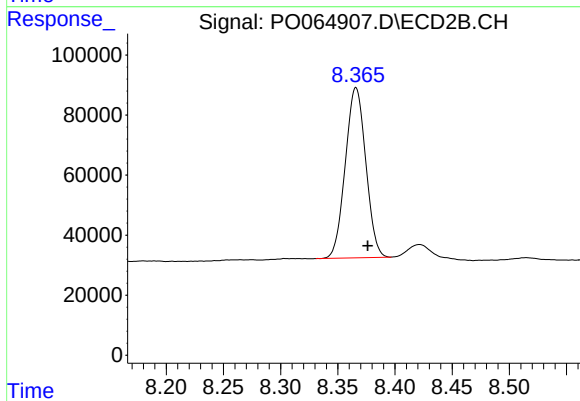

#2 Decachlorobiphenyl

R.T.: 8.366 min
Delta R.T.: -0.010 min
Response: 707194
Conc: 20.36 ng/ml