

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0122320\
 Data File : P0074155.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Dec 2020 7:58
 Operator : DD\AJ
 Sample : L5192-01
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CL-02-122220

Manual Integrations
 APPROVED

Ankita
 12/24/2020 12:59:33 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 24 11:28:31 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0122320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Dec 24 01:16:32 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.933	3.991	2503085	1438848	24.549m	25.080
2) SA Decachlor...	10.953	9.251	1943761	1032200	19.959	19.200

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122320\
Data File : PO074155.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Dec 2020 7:58
Operator : DD\AJ
Sample : L5192-01
Misc :
ALS Vial : 45 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
CL-02-122220


Manual Integrations
APPROVED

Ankita
12/24/2020 12:59:33 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 24 11:28:31 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO122320.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Dec 24 01:16:32 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

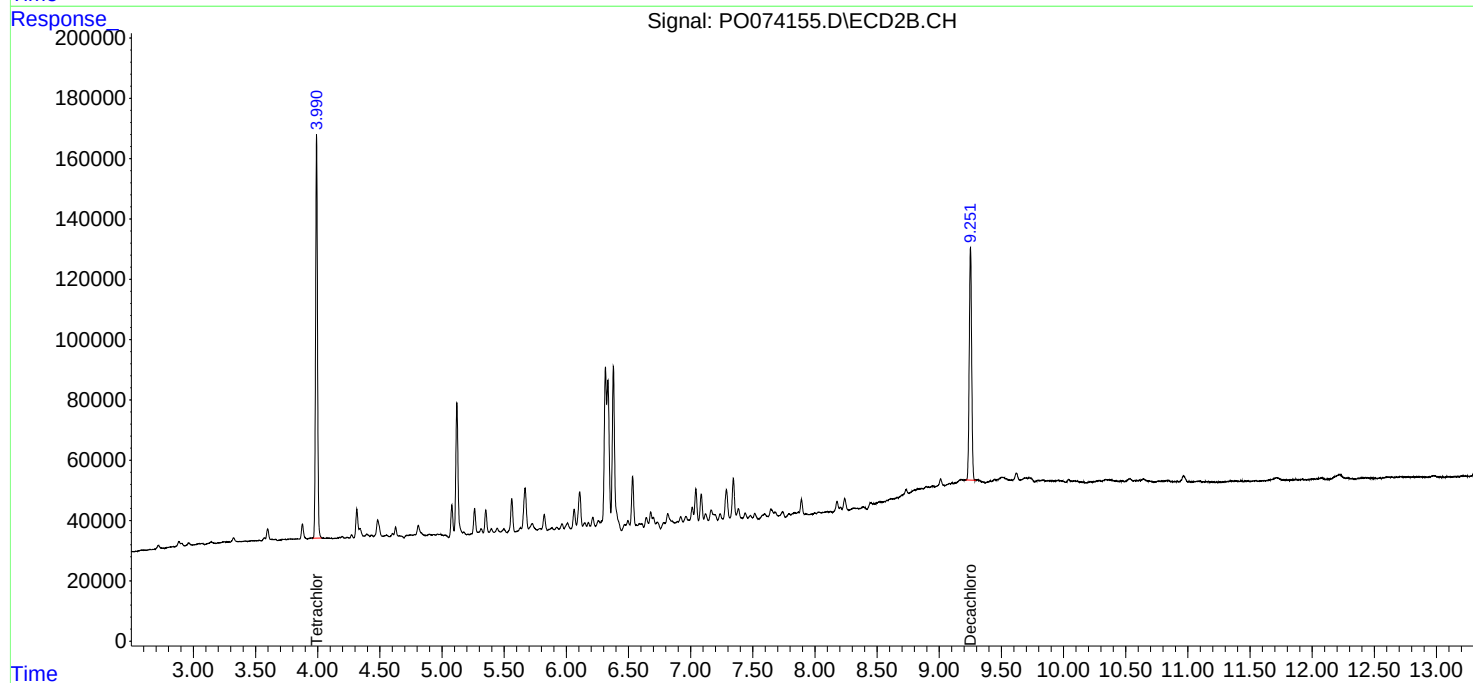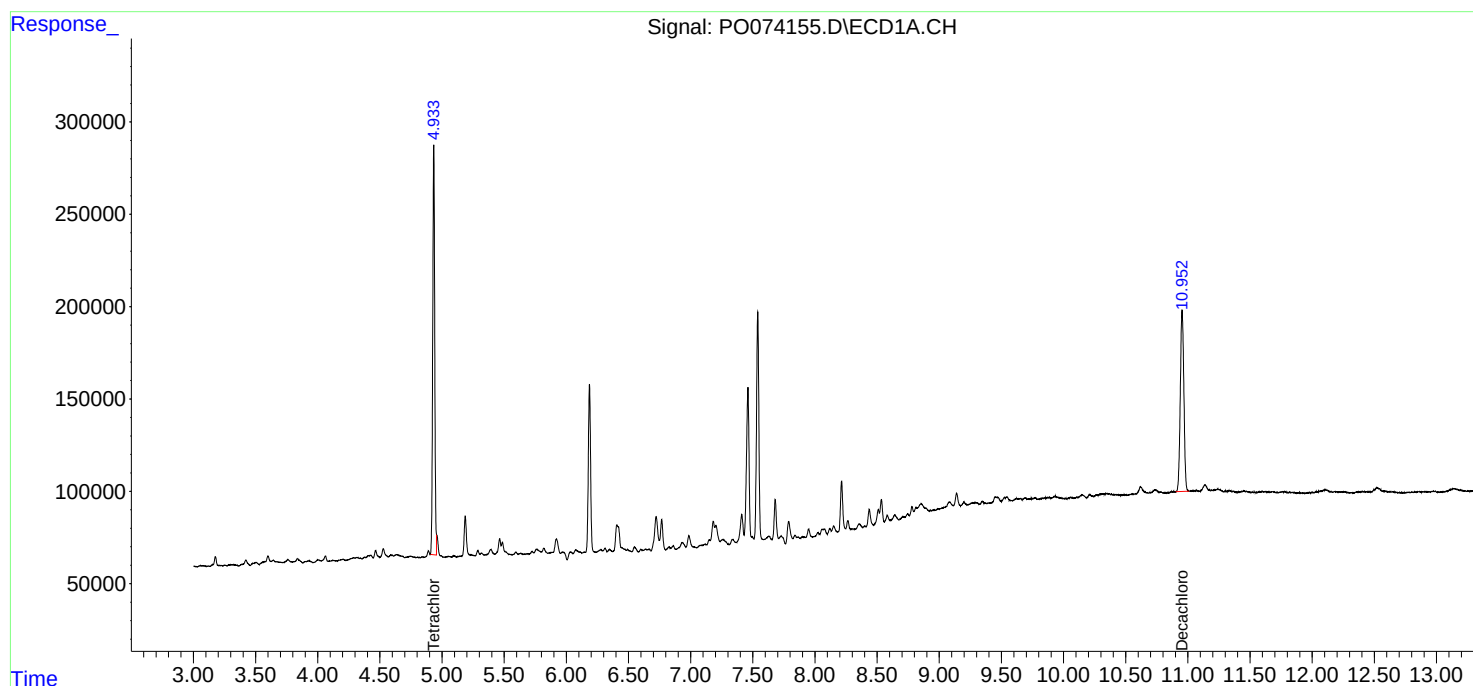

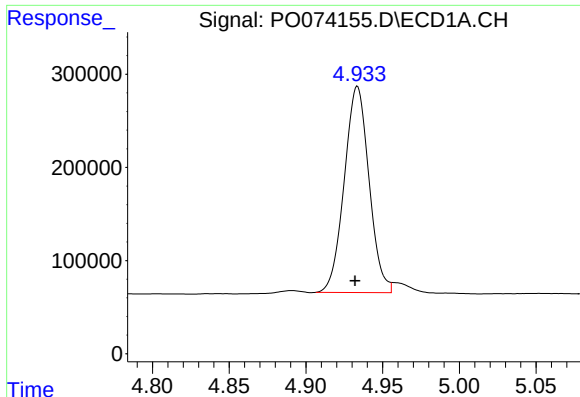


#1 Tetrachloro-m-xylene

R.T.: 4.933 min
Delta R.T.: 0.001 min
Response: 2503085
Conc: 24.55 ng/ml m

Instrument :
ECD_O
ClientSampleId :
CL-02-122220


Manual Integrations
APPROVED

Ankita
12/24/2020 12:59:33 PM

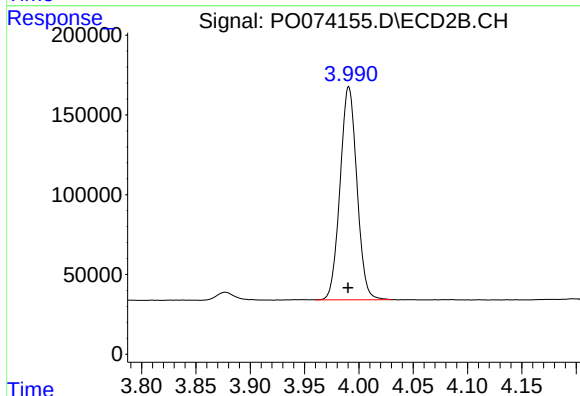


#1 Tetrachloro-m-xylene

R.T.: 3.991 min
Delta R.T.: 0.000 min
Response: 1438848
Conc: 25.08 ng/ml

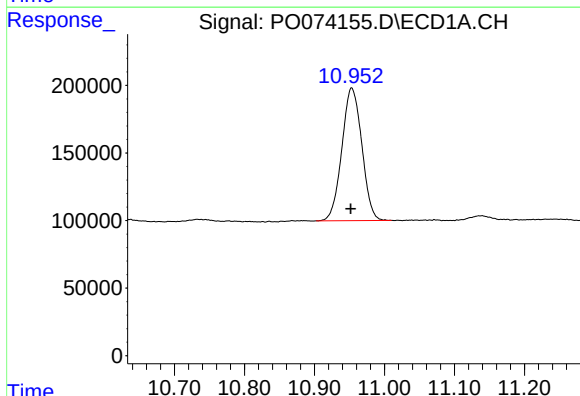

#2 Decachlorobiphenyl

R.T.: 10.953 min
Delta R.T.: 0.001 min
Response: 1943761
Conc: 19.96 ng/ml

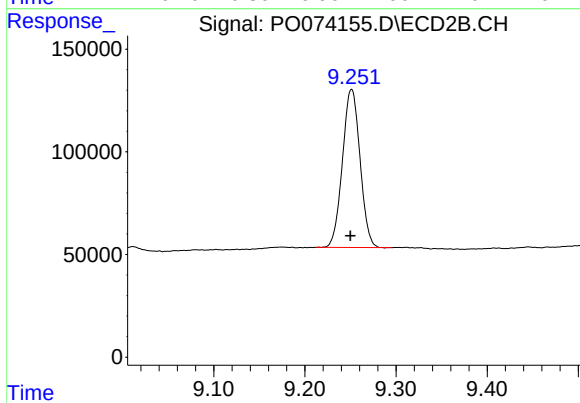

#2 Decachlorobiphenyl

R.T.: 9.251 min
Delta R.T.: 0.001 min
Response: 1032200
Conc: 19.20 ng/ml