

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0122322\
 Data File : P0091607.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Dec 2022 13:19
 Operator : YP/AJ
 Sample : N6162-02 10X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BC260597LOZ-1-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/27/2022
 Supervised By :Ankita Jodhani 12/27/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 27 00:50:29 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0122122.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Dec 22 03:53:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.294	3.471	4432640	1850842	1.632	1.825
2) SA Decachlor...	10.052	8.479	3889788	1671466	2.067m	1.916

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122322\
Data File : P0091607.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Dec 2022 13:19
Operator : YP/AJ
Sample : N6162-02 10X
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
BC260597LOZ-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/27/2022
Supervised By :Ankita Jodhani 12/27/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 27 00:50:29 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO122122.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Dec 22 03:53:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

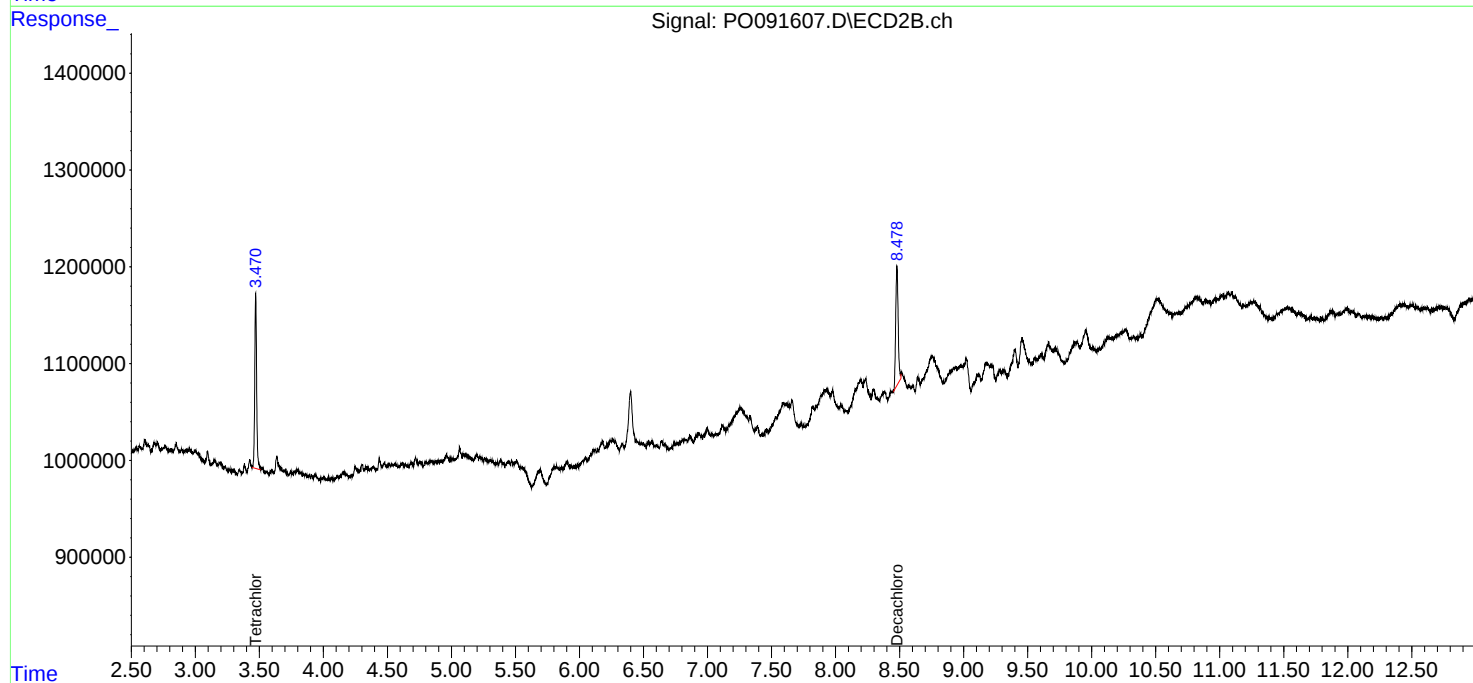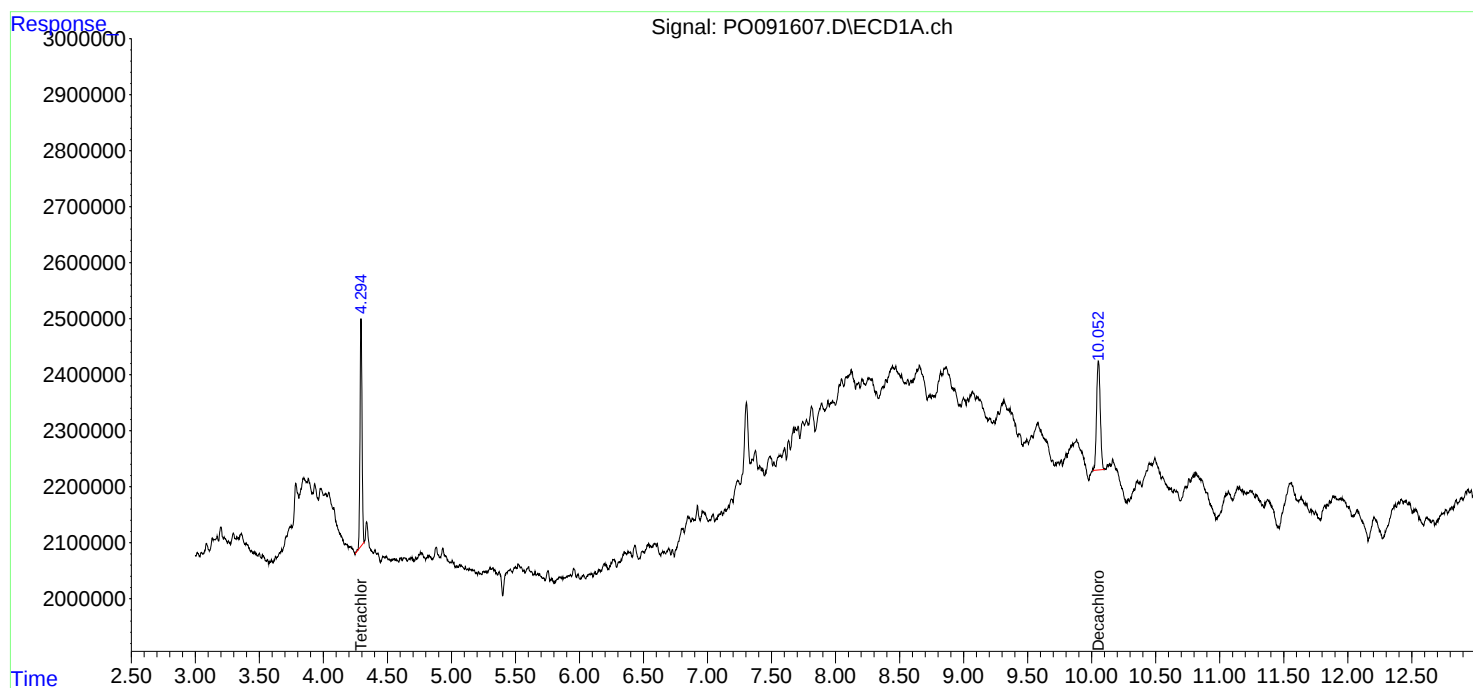

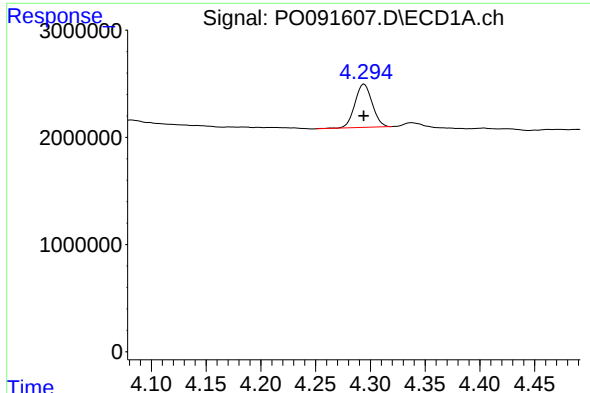


#1 Tetrachloro-m-xylene

R.T.: 4.294 min
Delta R.T.: 0.000 min
Response: 4432640
Conc: 1.63 ng/ml

Instrument :
ECD_O
ClientSampleId :
BC260597LOZ-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/27/2022
Supervised By :Ankita Jodhani 12/27/2022

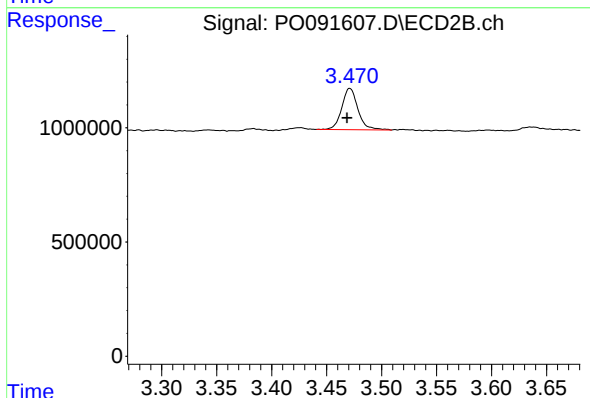


#1 Tetrachloro-m-xylene

R.T.: 3.471 min
Delta R.T.: 0.002 min
Response: 1850842
Conc: 1.83 ng/ml

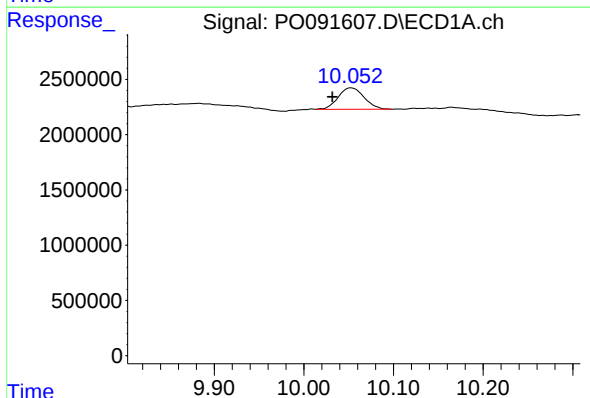

#2 Decachlorobiphenyl

R.T.: 10.052 min
Delta R.T.: 0.020 min
Response: 3889788
Conc: 2.07 ng/ml m

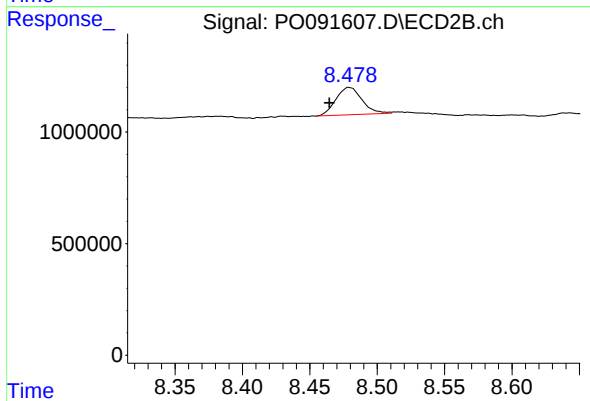

#2 Decachlorobiphenyl

R.T.: 8.479 min
Delta R.T.: 0.014 min
Response: 1671466
Conc: 1.92 ng/ml