

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0122324\
 Data File : P0108746.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Dec 2024 12:04
 Operator : YP/AJ
 Sample : P5357-03RE
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 121824-CRE

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/26/2024
 Supervised By :Ankita Jodhani 12/27/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 23 12:35:05 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0120624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 07 05:58:15 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.702	3.700	15426583	7761941	1.773m	1.531
2) SA Decachlor...	8.765	8.715	1701273	1288065	0.233m	0.332m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122324\
Data File : PO108746.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Dec 2024 12:04
Operator : YP/AJ
Sample : P5357-03RE
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
121824-CRE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/26/2024
Supervised By :Ankita Jodhani 12/27/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 23 12:35:05 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 07 05:58:15 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

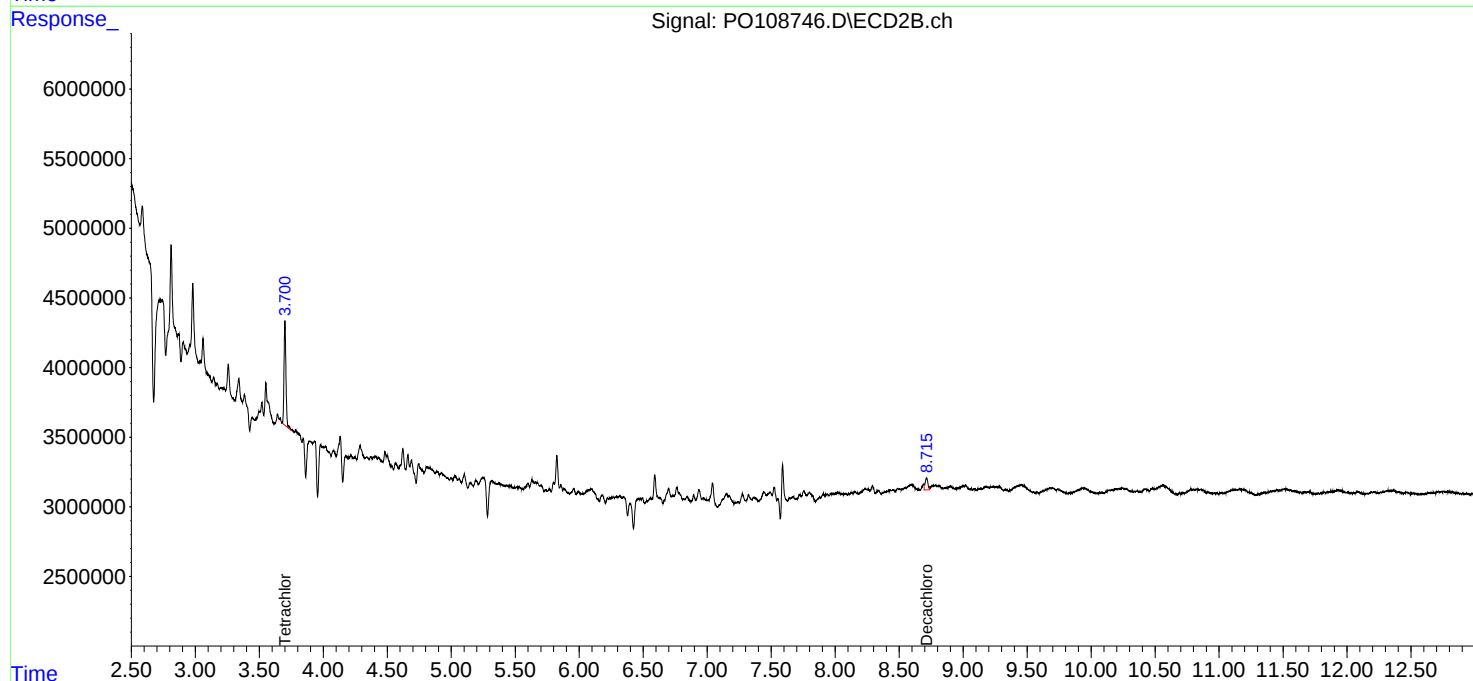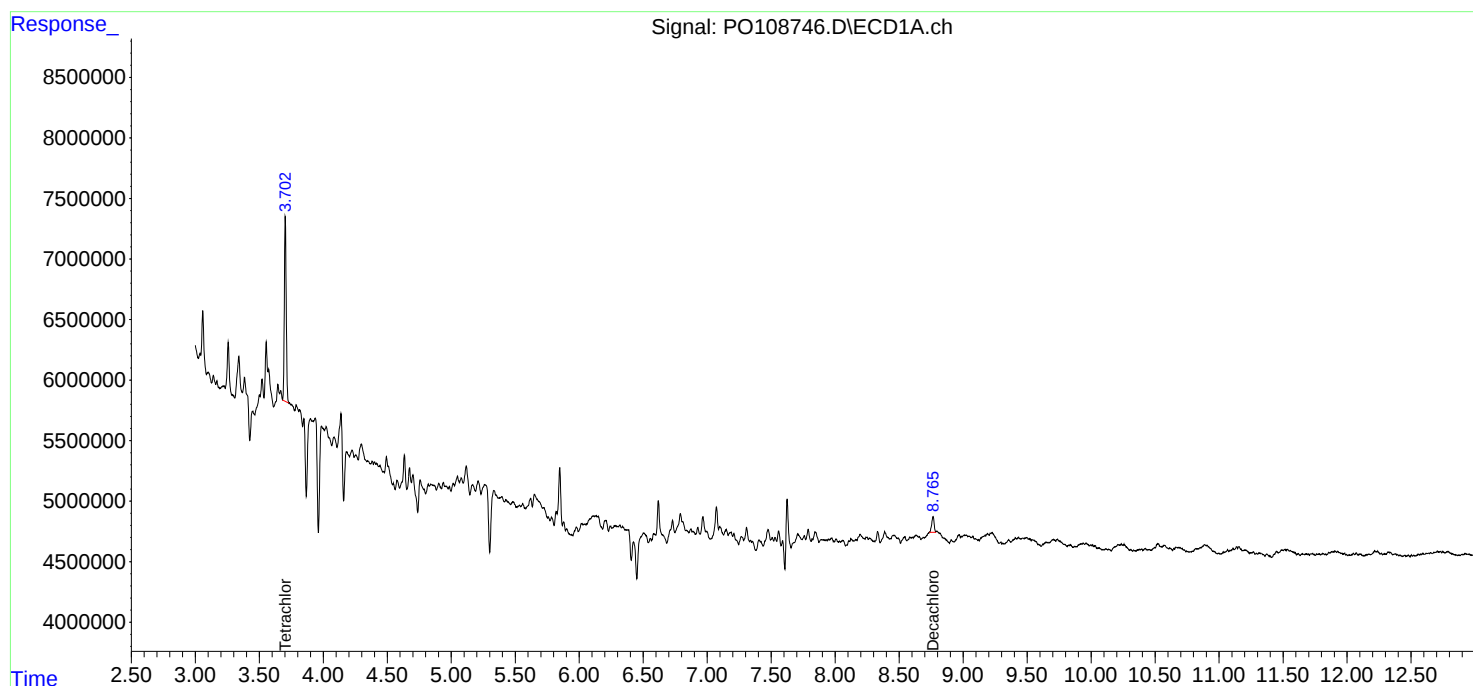

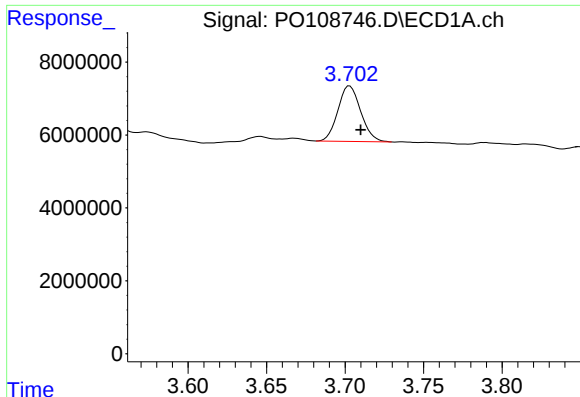


#1 Tetrachloro-m-xylene

R.T.: 3.702 min
Delta R.T.: -0.008 min
Response: 15426583
Conc: 1.77 ng/ml

Instrument :
ECD_O
ClientSampleId :
121824-CRE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/26/2024
Supervised By :Ankita Jodhani 12/27/2024

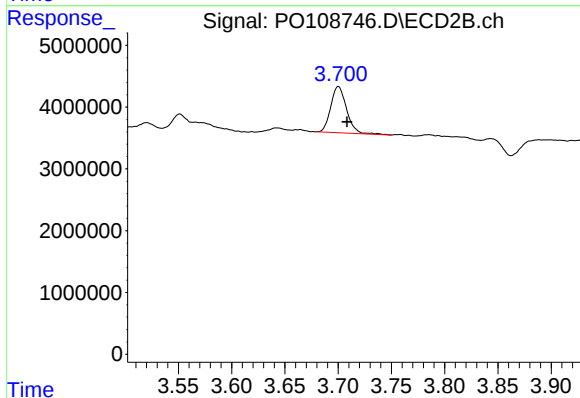


#1 Tetrachloro-m-xylene

R.T.: 3.700 min
Delta R.T.: -0.008 min
Response: 7761941
Conc: 1.53 ng/ml

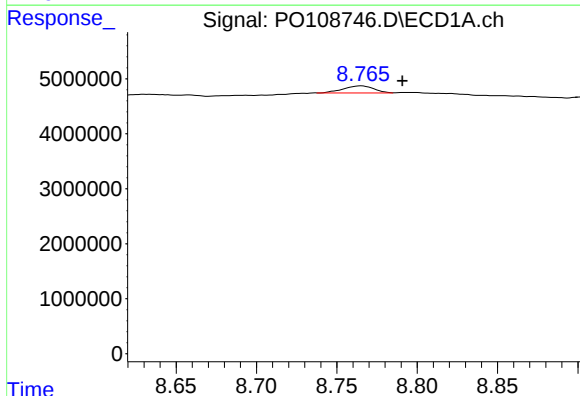

#2 Decachlorobiphenyl

R.T.: 8.765 min
Delta R.T.: -0.026 min
Response: 1701273
Conc: 0.23 ng/ml m

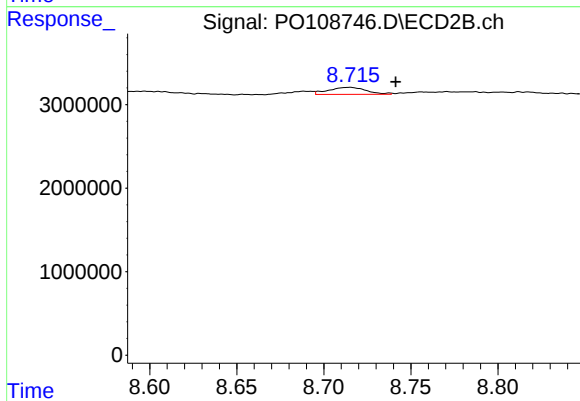

#2 Decachlorobiphenyl

R.T.: 8.715 min
Delta R.T.: -0.026 min
Response: 1288065
Conc: 0.33 ng/ml m