

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0122420\
 Data File : P0074209.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Dec 2020 00:47
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 25 04:19:32 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0122320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Dec 24 01:16:32 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.937	3.993	2446788	1399042	23.997	24.386
2)	SA Decachlor...	10.965	9.257	2103240	1222522	21.597	22.740
Target Compounds							
20)	L4 AR-1242-5	0.000	6.132f	0	267674	N.D.	170.107 #
24)	L5 AR-1248-4	7.182f	0.000	616901	0	153.715	N.D. #
25)	L5 AR-1248-5	0.000	6.132	0	267674	N.D.	116.452 #
26)	L6 AR-1254-1	7.182	6.132f	616901	267674	159.803	77.391 #
28)	L6 AR-1254-3	7.809f	0.000	126417	0	21.043	N.D. #
32)	L7 AR-1260-2	0.000	6.983f	0	46524	N.D.	9.853 #
33)	L7 AR-1260-3	0.000	7.165	0	61759	N.D.	15.762 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122420\
Data File : PO074209.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Dec 2020 00:47
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 25 04:19:32 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO122320.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Dec 24 01:16:32 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

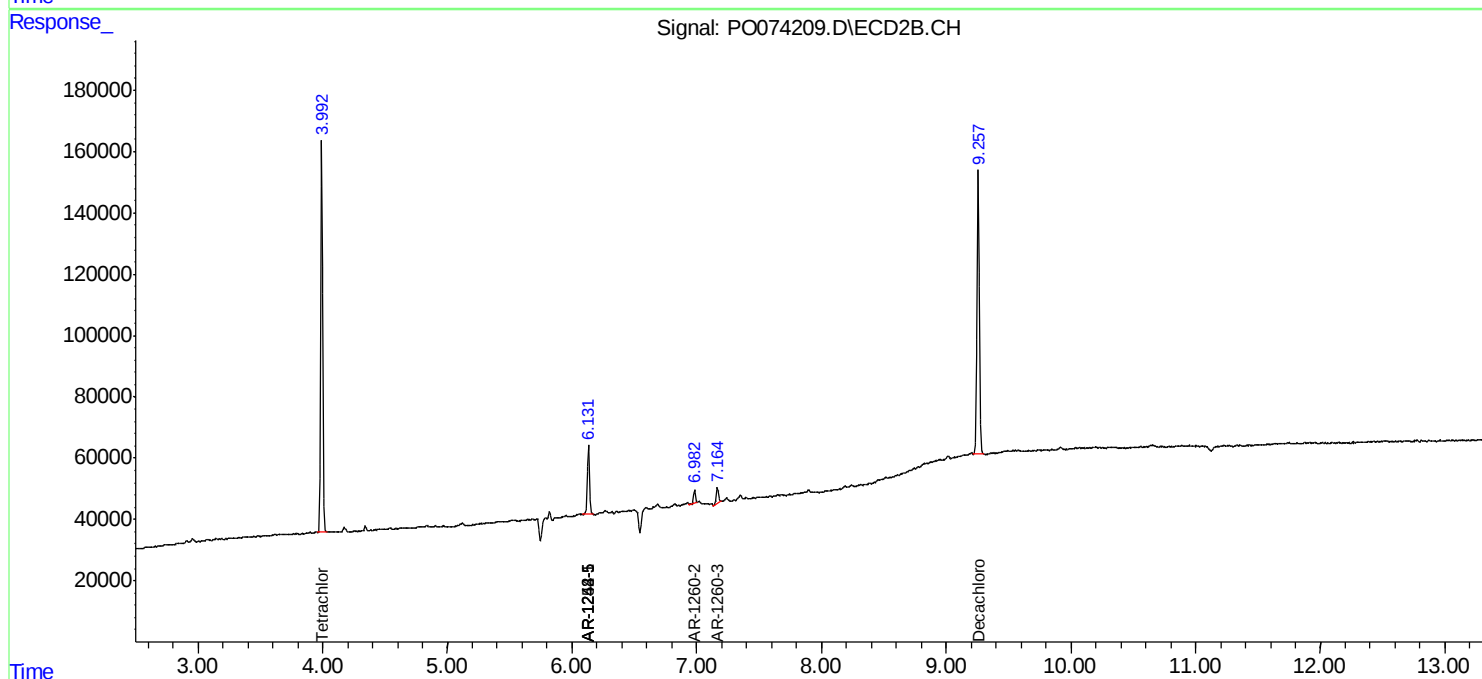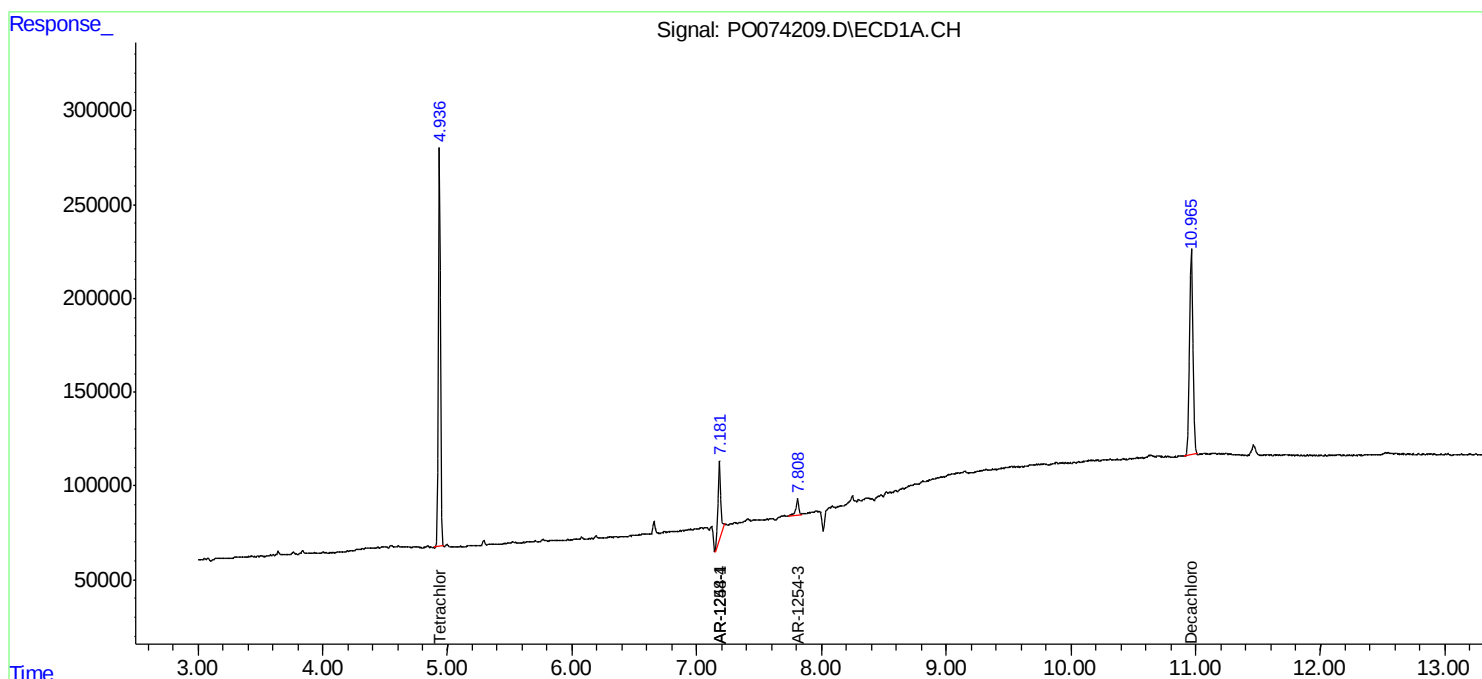


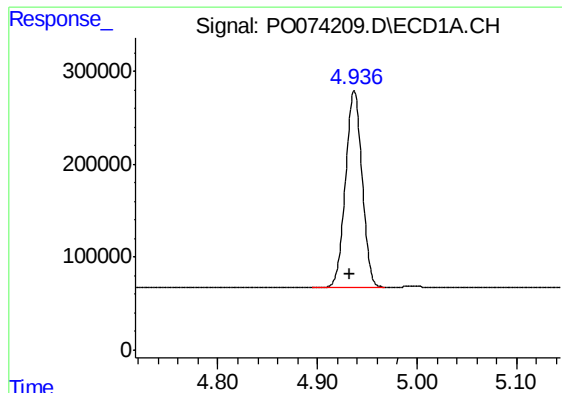

#1 Tetrachloro-m-xylene


R.T.: 4.937 min
Delta R.T.: 0.005 min
Response: 2446788
Conc: 24.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

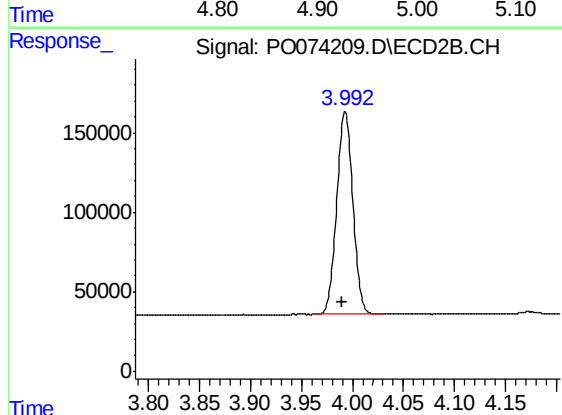


#1 Tetrachloro-m-xylene

R.T.: 3.993 min
Delta R.T.: 0.003 min
Response: 1399042
Conc: 24.39 ng/ml

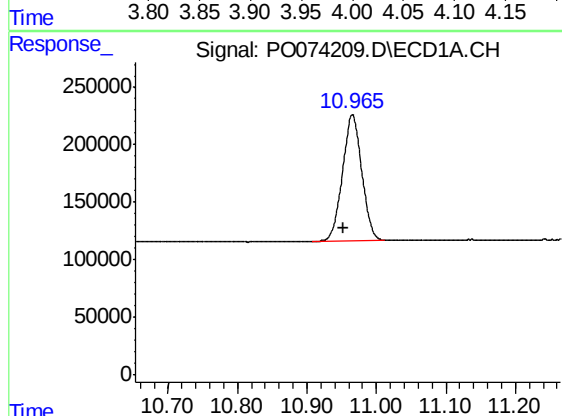


#2 Decachlorobiphenyl

R.T.: 10.965 min
Delta R.T.: 0.014 min
Response: 2103240
Conc: 21.60 ng/ml

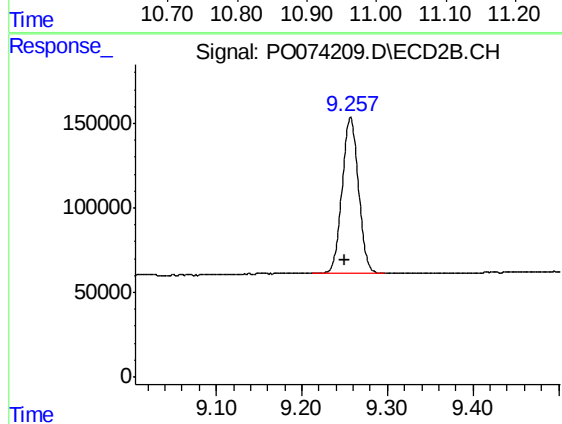

#2 Decachlorobiphenyl


R.T.: 9.257 min
Delta R.T.: 0.007 min
Response: 1222522
Conc: 22.74 ng/ml

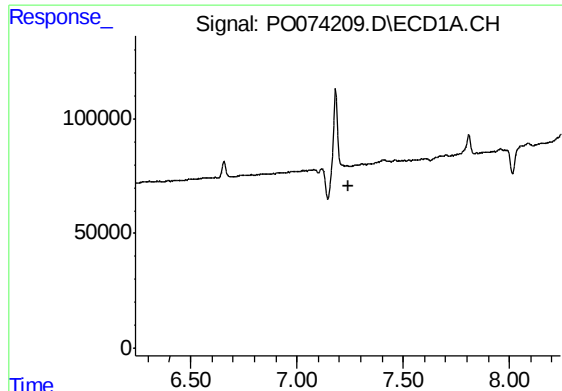

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T. : 7.240 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

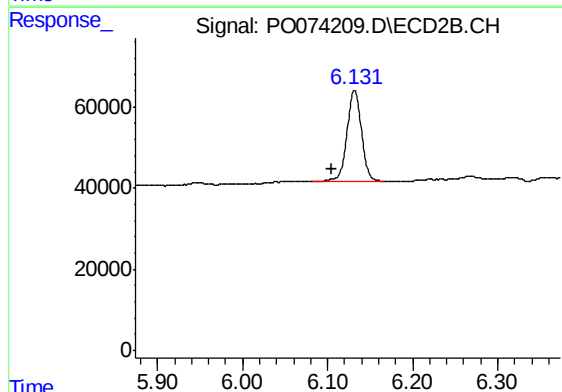


#20 AR-1242-5

R.T.: 6.132 min
Delta R.T.: 0.027 min
Response: 267674
Conc: 170.11 ng/ml

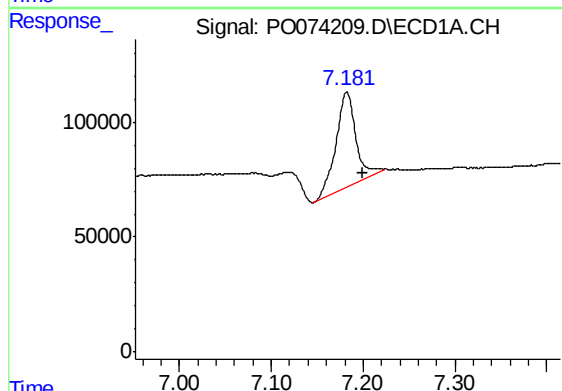


#24 AR-1248-4

R.T.: 7.182 min
Delta R.T.: -0.017 min
Response: 616901
Conc: 153.71 ng/ml

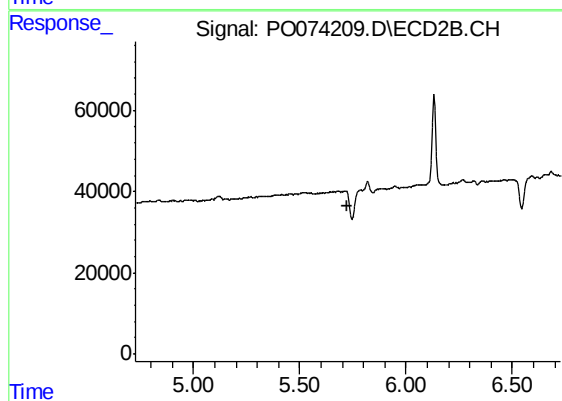

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T. : 5.727 min
Response: 0
Conc: N.D.

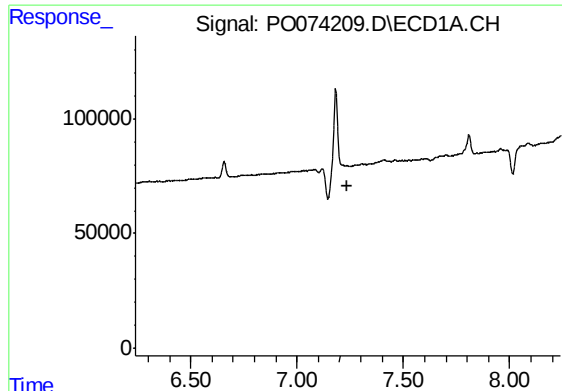

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T.: 7.239 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

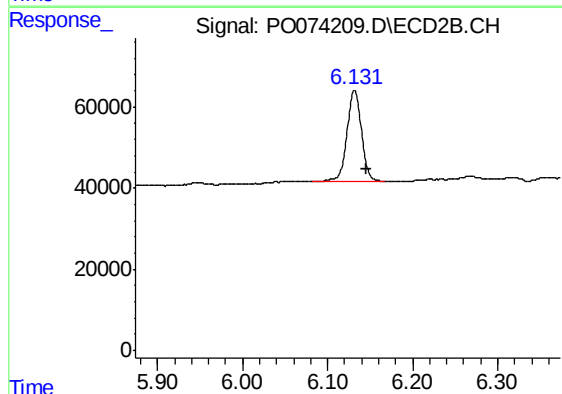


#25 AR-1248-5

R.T.: 6.132 min
Delta R.T.: -0.015 min
Response: 267674
Conc: 116.45 ng/ml

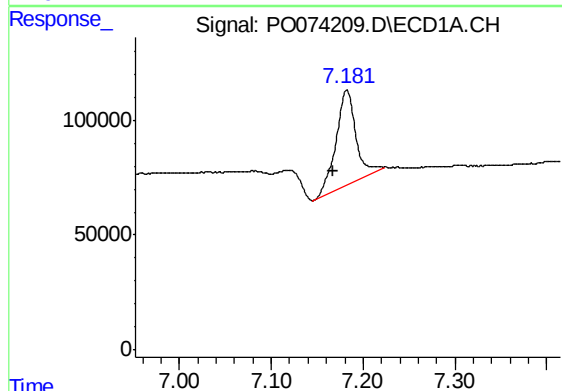


#26 AR-1254-1

R.T.: 7.182 min
Delta R.T.: 0.014 min
Response: 616901
Conc: 159.80 ng/ml

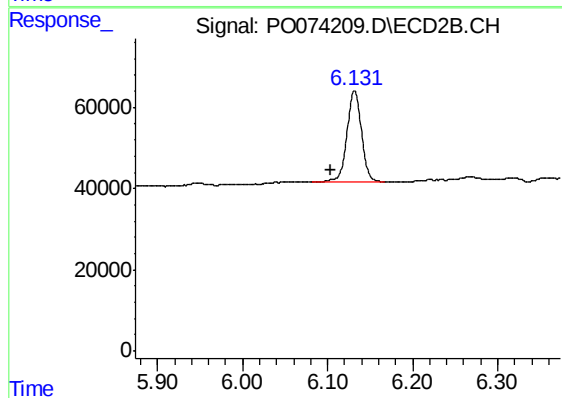

#26 AR-1254-1


R.T.: 6.132 min
Delta R.T.: 0.028 min
Response: 267674
Conc: 77.39 ng/ml

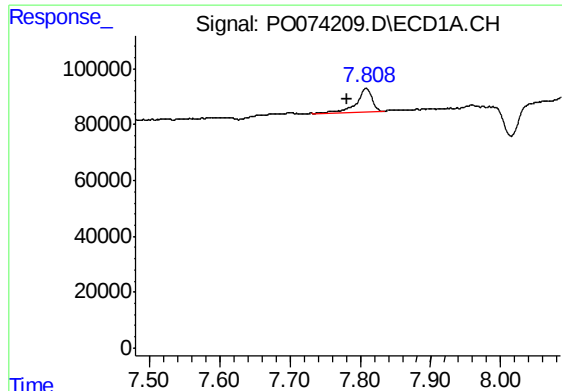

#28 AR-1254-3


R.T.: 7.809 min
Delta R.T.: 0.027 min
Response: 126417
Conc: 21.04 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

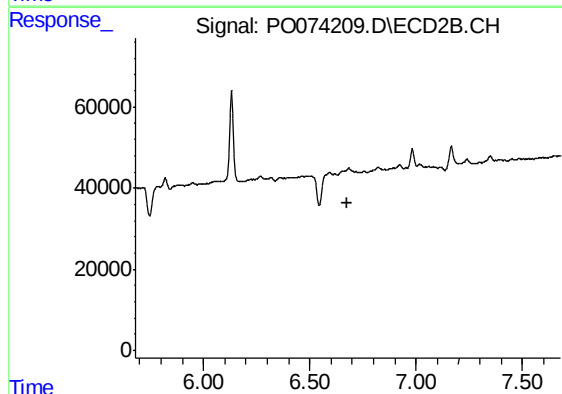


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.679 min
Response: 0
Conc: N.D.

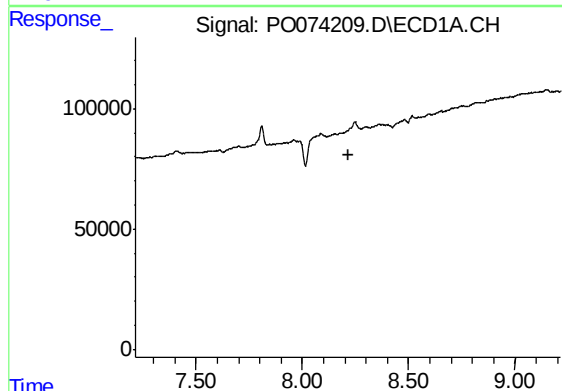


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 8.214 min
Response: 0
Conc: N.D.

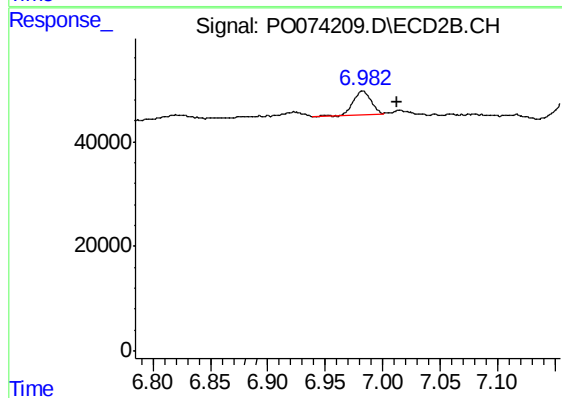

#32 AR-1260-2


R.T.: 6.983 min
Delta R.T.: -0.030 min
Response: 46524
Conc: 9.85 ng/ml

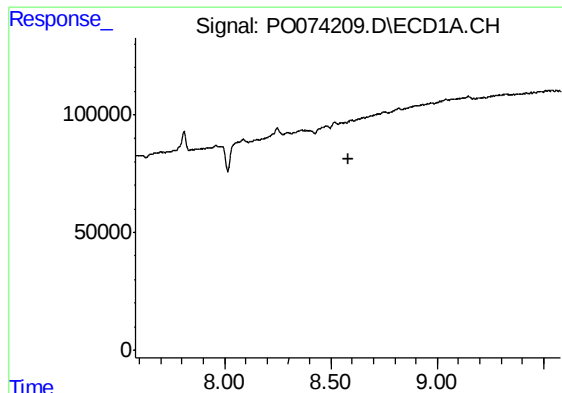

#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 8.580 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

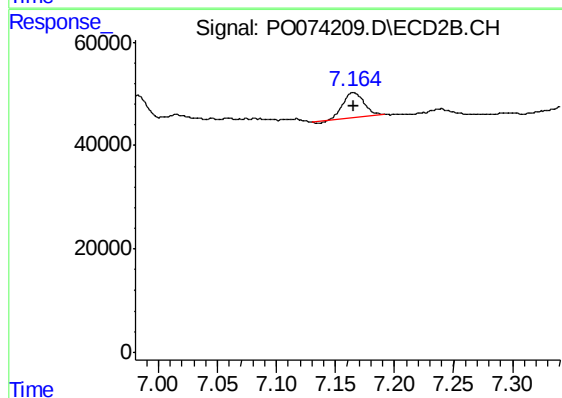

#33 AR-1260-3

R.T.: 7.165 min
Delta R.T.: 0.000 min
Response: 61759
Conc: 15.76 ng/ml