

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122623\
 Data File : PO100749.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Dec 2023 17:29
 Operator : YP/AJ
 Sample : 06010-04 10X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 KMH233N-F

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/27/2023
 Supervised By :Ankita Jodhani 12/28/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 27 00:41:41 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO122023.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Dec 21 04:28:19 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.348	3.645	3573048	2970610	1.145	1.454m#
2) SA Decachlor...	10.090	8.704	2411577	2248728	1.154m	1.490 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122623\
Data File : PO100749.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Dec 2023 17:29
Operator : YP/AJ
Sample : 06010-04 10X
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
KMH233N-F


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/27/2023
Supervised By :Ankita Jodhani 12/28/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 27 00:41:41 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO122023.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Dec 21 04:28:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

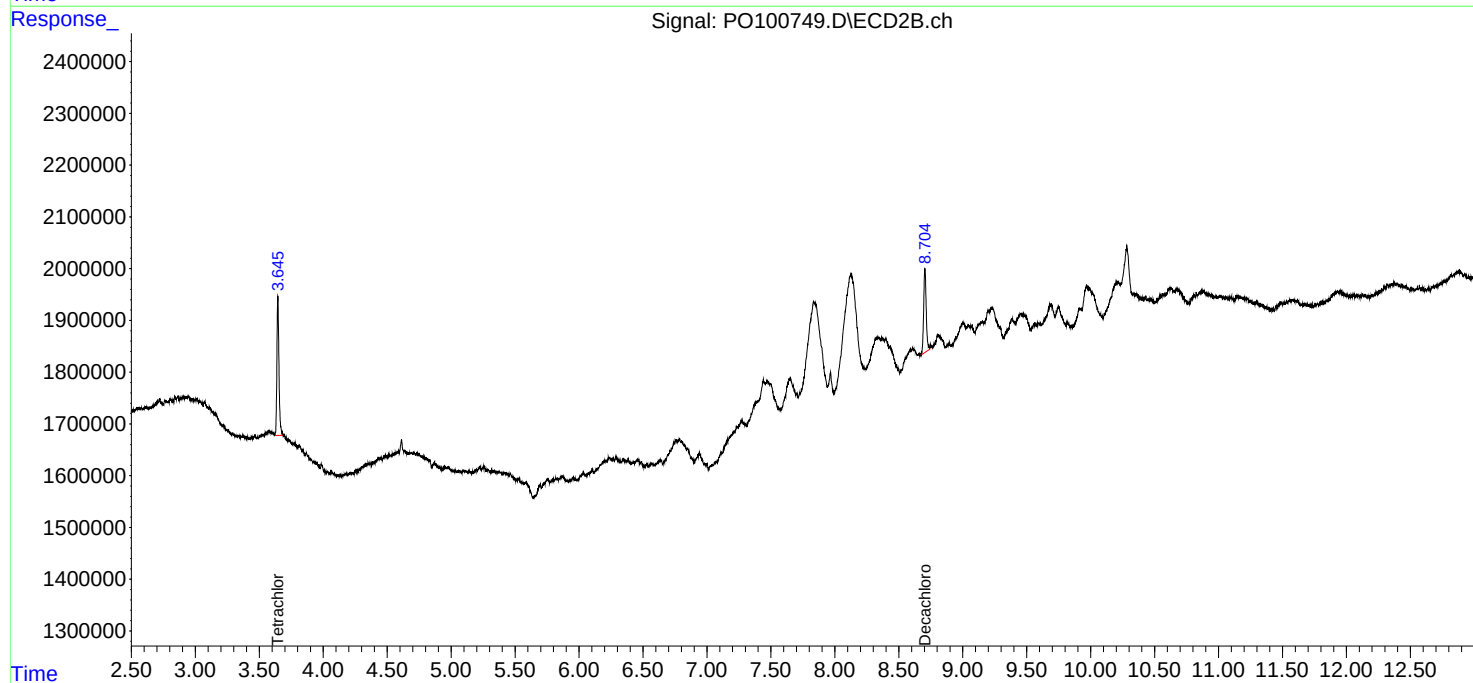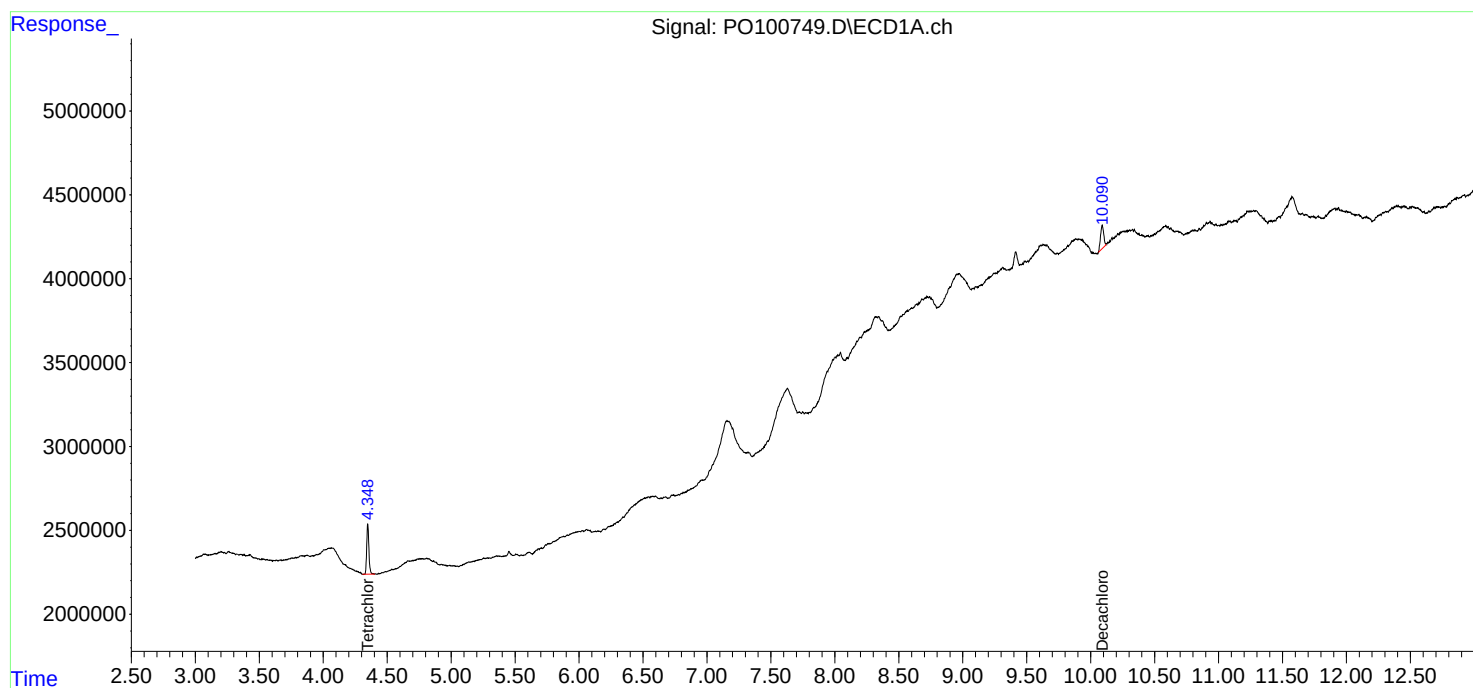

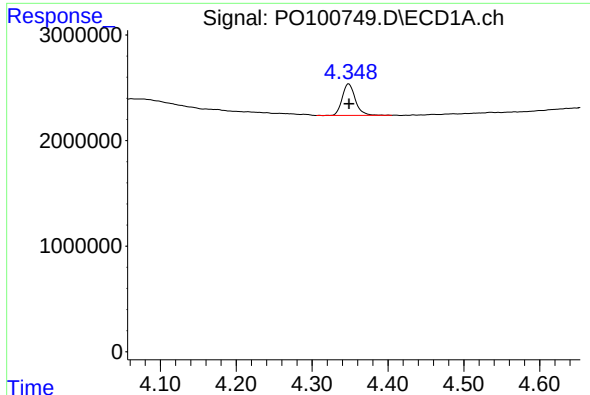


#1 Tetrachloro-m-xylene

R.T.: 4.348 min
Delta R.T.: 0.000 min
Response: 3573048
Conc: 1.15 ng/ml

Instrument :
ECD_O
ClientSampleId :
KMH233N-F


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/27/2023
Supervised By :Ankita Jodhani 12/28/2023

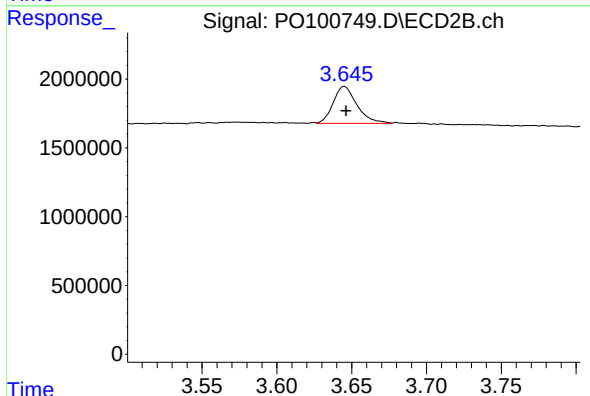


#1 Tetrachloro-m-xylene

R.T.: 3.645 min
Delta R.T.: -0.002 min
Response: 2970610
Conc: 1.45 ng/ml m

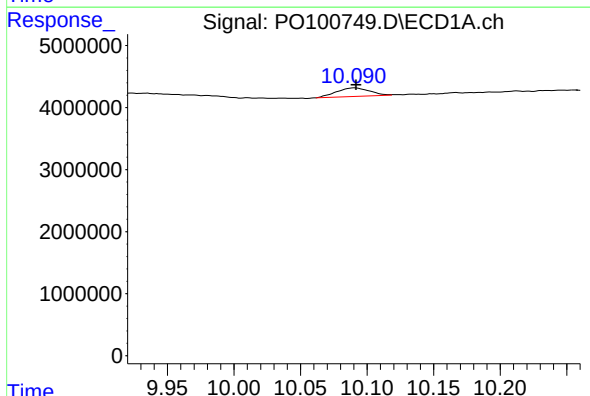

#2 Decachlorobiphenyl

R.T.: 10.090 min
Delta R.T.: -0.002 min
Response: 2411577
Conc: 1.15 ng/ml m

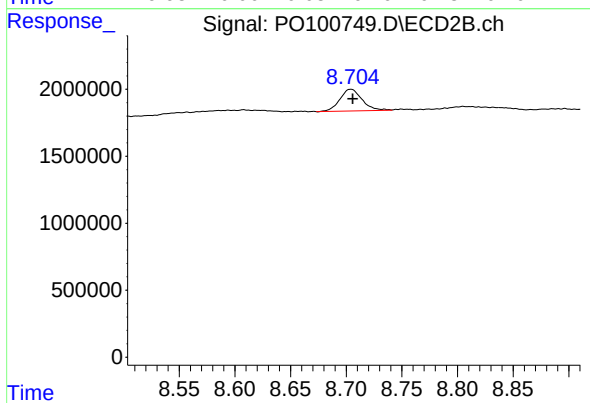

#2 Decachlorobiphenyl

R.T.: 8.704 min
Delta R.T.: -0.002 min
Response: 2248728
Conc: 1.49 ng/ml