

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0122624\
 Data File : P0108781.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Dec 2024 18:37
 Operator : YP/AJ
 Sample : P5377-02 10X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 GAS-TRE-1114

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/27/2024
 Supervised By :Ankita Jodhani 12/27/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 26 20:30:13 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0120624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 07 05:58:15 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.702	3.699	2848663	1541052	0.327	0.304
2) SA Decachlor...	8.766	8.718	950901	485355	0.130m	0.125m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122624\
Data File : PO108781.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Dec 2024 18:37
Operator : YP/AJ
Sample : P5377-02 10X
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
GAS-TRE-1114


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/27/2024
Supervised By :Ankita Jodhani 12/27/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 26 20:30:13 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 07 05:58:15 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

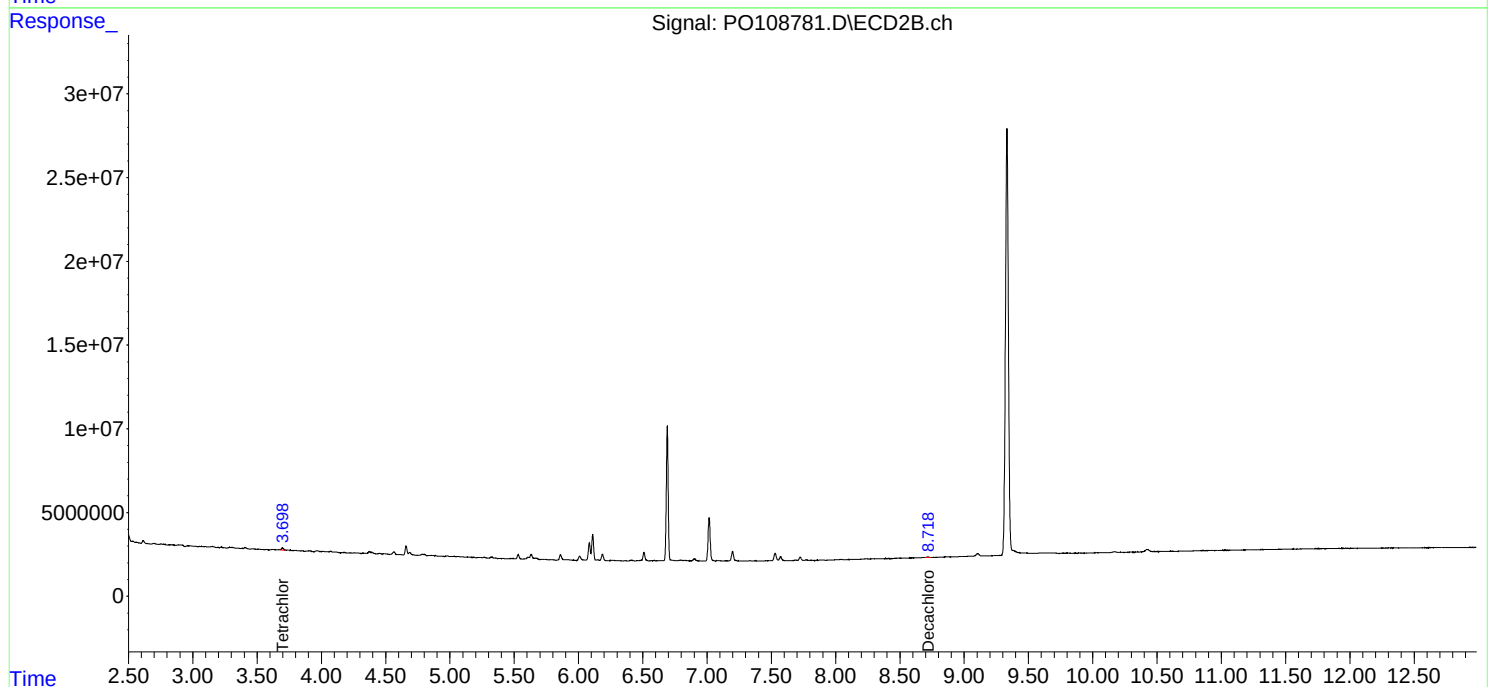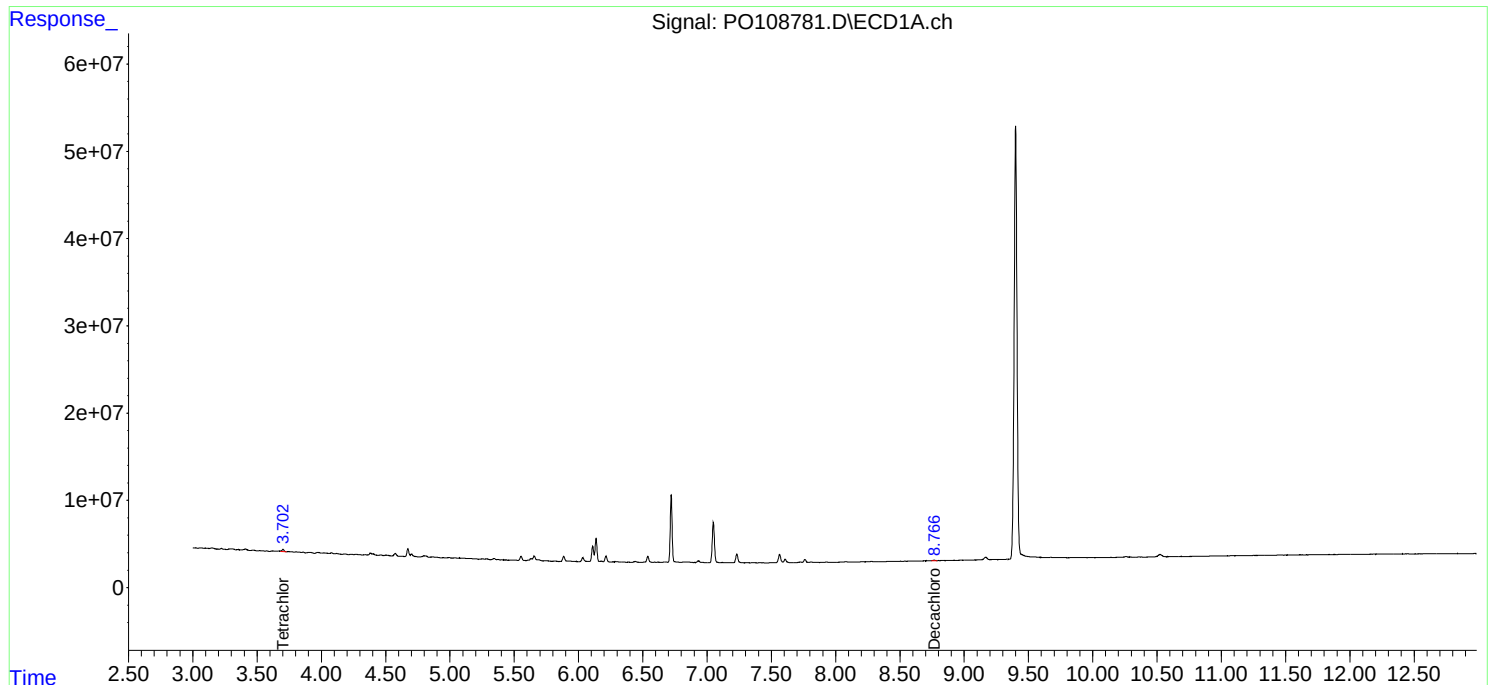

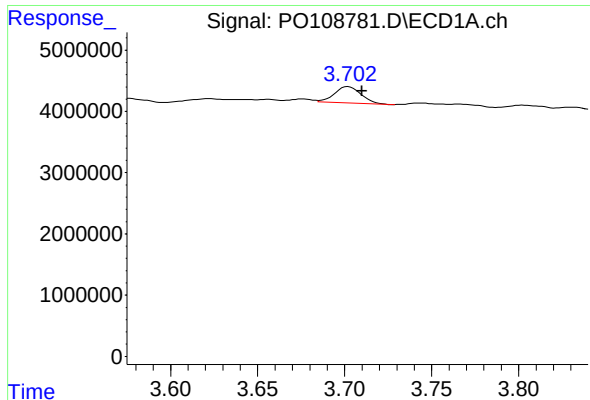


#1 Tetrachloro-m-xylene

R.T.: 3.702 min
Delta R.T.: -0.008 min
Response: 2848663
Conc: 0.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
GAS-TRE-1114


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/27/2024
Supervised By :Ankita Jodhani 12/27/2024

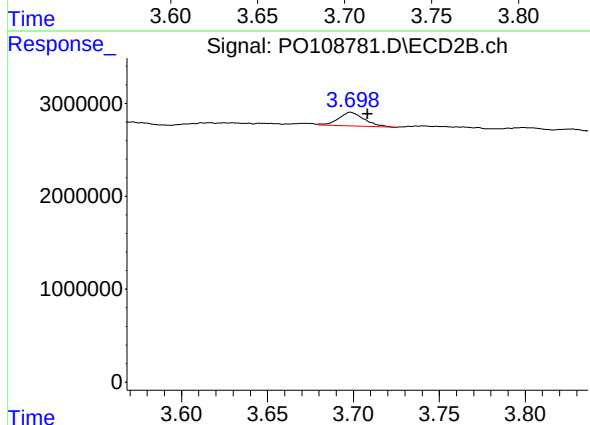


#1 Tetrachloro-m-xylene

R.T.: 3.699 min
Delta R.T.: -0.010 min
Response: 1541052
Conc: 0.30 ng/ml

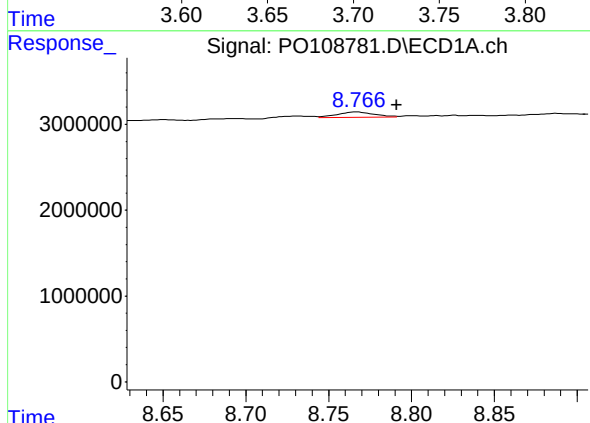

#2 Decachlorobiphenyl

R.T.: 8.766 min
Delta R.T.: -0.025 min
Response: 950901
Conc: 0.13 ng/ml m

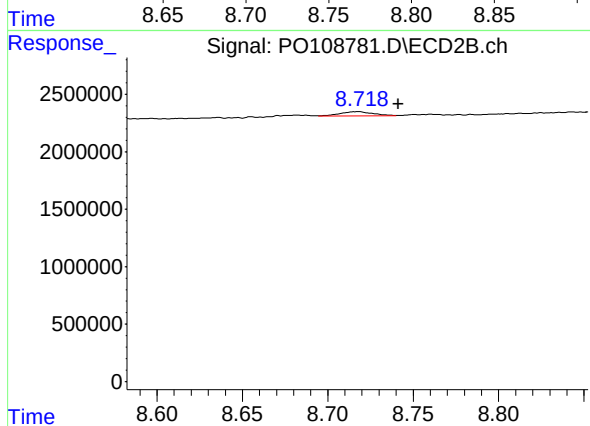

#2 Decachlorobiphenyl

R.T.: 8.718 min
Delta R.T.: -0.023 min
Response: 485355
Conc: 0.13 ng/ml m