

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0122719\
 Data File : P0065017.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Dec 2019 13:01
 Operator : SM/AJ
 Sample : K6297-04
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SIMW-02-20191218-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 27 13:54:50 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0122619.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Dec 26 13:32:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.171	3.446	462804	596303	19.704	21.170
2) SA Decachlor...	9.682	8.357	424213	585777	16.709	17.880

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122719\
Data File : P0065017.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Dec 2019 13:01
Operator : SM/AJ
Sample : K6297-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SIMW-02-20191218-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 27 13:54:50 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO122619.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Dec 26 13:32:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

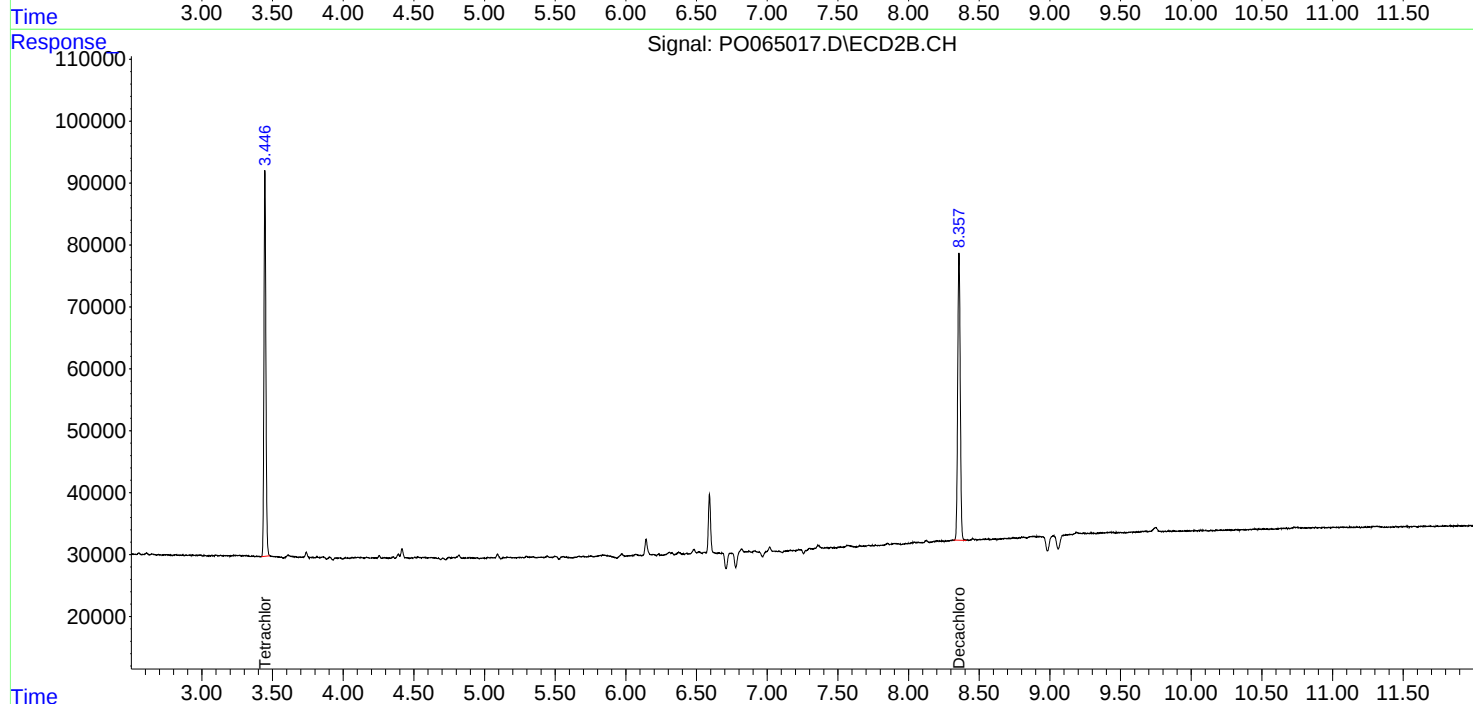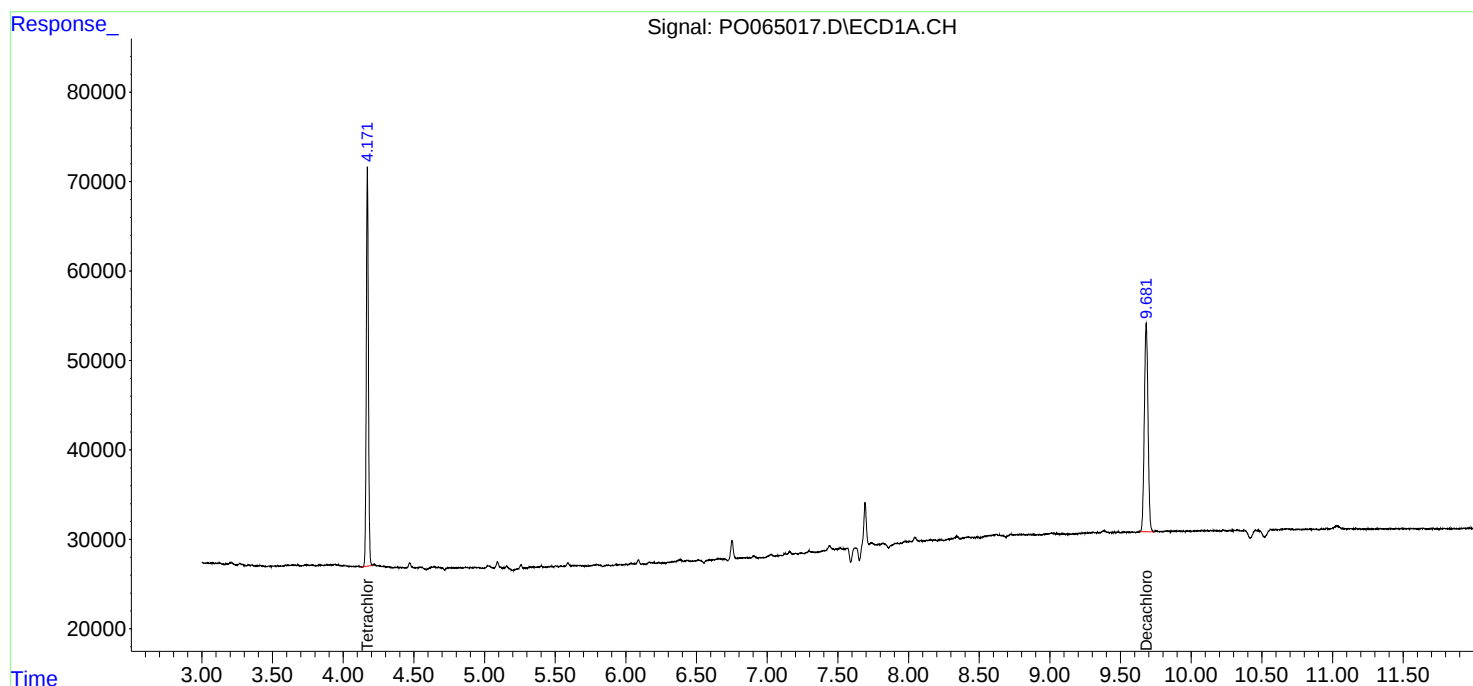


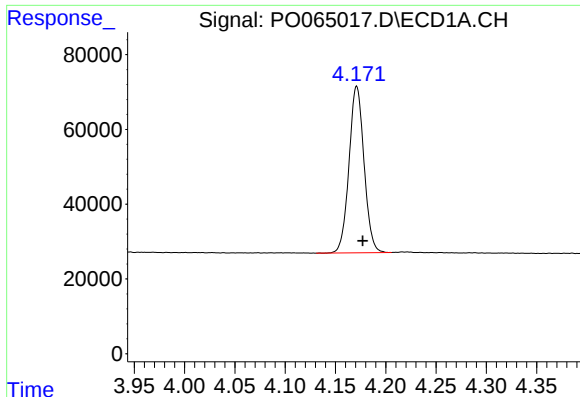

#1 Tetrachloro-m-xylene


R.T.: 4.171 min
Delta R.T.: -0.006 min
Response: 462804
Conc: 19.70 ng/ml

Instrument :
ECD_O
ClientSampleId :
SIMW-02-20191218-A

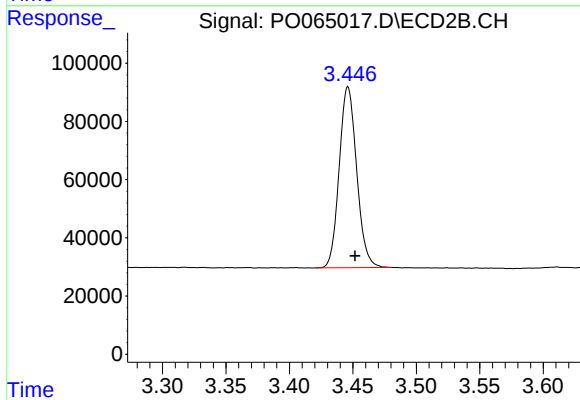


#1 Tetrachloro-m-xylene

R.T.: 3.446 min
Delta R.T.: -0.006 min
Response: 596303
Conc: 21.17 ng/ml

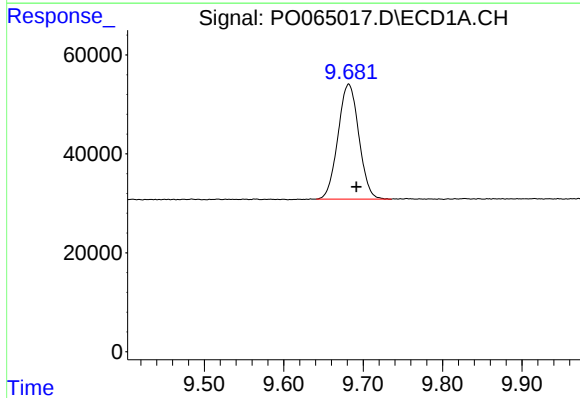

#2 Decachlorobiphenyl

R.T.: 9.682 min
Delta R.T.: -0.009 min
Response: 424213
Conc: 16.71 ng/ml

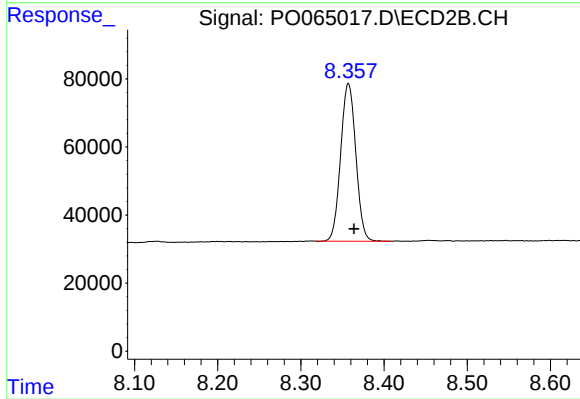

#2 Decachlorobiphenyl

R.T.: 8.357 min
Delta R.T.: -0.007 min
Response: 585777
Conc: 17.88 ng/ml