

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0122722\
 Data File : P0091661.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Dec 2022 23:03
 Operator : YP/AJ
 Sample : N6204-03
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PCB-03

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/28/2022
 Supervised By :Ankita Jodhani 12/28/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 28 03:02:20 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0122122.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Dec 22 03:53:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.289	3.468	38980211	21440782	14.347m	21.144 #
2) SA Decachlor...	10.030	8.463	94249375	21819118	50.087	25.010 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122722\
Data File : PO091661.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Dec 2022 23:03
Operator : YP/AJ
Sample : N6204-03
Misc :
ALS Vial : 31 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PCB-03


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/28/2022
Supervised By :Ankita Jodhani 12/28/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 28 03:02:20 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO122122.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Dec 22 03:53:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

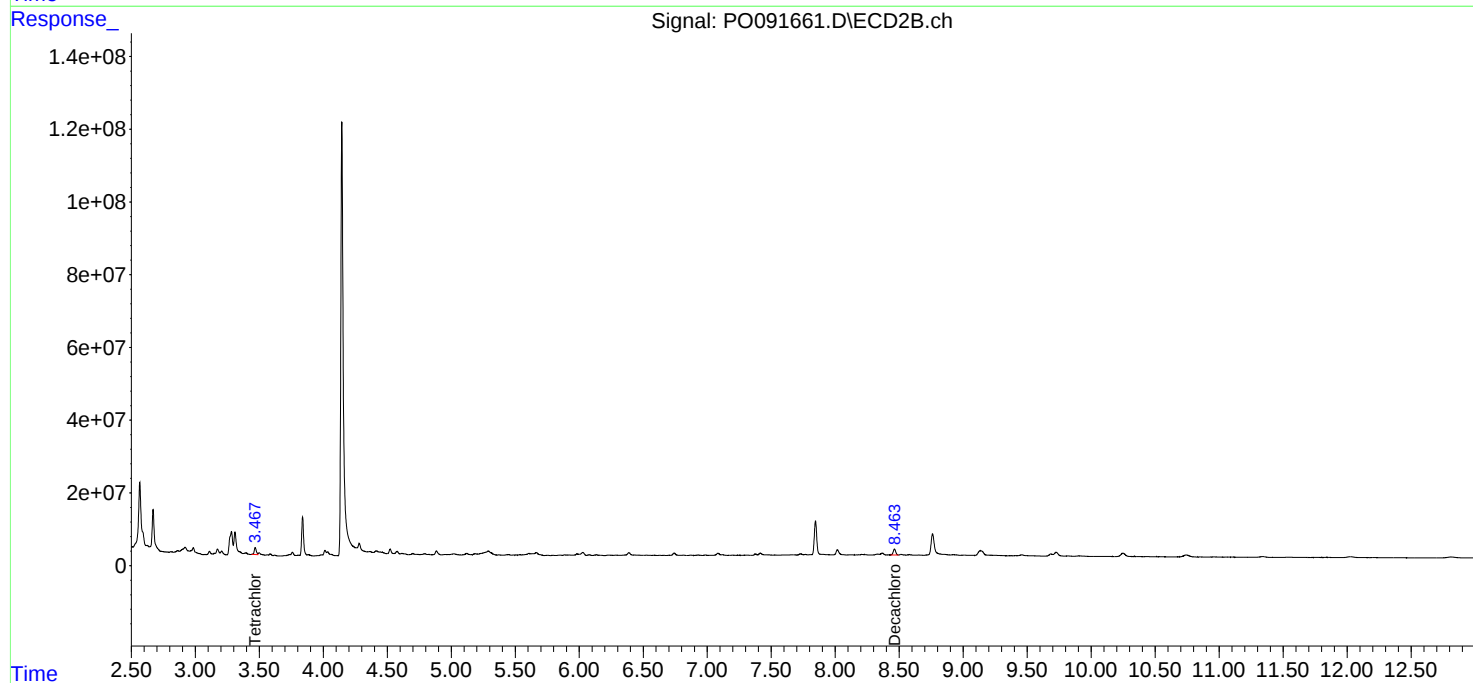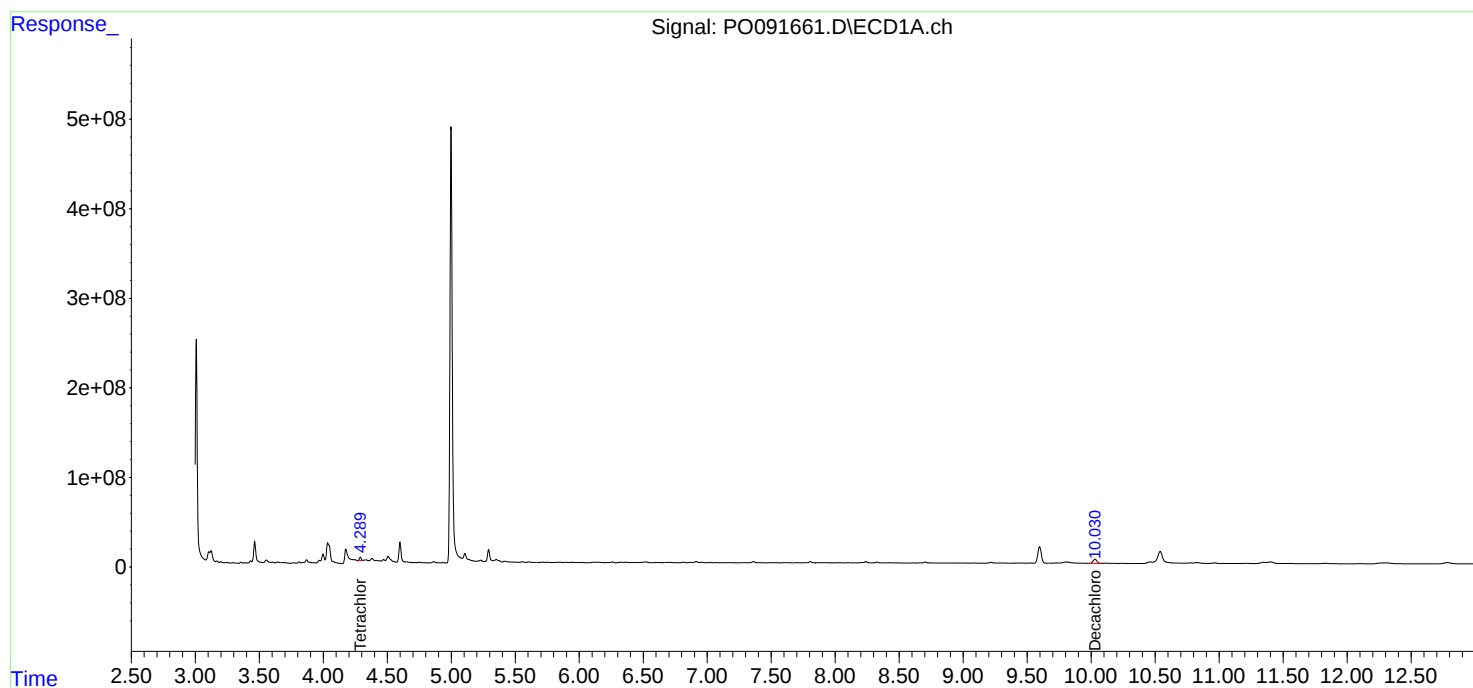

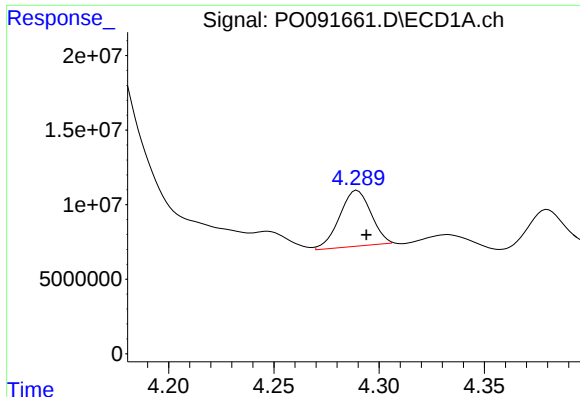


#1 Tetrachloro-m-xylene

R.T.: 4.289 min
Delta R.T.: -0.005 min
Response: 38980211
Conc: 14.35 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-03


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/28/2022
Supervised By :Ankita Jodhani 12/28/2022

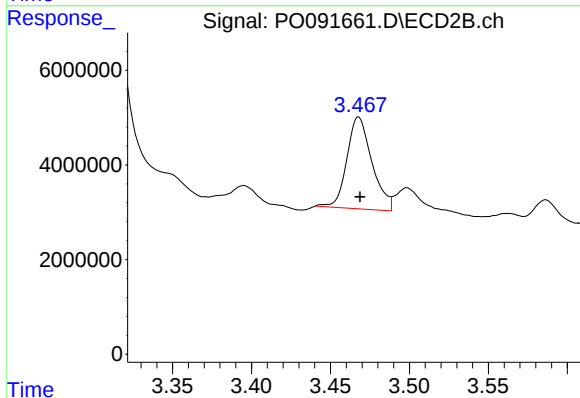


#1 Tetrachloro-m-xylene

R.T.: 3.468 min
Delta R.T.: 0.000 min
Response: 21440782
Conc: 21.14 ng/ml

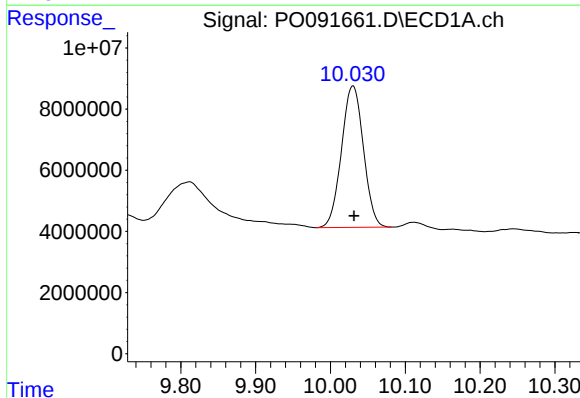

#2 Decachlorobiphenyl

R.T.: 10.030 min
Delta R.T.: -0.002 min
Response: 94249375
Conc: 50.09 ng/ml

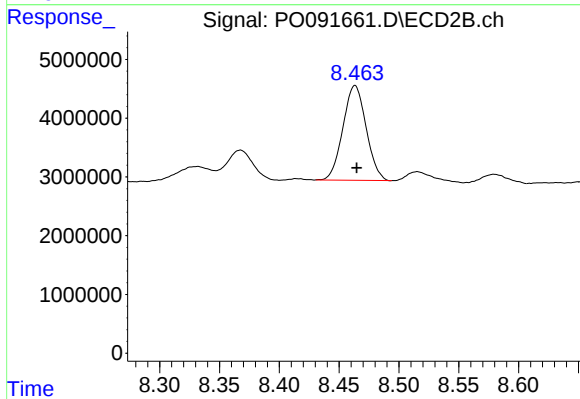

#2 Decachlorobiphenyl

R.T.: 8.463 min
Delta R.T.: -0.001 min
Response: 21819118
Conc: 25.01 ng/ml