

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0122820\
 Data File : P0074220.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Dec 2020 11:41
 Operator : DD\AJ
 Sample : L5212-02DL 5X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S5-02-ADL

Manual Integrations
 APPROVED

mohammad
 12/29/2020 2:36:26 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 28 15:00:08 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0122320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Dec 24 01:16:32 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.932	3.990	442370	260939	4.339m	4.548
2) SA Decachlor...	10.953	9.249	311780	184796	3.201	3.437
Target Compounds						
26) L6 AR-1254-1	7.169	6.103	486512	404286	126.026	116.889
27) L6 AR-1254-2	7.399	6.261	1078399	592606	179.445	195.256
28) L6 AR-1254-3	7.782	6.678	1473812	1186429	245.328	245.174
29) L6 AR-1254-4	8.078	6.917	1451213	924614	276.706	259.905
30) L6 AR-1254-5	8.508	7.343	2526770	2595182	494.859	565.548

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122820\
Data File : PO074220.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Dec 2020 11:41
Operator : DD\AJ
Sample : L5212-02DL 5X
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
S5-02-ADL


Manual Integrations
APPROVED

mohammad
12/29/2020 2:36:26 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 28 15:00:08 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO122320.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Dec 24 01:16:32 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

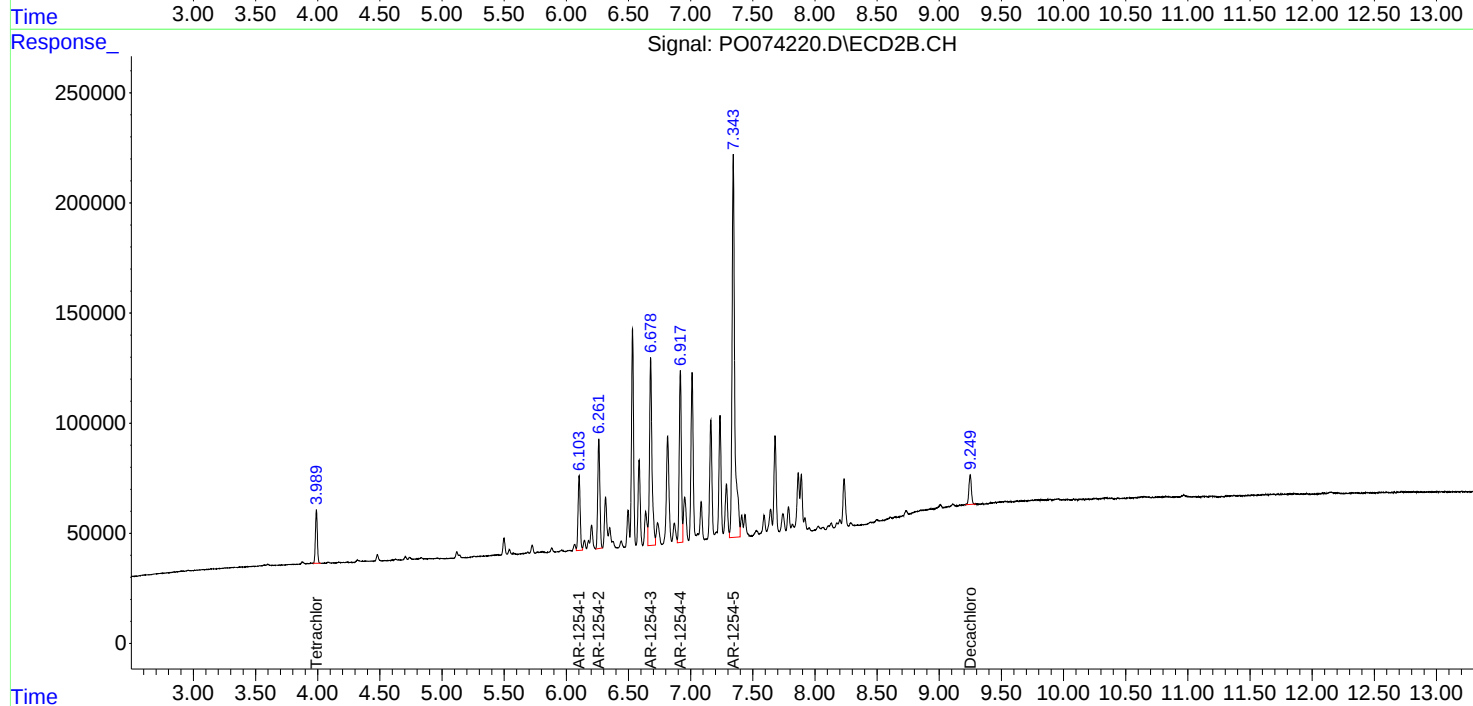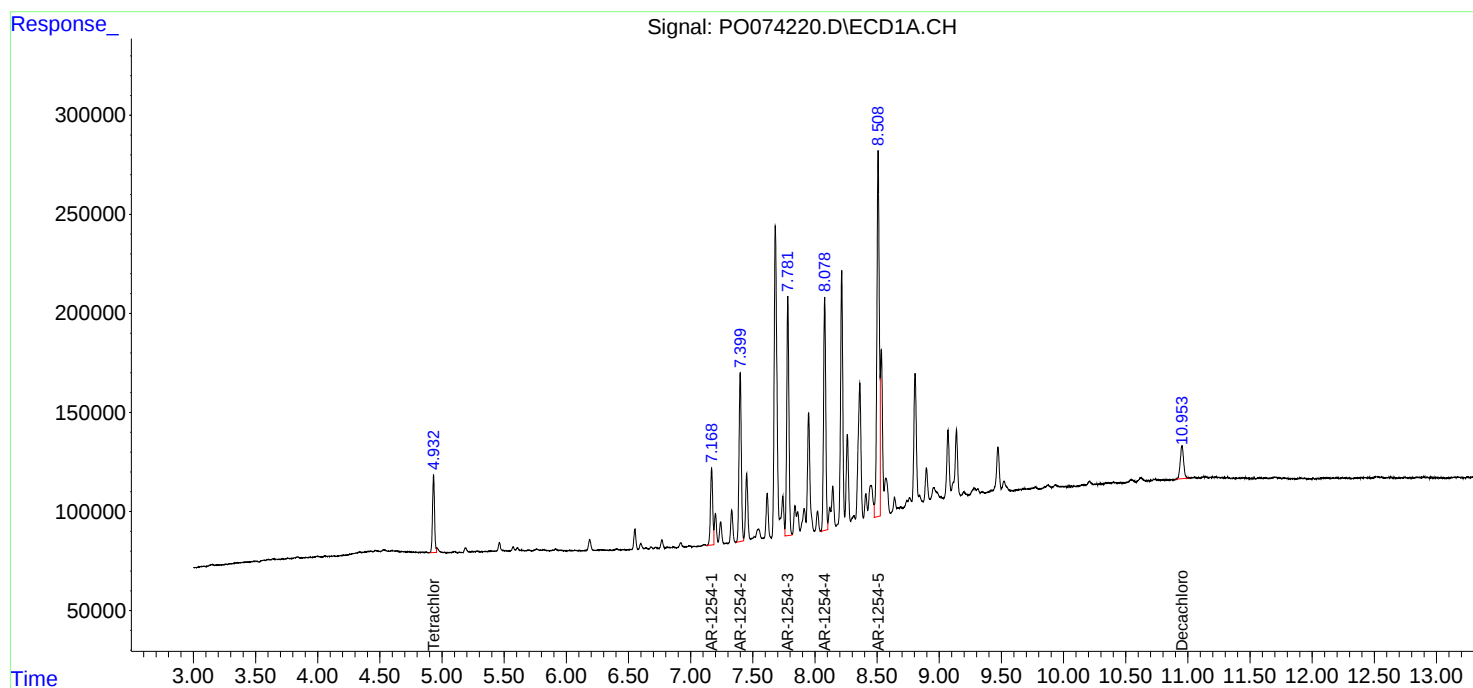

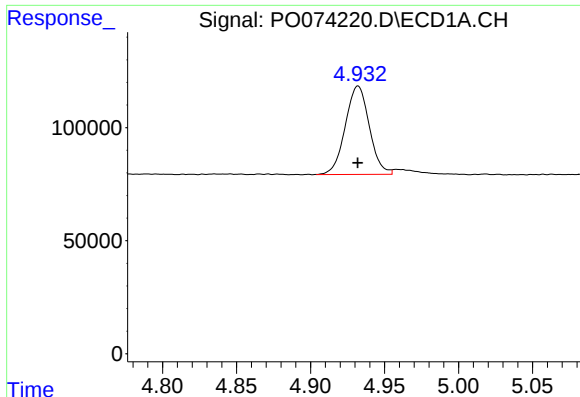


#1 Tetrachloro-m-xylene

R.T.: 4.932 min
Delta R.T.: 0.000 min
Response: 442370
Conc: 4.34 ng/ml m

Instrument :
ECD_O
ClientSampleId :
S5-02-ADL


Manual Integrations
APPROVED

mohammad
12/29/2020 2:36:26 PM

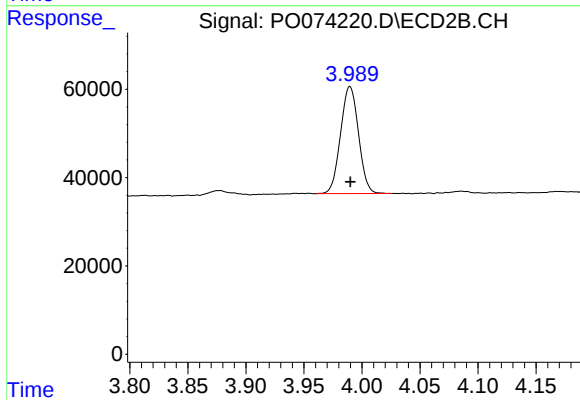


#1 Tetrachloro-m-xylene

R.T.: 3.990 min
Delta R.T.: 0.000 min
Response: 260939
Conc: 4.55 ng/ml

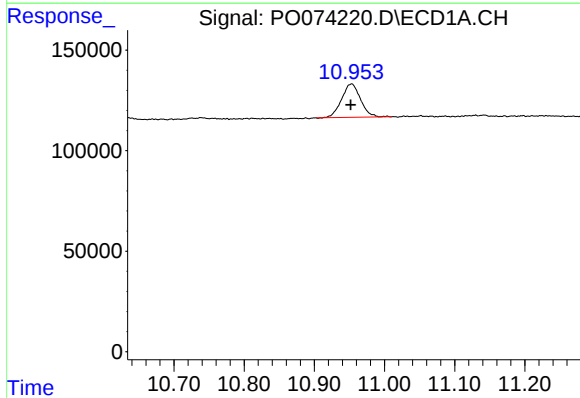


#2 Decachlorobiphenyl

R.T.: 10.953 min
Delta R.T.: 0.001 min
Response: 311780
Conc: 3.20 ng/ml

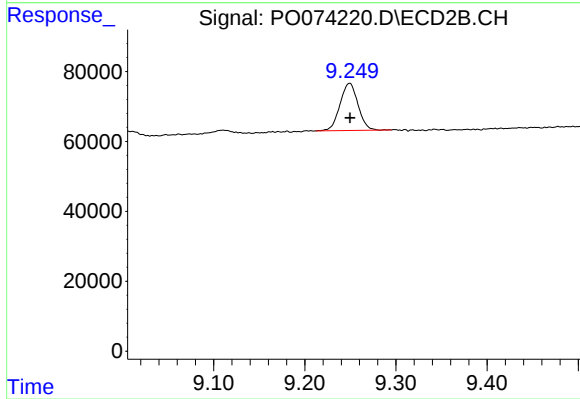

#2 Decachlorobiphenyl

R.T.: 9.249 min
Delta R.T.: 0.000 min
Response: 184796
Conc: 3.44 ng/ml

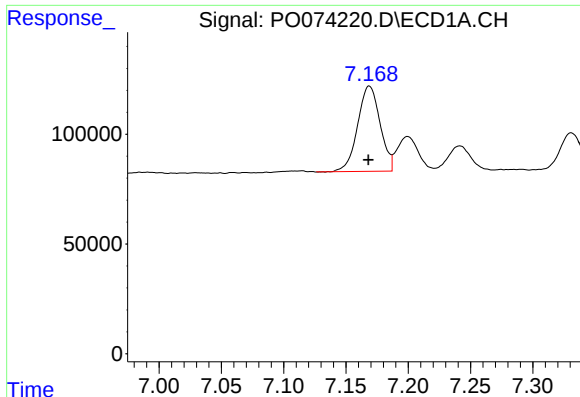


#26 AR-1254-1

R.T.: 7.169 min
Delta R.T.: 0.000 min
Response: 486512
Conc: 126.03 ng/ml

Instrument :
ECD_O
ClientSampleId :
S5-02-ADL


Manual Integrations
APPROVED

mohammad
12/29/2020 2:36:26 PM

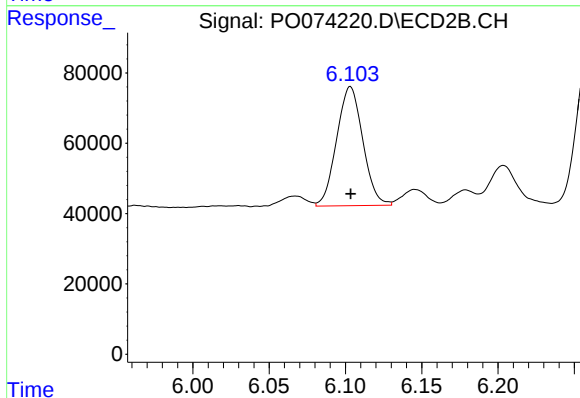


#26 AR-1254-1

R.T.: 6.103 min
Delta R.T.: 0.000 min
Response: 404286
Conc: 116.89 ng/ml

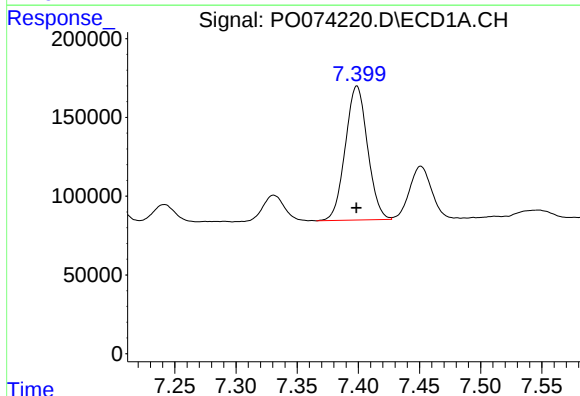


#27 AR-1254-2

R.T.: 7.399 min
Delta R.T.: 0.000 min
Response: 1078399
Conc: 179.44 ng/ml

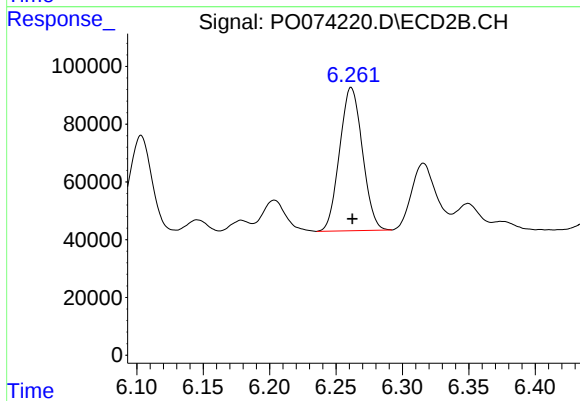

#27 AR-1254-2

R.T.: 6.261 min
Delta R.T.: 0.000 min
Response: 592606
Conc: 195.26 ng/ml

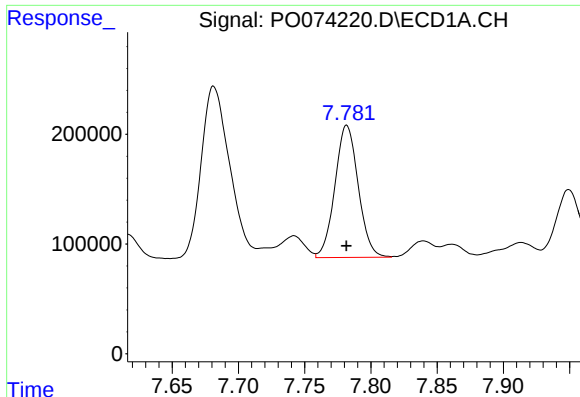


#28 AR-1254-3

R.T.: 7.782 min
Delta R.T.: 0.000 min
Response: 1473812
Conc: 245.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
S5-02-ADL


Manual Integrations
APPROVED

mohammad
12/29/2020 2:36:26 PM

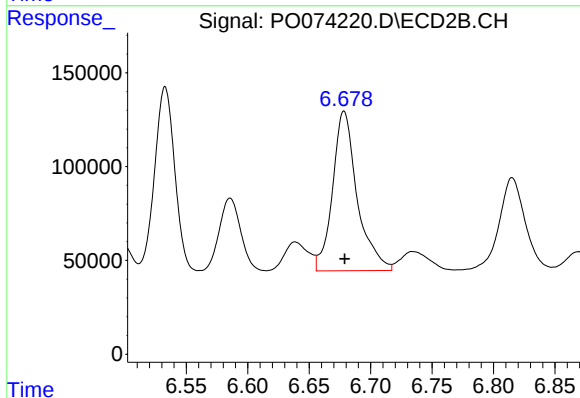


#28 AR-1254-3

R.T.: 6.678 min
Delta R.T.: 0.000 min
Response: 1186429
Conc: 245.17 ng/ml

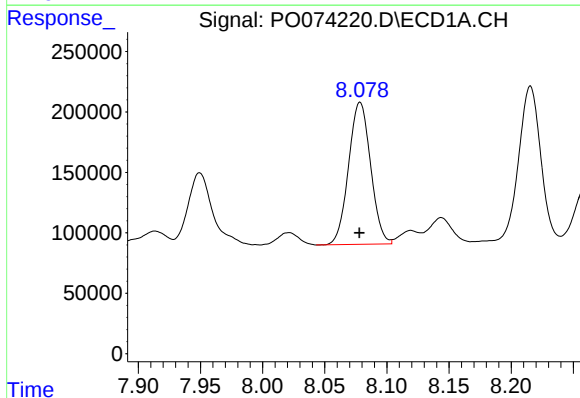


#29 AR-1254-4

R.T.: 8.078 min
Delta R.T.: 0.000 min
Response: 1451213
Conc: 276.71 ng/ml

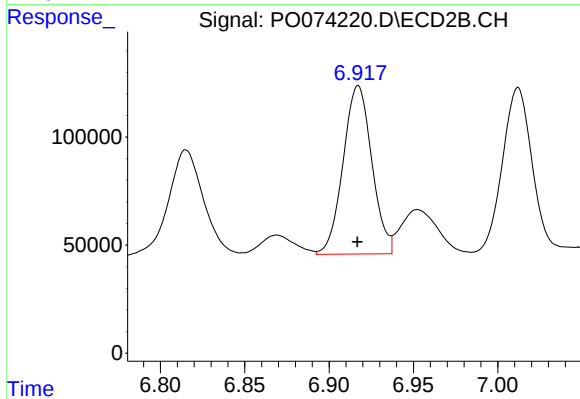

#29 AR-1254-4

R.T.: 6.917 min
Delta R.T.: 0.000 min
Response: 924614
Conc: 259.90 ng/ml

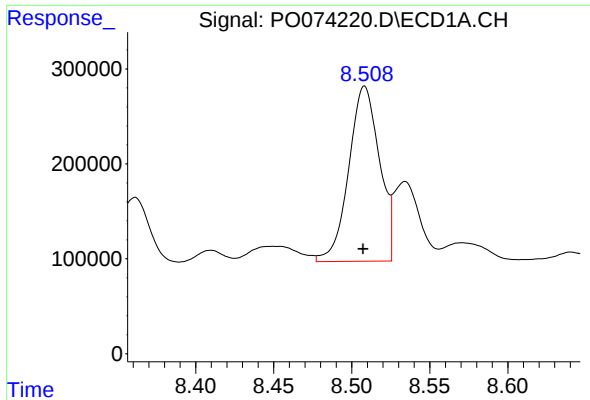


#30 AR-1254-5

R.T.: 8.508 min
Delta R.T.: 0.001 min
Response: 2526770
Conc: 494.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
S5-02-ADL

Manual Integrations
APPROVED

mohammad
12/29/2020 2:36:26 PM

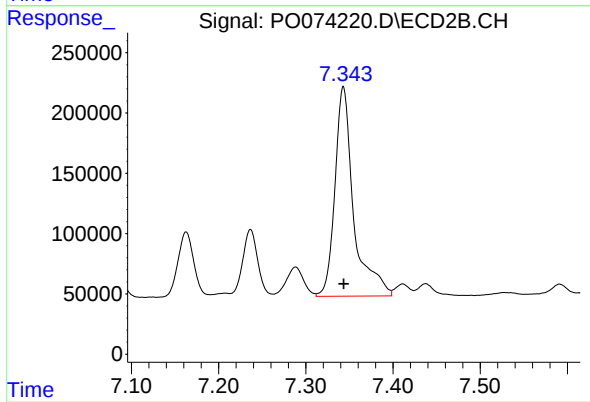

#30 AR-1254-5

R.T.: 7.343 min
Delta R.T.: 0.000 min
Response: 2595182
Conc: 565.55 ng/ml