

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122820\
 Data File : PO074256.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Dec 2020 22:13
 Operator : DD\AJ
 Sample : L5215-03
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 DRUMS-1-4

Manual Integrations
 APPROVED

mohammad
 12/29/2020 2:36:55 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 29 03:40:27 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO122320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Dec 24 01:16:32 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.955f	4.028f	2027606	1094261	19.886m	19.073m
2) SA Decachlor...	10.954	9.251	2121159	996457	21.781	18.535

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122820\
Data File : PO074256.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Dec 2020 22:13
Operator : DD\AJ
Sample : L5215-03
Misc :
ALS Vial : 43 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
DRUMS-1-4


Manual Integrations
APPROVED

mohammad
12/29/2020 2:36:55 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 29 03:40:27 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO122320.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Dec 24 01:16:32 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

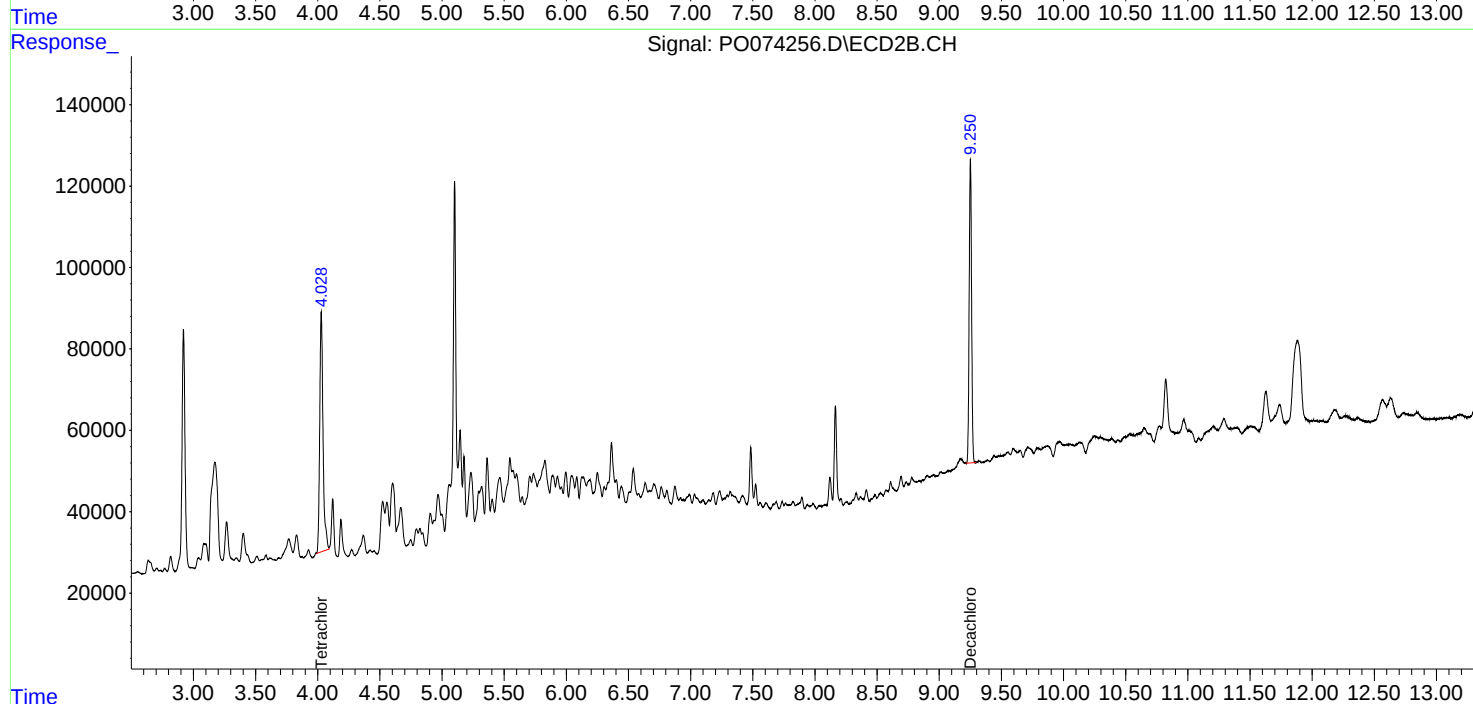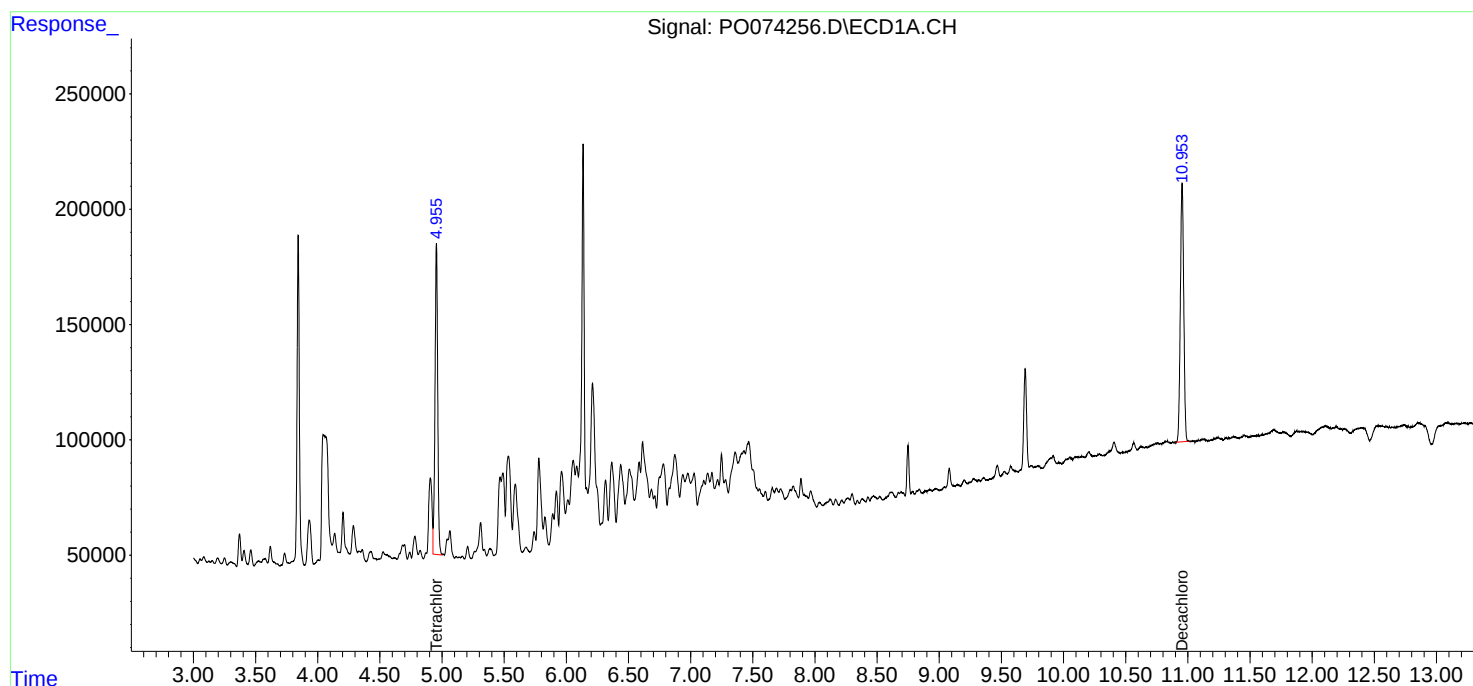

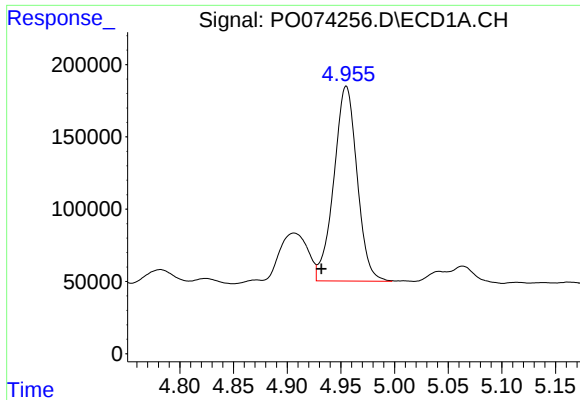


#1 Tetrachloro-m-xylene

R.T.: 4.955 min
Delta R.T.: 0.023 min
Response: 2027606
Conc: 19.89 ng/ml m

Instrument :
ECD_O
ClientSampleId :
DRUMS-1-4


Manual Integrations
APPROVED

mohammad
12/29/2020 2:36:55 PM

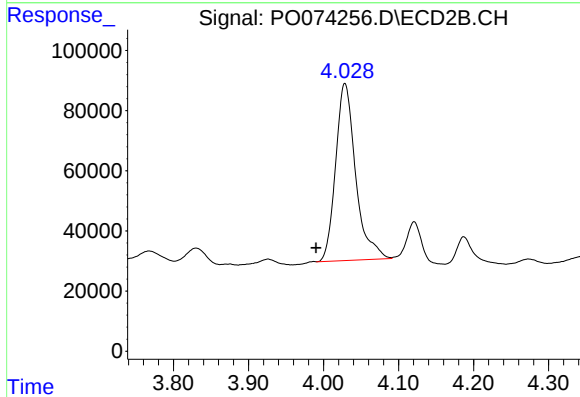


#1 Tetrachloro-m-xylene

R.T.: 4.028 min
Delta R.T.: 0.038 min
Response: 1094261
Conc: 19.07 ng/ml m

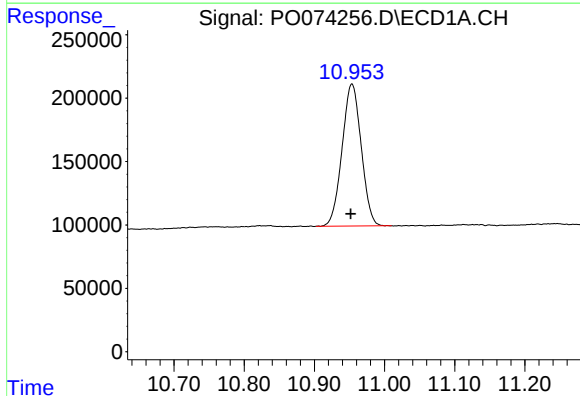

#2 Decachlorobiphenyl

R.T.: 10.954 min
Delta R.T.: 0.002 min
Response: 2121159
Conc: 21.78 ng/ml

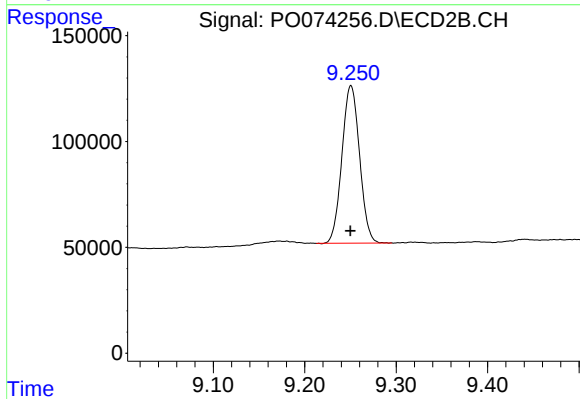

#2 Decachlorobiphenyl

R.T.: 9.251 min
Delta R.T.: 0.000 min
Response: 996457
Conc: 18.53 ng/ml