

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122822\
 Data File : PO091673.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Dec 2022 10:48
 Operator : YP/AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 29 02:01:16 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO122122.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Dec 22 03:53:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.340f	3.423f	714193	92335	0.263	0.091 #
Target Compounds						
8) L2 AR-1221-1	0.000	3.631f	0	202761	N.D.	15.896 #
20) L4 AR-1242-5	0.000	5.354	0	111119	N.D.	4.156 #
25) L5 AR-1248-5	0.000	5.379	0	103005	N.D.	3.022 #
26) L6 AR-1254-1	0.000	5.354	0	111119	N.D.	2.024 #
27) L6 AR-1254-2	0.000	5.505	0	175556	N.D.	3.500 #
28) L6 AR-1254-3	6.927	0.000	371763	0	2.485	N.D. #
29) L6 AR-1254-4	7.271f	6.139	2203098	32103	19.815	0.686 #
32) L7 AR-1260-2	7.295f	0.000	1274475	0	9.310	N.D. #
33) L7 AR-1260-3	7.707	6.376	388857	518410	4.761	7.762 #
36) L8 AR-1262-1	7.707	0.000	388857	0	2.617	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122822\
Data File : PO091673.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Dec 2022 10:48
Operator : YP/AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 29 02:01:16 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO122122.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Dec 22 03:53:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

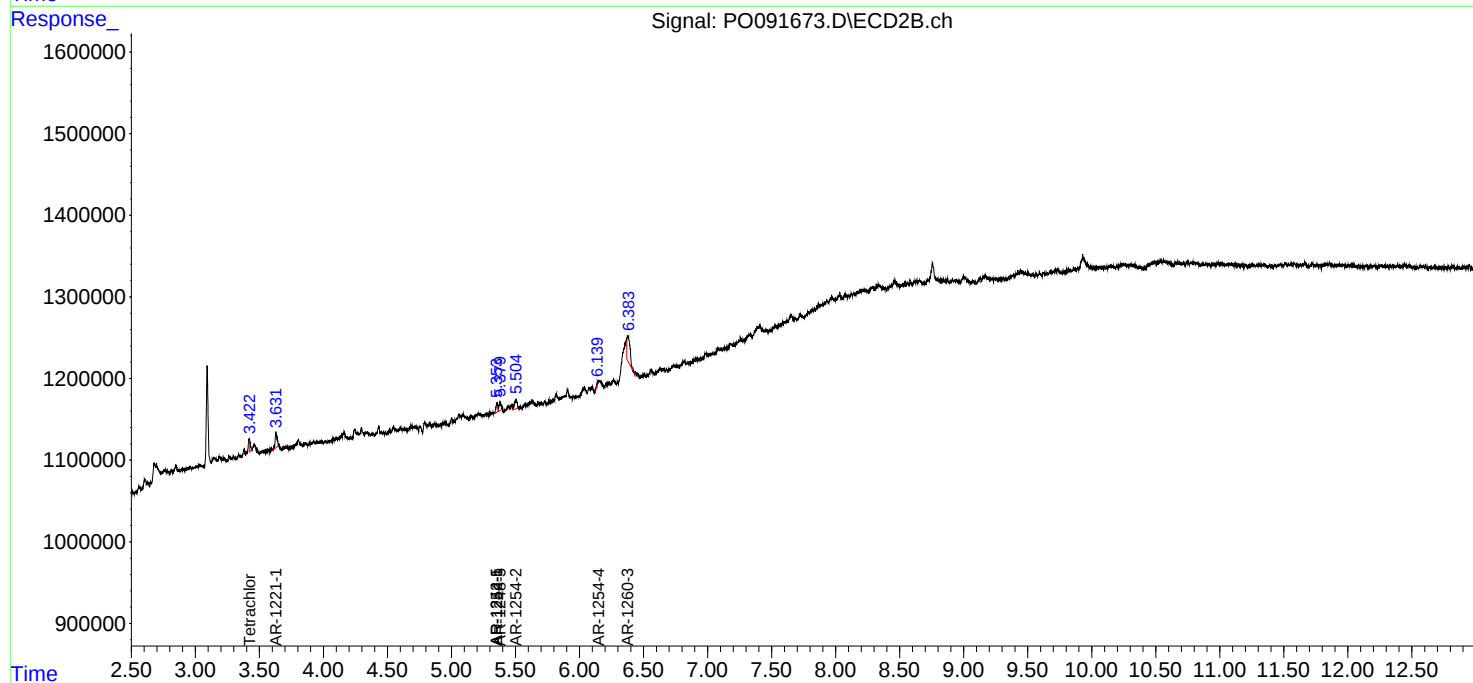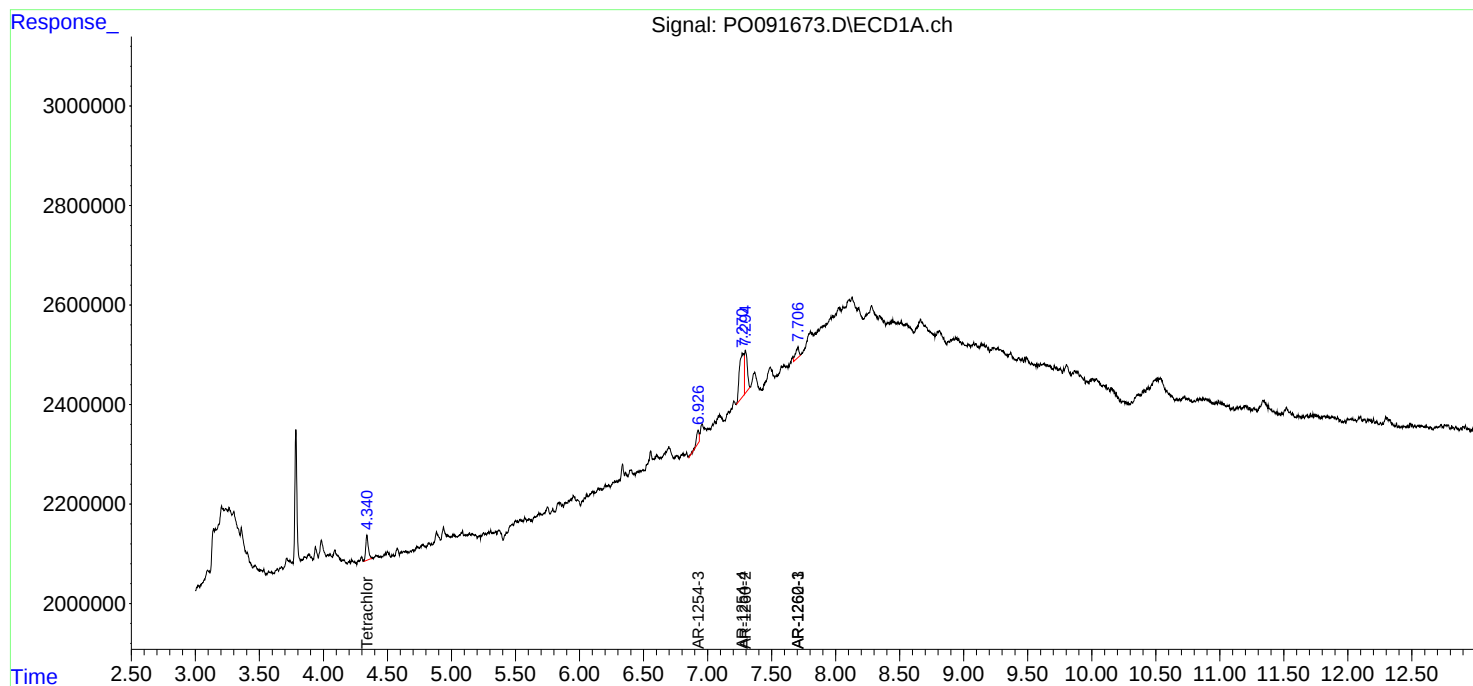


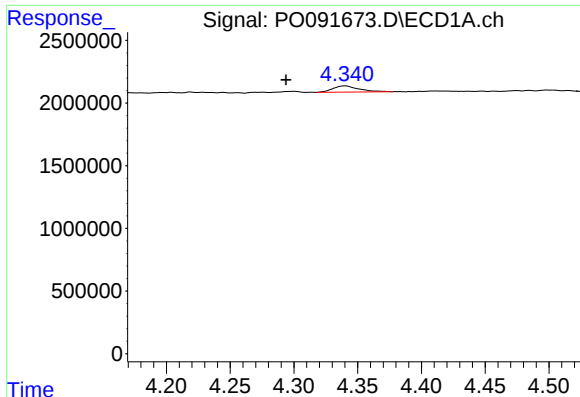

#1 Tetrachloro-m-xylene


R.T.: 4.340 min
Delta R.T.: 0.046 min
Response: 714193
Conc: 0.26 ng/ml

Instrument :
ECD_O
ClientSampleId :

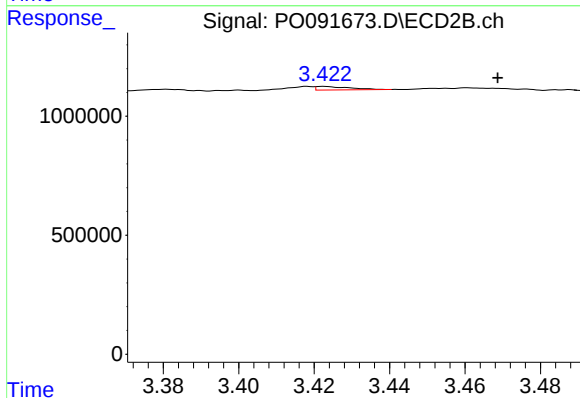


#1 Tetrachloro-m-xylene

R.T.: 3.423 min
Delta R.T.: -0.046 min
Response: 92335
Conc: 0.09 ng/ml

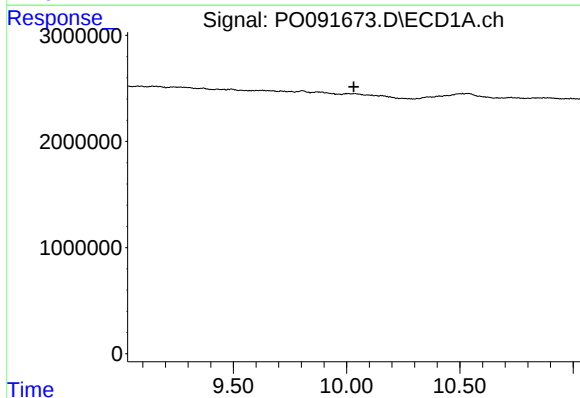


#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.032 min
Response: 0
Conc: N.D.

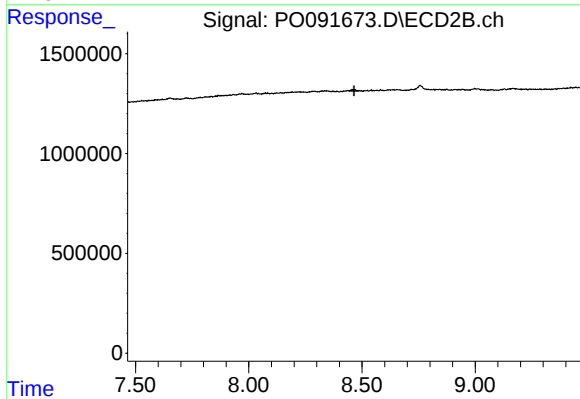

#2 Decachlorobiphenyl


R.T.: 0.000 min
Exp R.T. : 8.465 min
Response: 0
Conc: N.D.

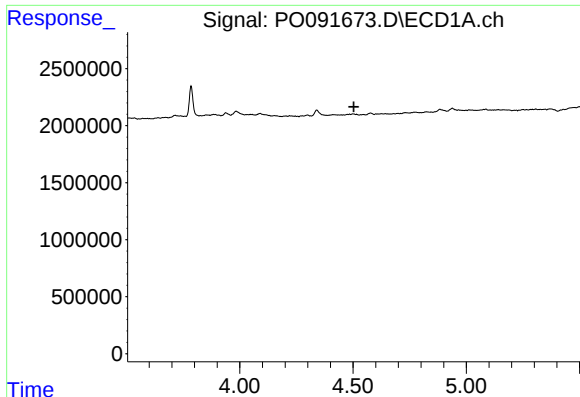

#8 AR-1221-1


R.T.: 0.000 min
Exp R.T.: 4.503 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

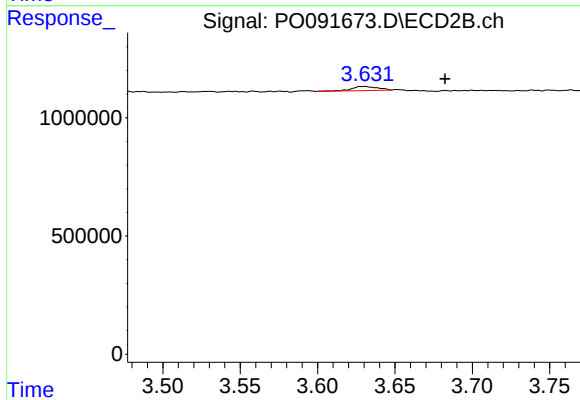


#8 AR-1221-1

R.T.: 3.631 min
Delta R.T.: -0.052 min
Response: 202761
Conc: 15.90 ng/ml

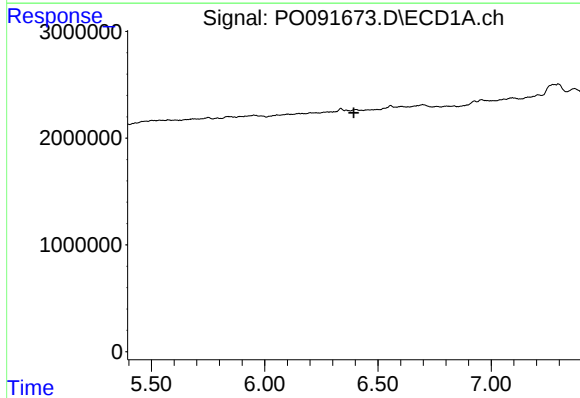


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T.: 6.393 min
Response: 0
Conc: N.D.

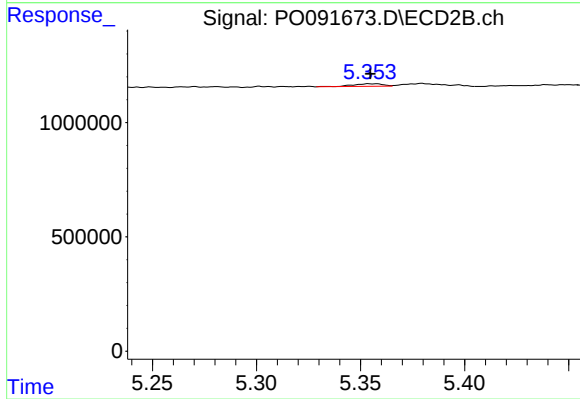

#20 AR-1242-5


R.T.: 5.354 min
Delta R.T.: 0.000 min
Response: 111119
Conc: 4.16 ng/ml

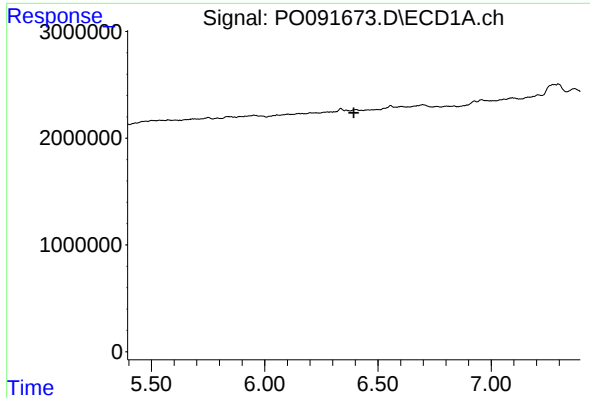

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T.: 6.393 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

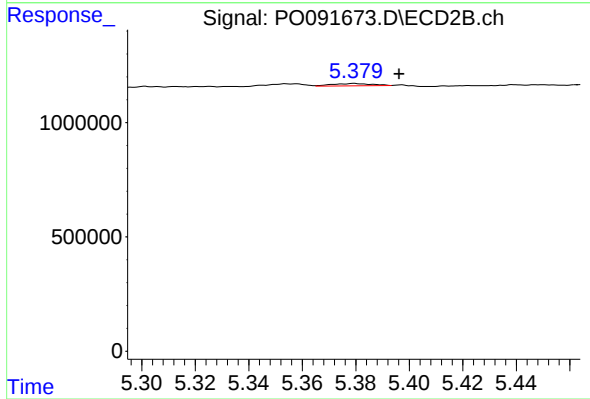


#25 AR-1248-5

R.T.: 5.379 min
Delta R.T.: -0.017 min
Response: 103005
Conc: 3.02 ng/ml

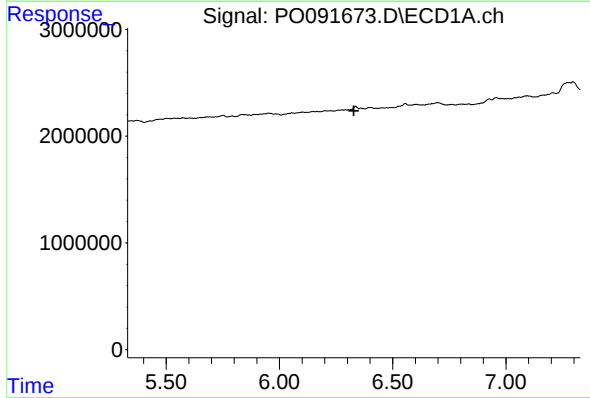


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T.: 6.328 min
Response: 0
Conc: N.D.

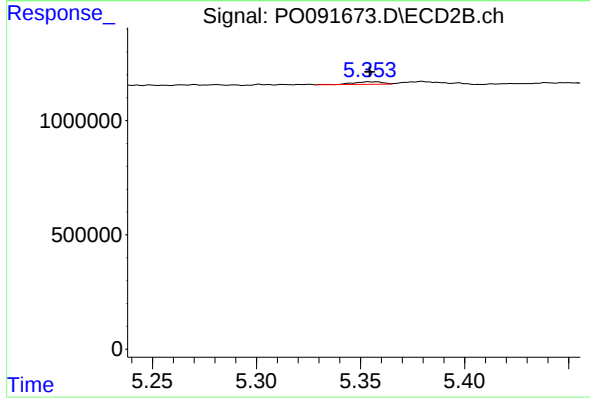

#26 AR-1254-1


R.T.: 5.354 min
Delta R.T.: 0.000 min
Response: 111119
Conc: 2.02 ng/ml

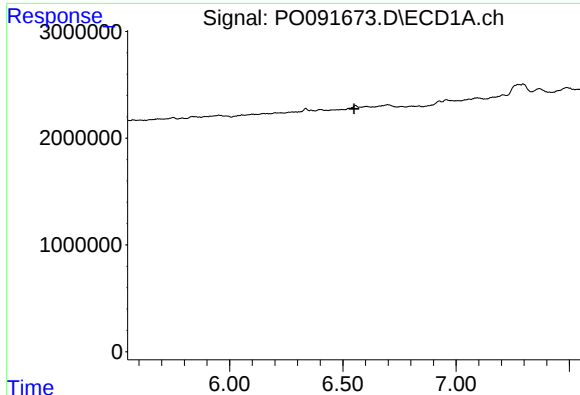

#27 AR-1254-2


R.T.: 0.000 min
Exp R.T.: 6.549 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

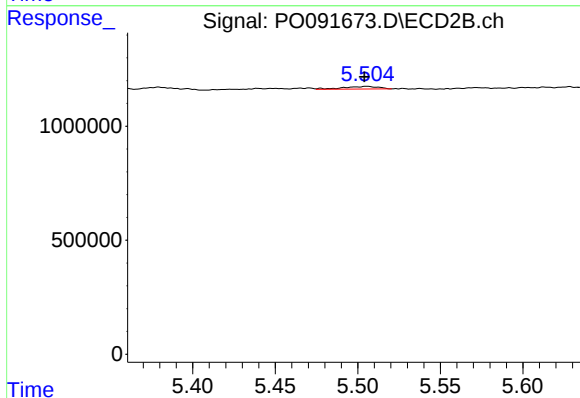


#27 AR-1254-2

R.T.: 5.505 min
Delta R.T.: 0.002 min
Response: 175556
Conc: 3.50 ng/ml

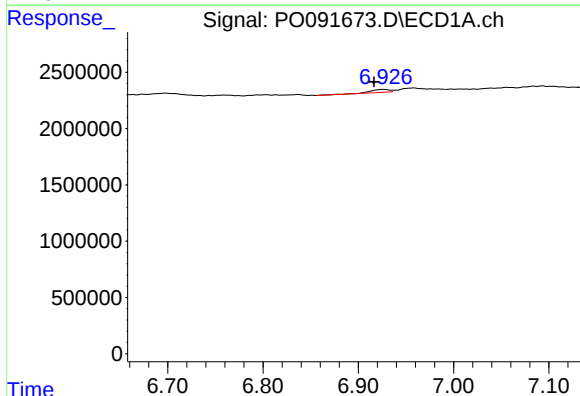


#28 AR-1254-3

R.T.: 6.927 min
Delta R.T.: 0.010 min
Response: 371763
Conc: 2.48 ng/ml

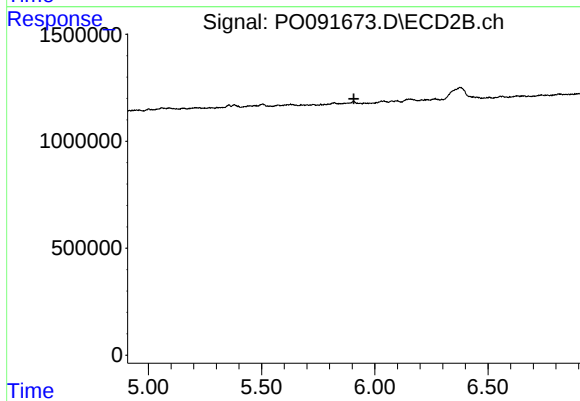

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T.: 5.907 min
Response: 0
Conc: N.D.

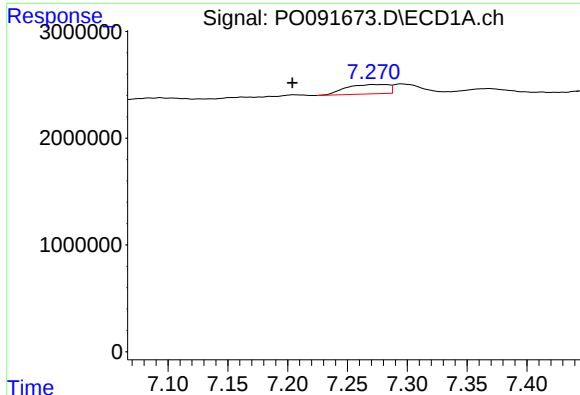

#29 AR-1254-4


R.T.: 7.271 min
Delta R.T.: 0.067 min
Response: 2203098
Conc: 19.82 ng/ml

Instrument :
ECD_O
ClientSampleId :

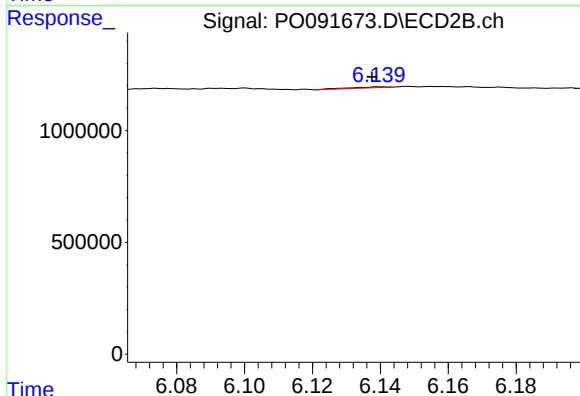


#29 AR-1254-4

R.T.: 6.139 min
Delta R.T.: 0.002 min
Response: 32103
Conc: 0.69 ng/ml

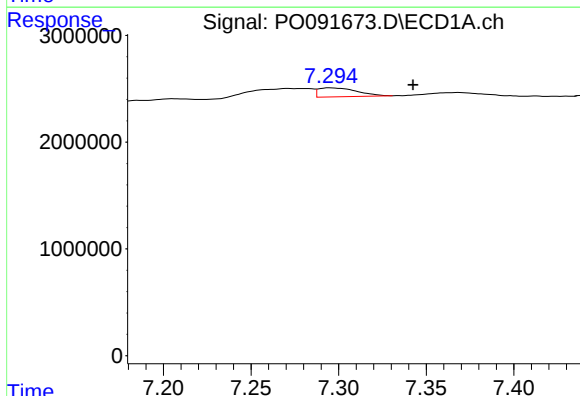


#32 AR-1260-2

R.T.: 7.295 min
Delta R.T.: -0.047 min
Response: 1274475
Conc: 9.31 ng/ml

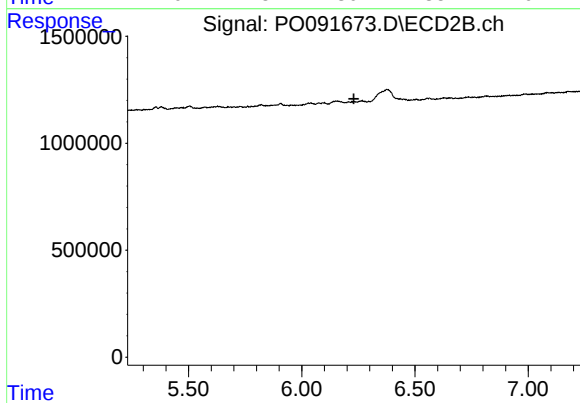

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T.: 6.230 min
Response: 0
Conc: N.D.

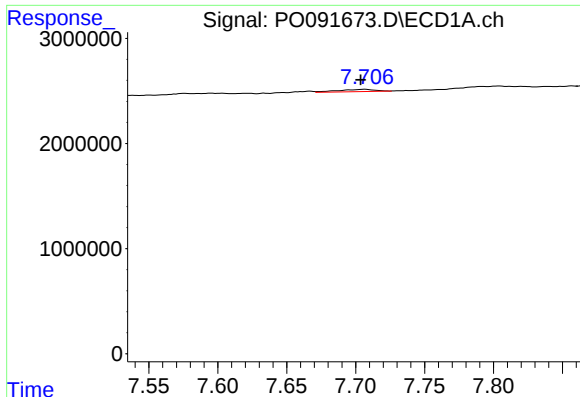

#33 AR-1260-3


R.T.: 7.707 min
Delta R.T.: 0.003 min
Response: 388857
Conc: 4.76 ng/ml

Instrument :
ECD_O
ClientSampleId :

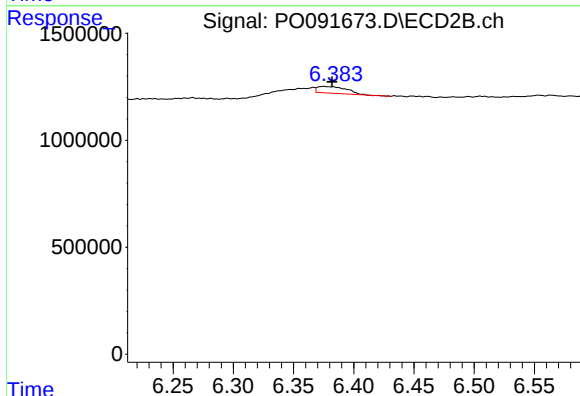


#33 AR-1260-3

R.T.: 6.376 min
Delta R.T.: -0.006 min
Response: 518410
Conc: 7.76 ng/ml

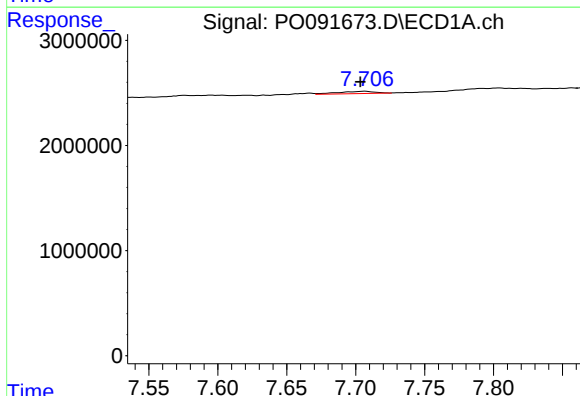

#36 AR-1262-1

R.T.: 7.707 min
Delta R.T.: 0.004 min
Response: 388857
Conc: 2.62 ng/ml

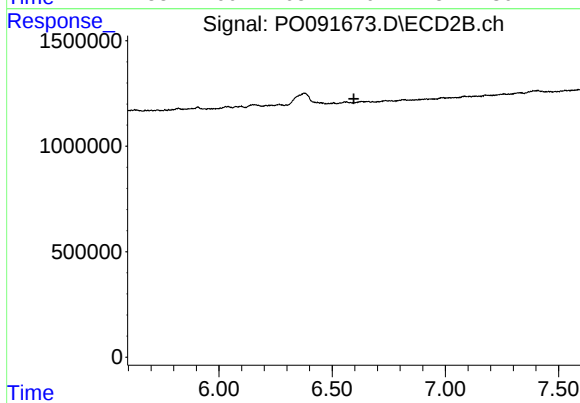

#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 6.596 min
Response: 0
Conc: N.D.