

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122822\
 Data File : PO091698.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Dec 2022 19:03
 Operator : YP/AJ
 Sample : N6213-06DL 200X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-6DL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/29/2022
 Supervised By :Ankita Jodhani 12/29/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 29 06:15:58 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO122122.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Dec 22 03:53:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds								
16)	L4	AR-1242-1	5.465	4.550	42817568	18341969	589.614	664.285
17)	L4	AR-1242-2	5.486	4.568	56905643	24281573	549.247	626.422
18)	L4	AR-1242-3	5.549	4.743	34813190	11808328	537.424	566.979
19)	L4	AR-1242-4	5.648	4.829	25087361	9015940	503.503	410.202
20)	L4	AR-1242-5	6.388	5.352	8874708	6230065	169.680m	232.996 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122822\
Data File : PO091698.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Dec 2022 19:03
Operator : YP/AJ
Sample : N6213-06DL 200X
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SB-6DL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/29/2022
Supervised By :Ankita Jodhani 12/29/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 29 06:15:58 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO122122.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Dec 22 03:53:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

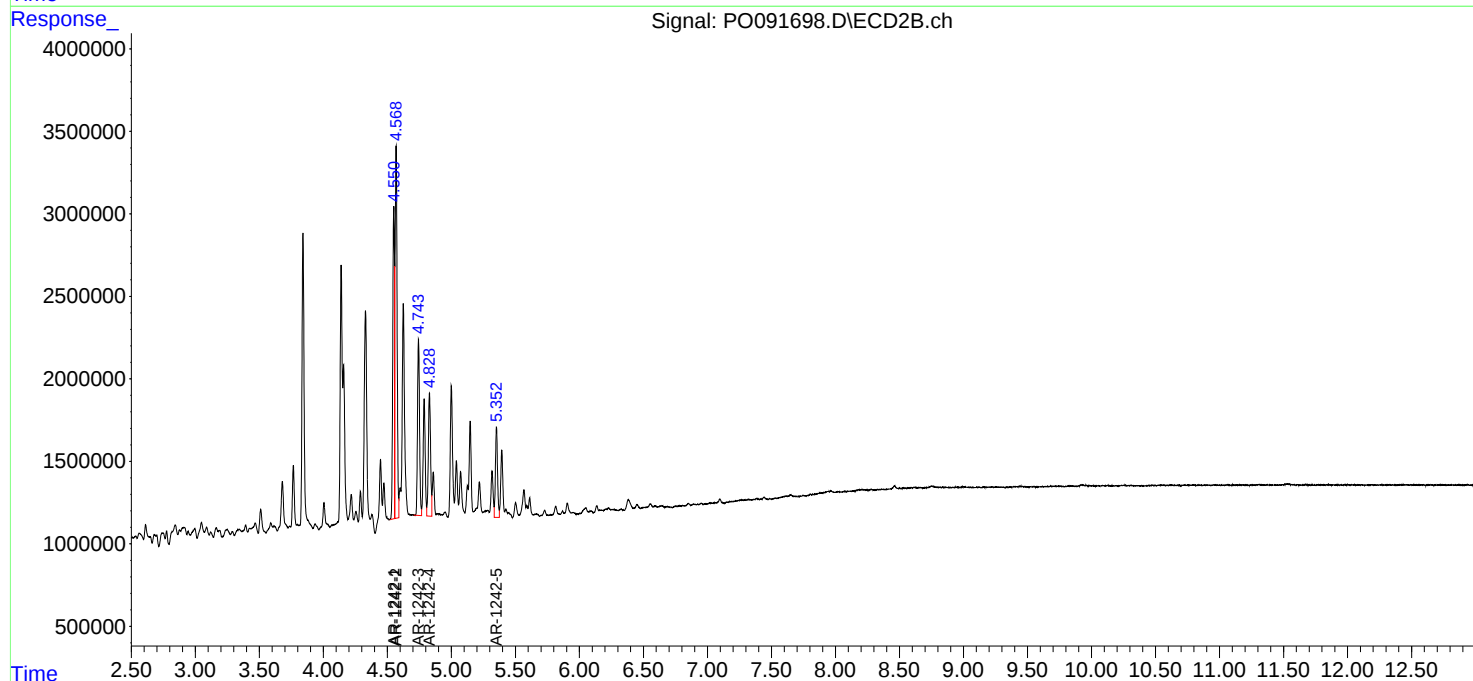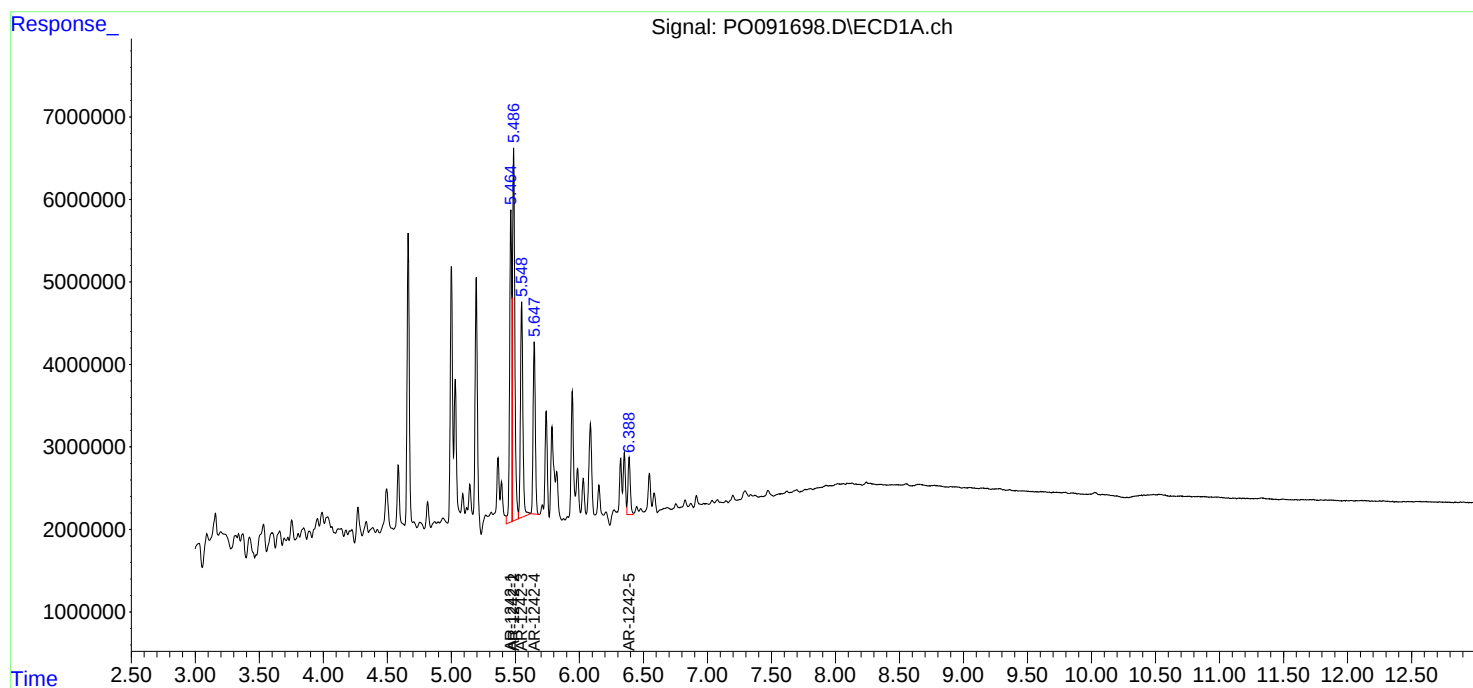

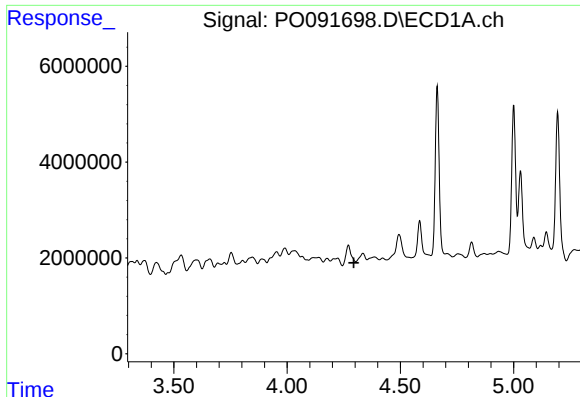


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.294 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
SB-6DL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/29/2022
Supervised By :Ankita Jodhani 12/29/2022

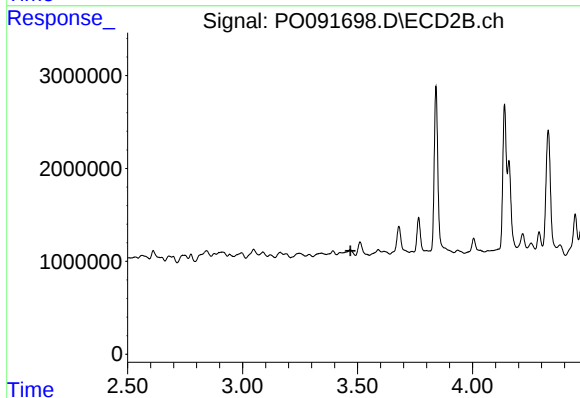


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.469 min
Response: 0
Conc: N.D.

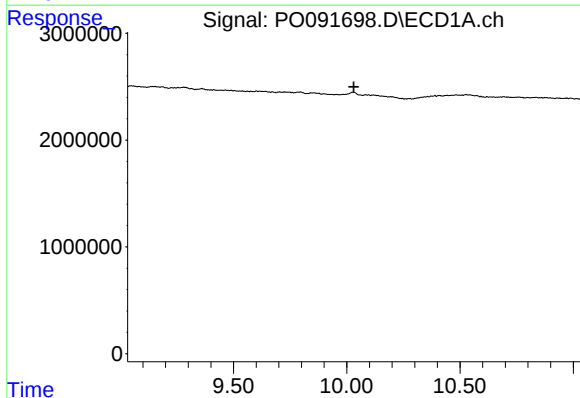


#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.032 min
Response: 0
Conc: N.D.

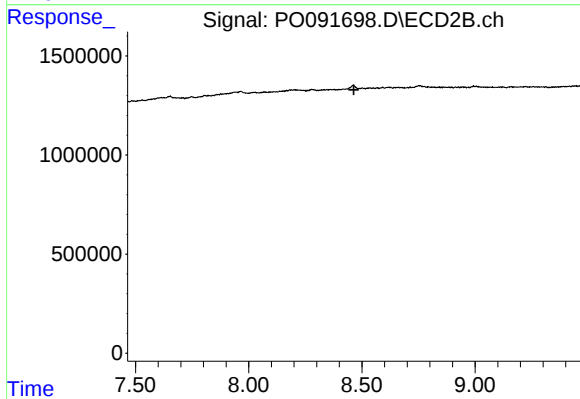

#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.465 min
Response: 0
Conc: N.D.

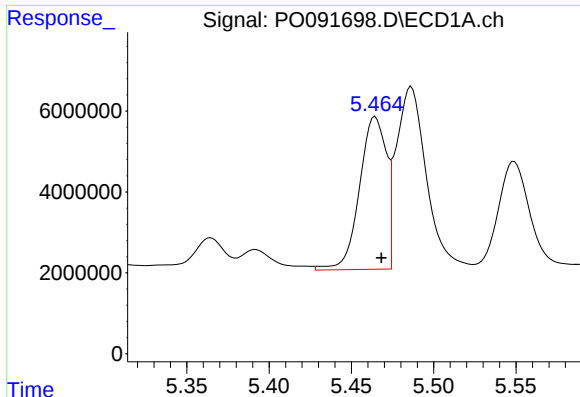


#16 AR-1242-1

R.T.: 5.465 min
Delta R.T.: -0.003 min
Response: 42817568
Conc: 589.61 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-6DL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/29/2022
Supervised By :Ankita Jodhani 12/29/2022

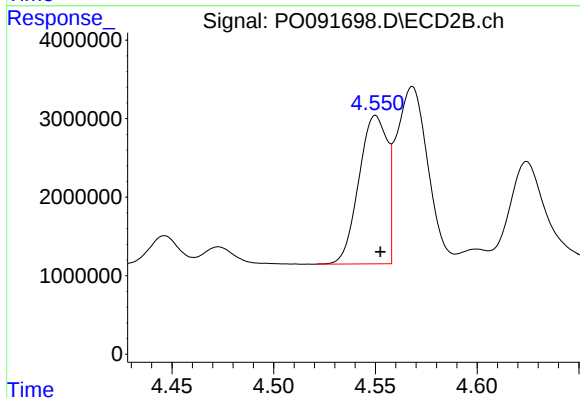


#16 AR-1242-1

R.T.: 4.550 min
Delta R.T.: -0.002 min
Response: 18341969
Conc: 664.28 ng/ml

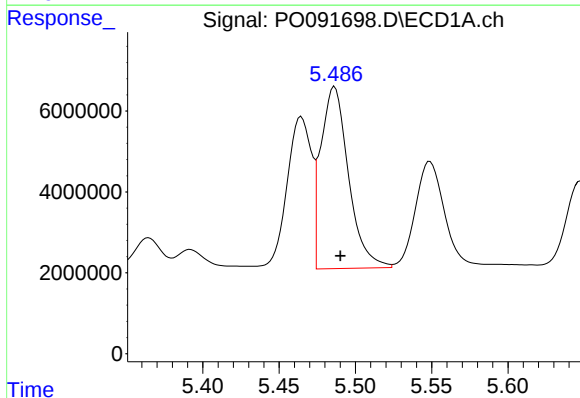


#17 AR-1242-2

R.T.: 5.486 min
Delta R.T.: -0.004 min
Response: 56905643
Conc: 549.25 ng/ml

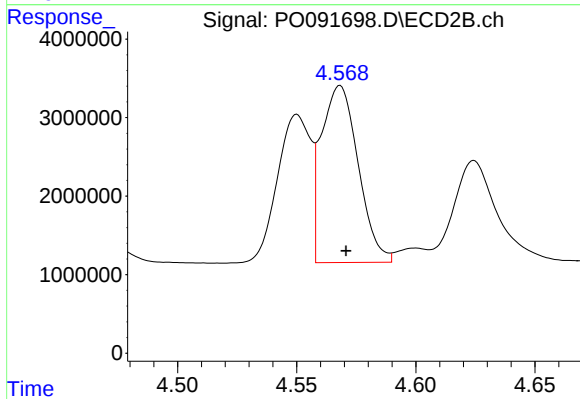

#17 AR-1242-2

R.T.: 4.568 min
Delta R.T.: -0.003 min
Response: 24281573
Conc: 626.42 ng/ml

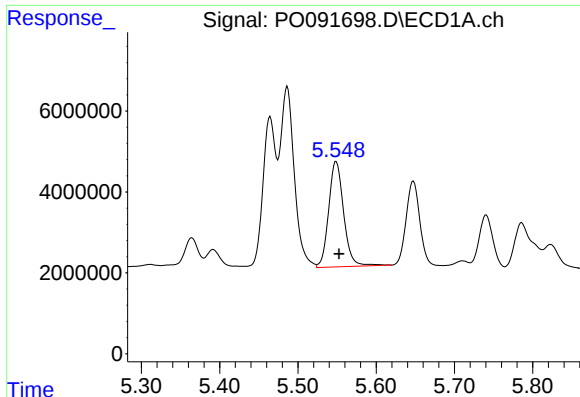


#18 AR-1242-3

R.T.: 5.549 min
Delta R.T.: -0.003 min
Response: 34813190
Conc: 537.42 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-6DL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/29/2022
Supervised By :Ankita Jodhani 12/29/2022

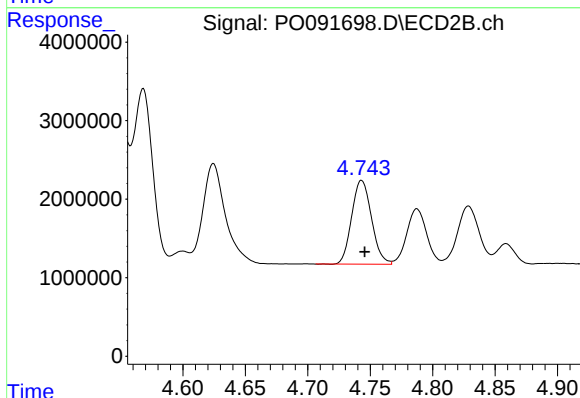


#18 AR-1242-3

R.T.: 4.743 min
Delta R.T.: -0.003 min
Response: 11808328
Conc: 566.98 ng/ml

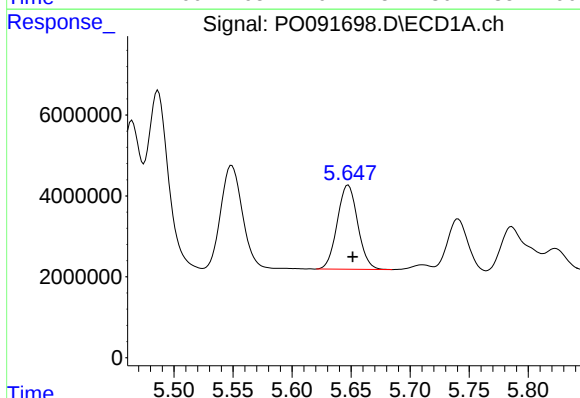


#19 AR-1242-4

R.T.: 5.648 min
Delta R.T.: -0.004 min
Response: 25087361
Conc: 503.50 ng/ml

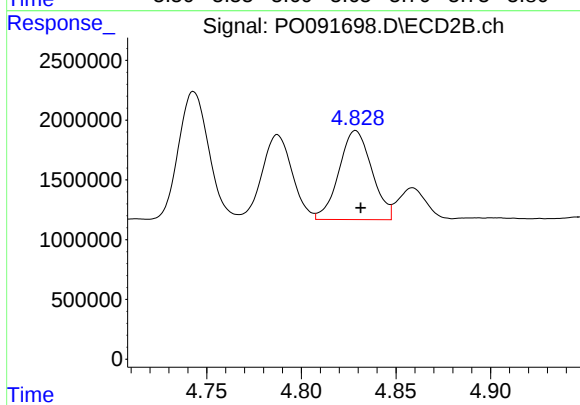

#19 AR-1242-4

R.T.: 4.829 min
Delta R.T.: -0.003 min
Response: 9015940
Conc: 410.20 ng/ml

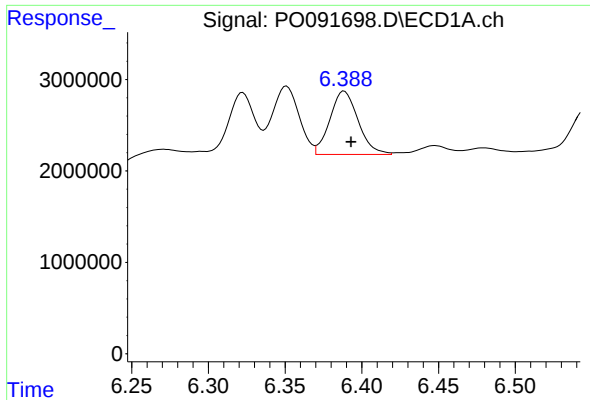


#20 AR-1242-5

R.T.: 6.388 min
Delta R.T.: -0.005 min
Response: 8874708
Conc: 169.68 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-6DL

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/29/2022
Supervised By :Ankita Jodhani 12/29/2022

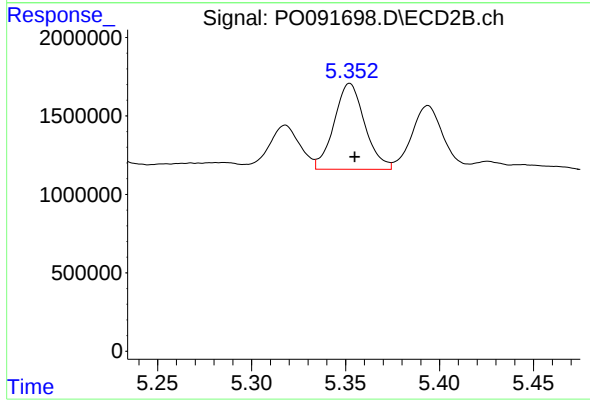

#20 AR-1242-5

R.T.: 5.352 min
Delta R.T.: -0.003 min
Response: 6230065
Conc: 233.00 ng/ml