

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0122823\
 Data File : P0100822.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Dec 2023 09:57
 Operator : YP/AJ
 Sample : 05977-07RE 10X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 34725RE

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/29/2023
 Supervised By :Ankita Jodhani 12/29/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 28 10:25:53 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0122023.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Dec 21 04:28:19 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.348	3.644	10395466	6395713	3.332	3.130
2) SA Decachlor...	10.094	8.707	6247527	4054940	2.991m	2.687

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122823\
Data File : PO100822.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Dec 2023 09:57
Operator : YP/AJ
Sample : 05977-07RE 10X
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
34725RE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/29/2023
Supervised By :Ankita Jodhani 12/29/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 28 10:25:53 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO122023.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Dec 21 04:28:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

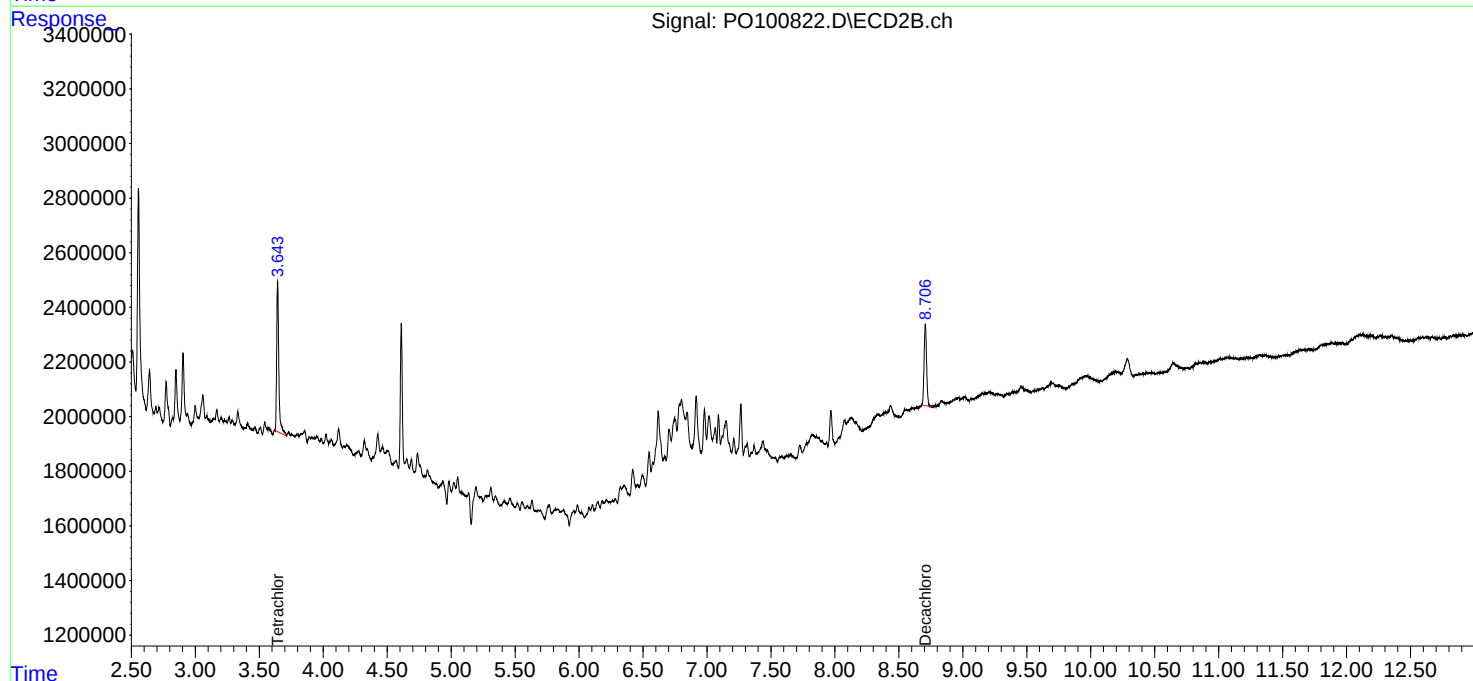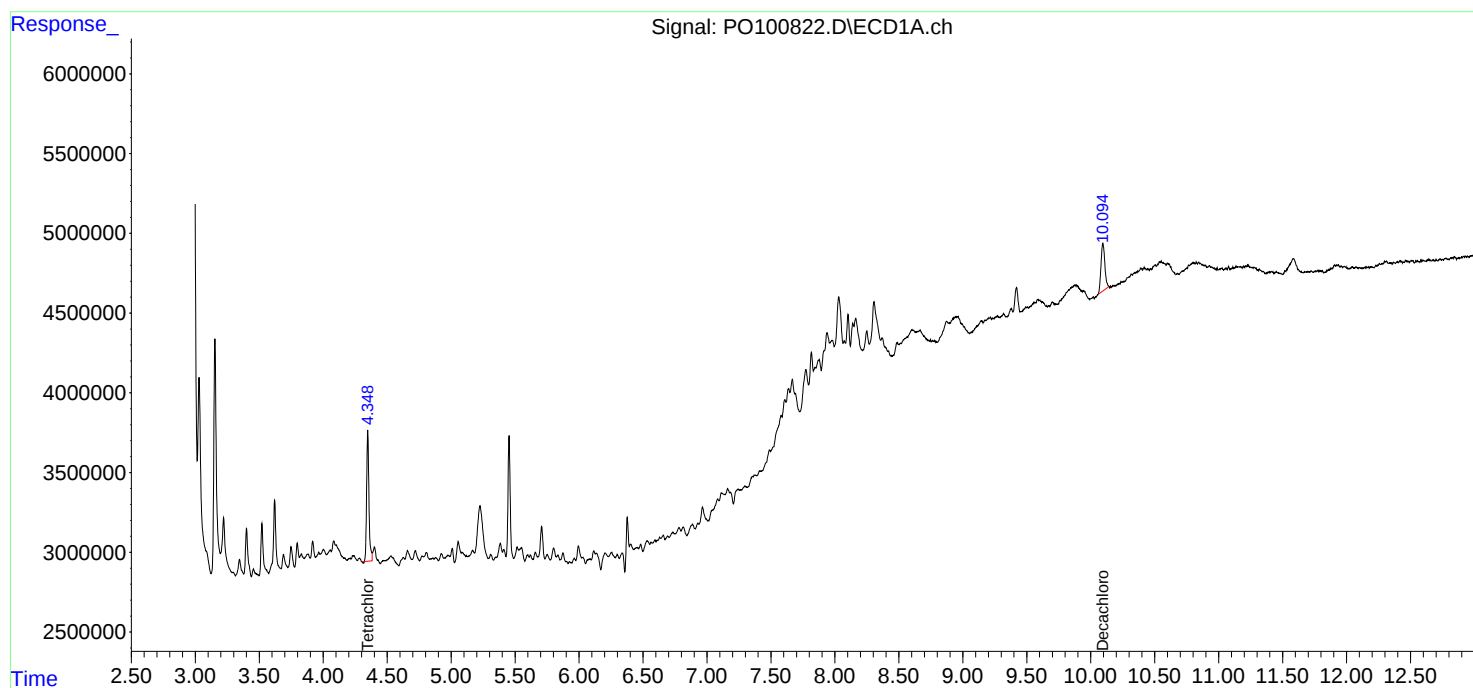

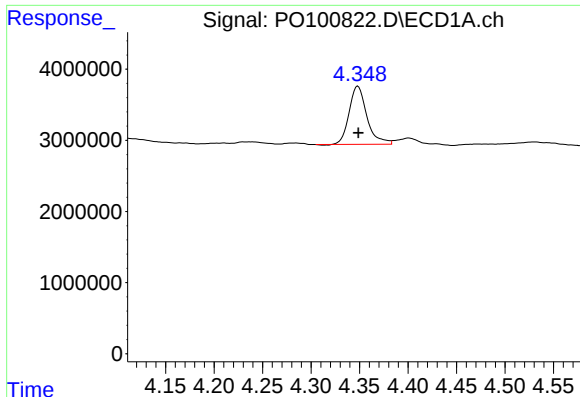

#1 Tetrachloro-m-xylene

R.T.: 4.348 min
Delta R.T.: 0.000 min
Response: 10395466
Conc: 3.33 ng/ml


Instrument :

ECD_O

ClientSampleId :
34725RE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/29/2023
Supervised By :Ankita Jodhani 12/29/2023

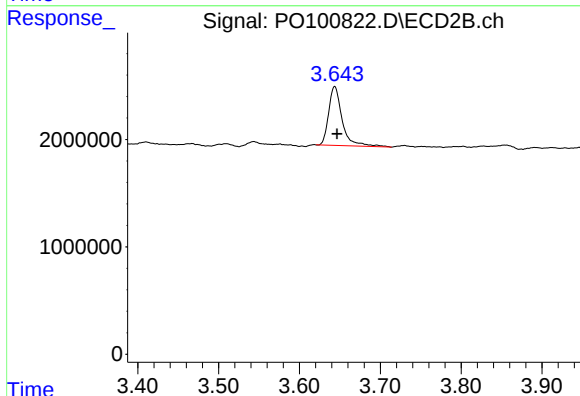


#1 Tetrachloro-m-xylene

R.T.: 3.644 min
Delta R.T.: -0.003 min
Response: 6395713
Conc: 3.13 ng/ml

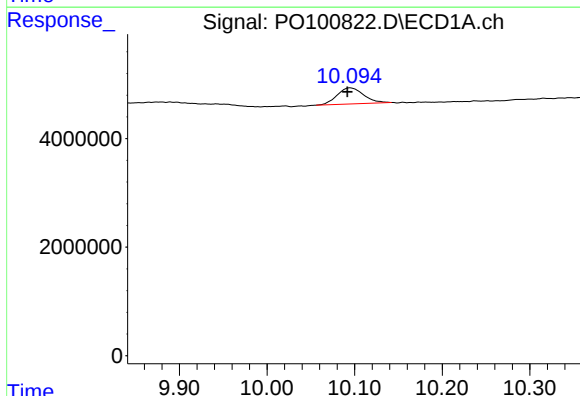

#2 Decachlorobiphenyl

R.T.: 10.094 min
Delta R.T.: 0.002 min
Response: 6247527
Conc: 2.99 ng/ml m

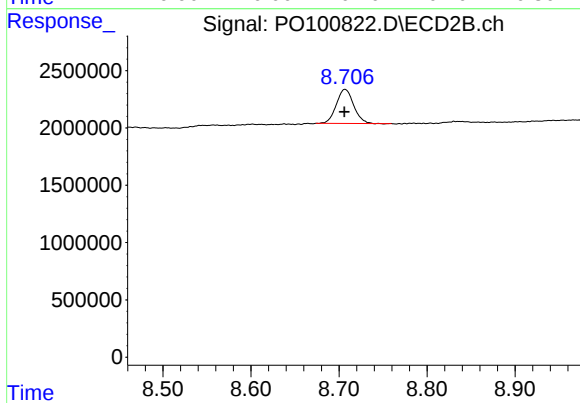

#2 Decachlorobiphenyl

R.T.: 8.707 min
Delta R.T.: 0.001 min
Response: 4054940
Conc: 2.69 ng/ml