

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122918\
 Data File : PO053077.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Dec 2018 00:44
 Operator : SM/SJ
 Sample : J6571-10
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 50081

Manual Integrations
 APPROVED

Sohil
 1/2/2019 12:01:16 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 29 01:32:34 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO122818.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 28 04:30:51 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.189	3.223	9552383	2075165	9.846m	10.687
2) SA Decachlor...	9.664	7.865	10192532	3620269	16.525	16.787

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122918\
Data File : PO053077.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Dec 2018 00:44
Operator : SM/SJ
Sample : J6571-10
Misc :
ALS Vial : 39 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
50081


Manual Integrations
APPROVED

Sohil
1/2/2019 12:01:16 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 29 01:32:34 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO122818.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 28 04:30:51 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

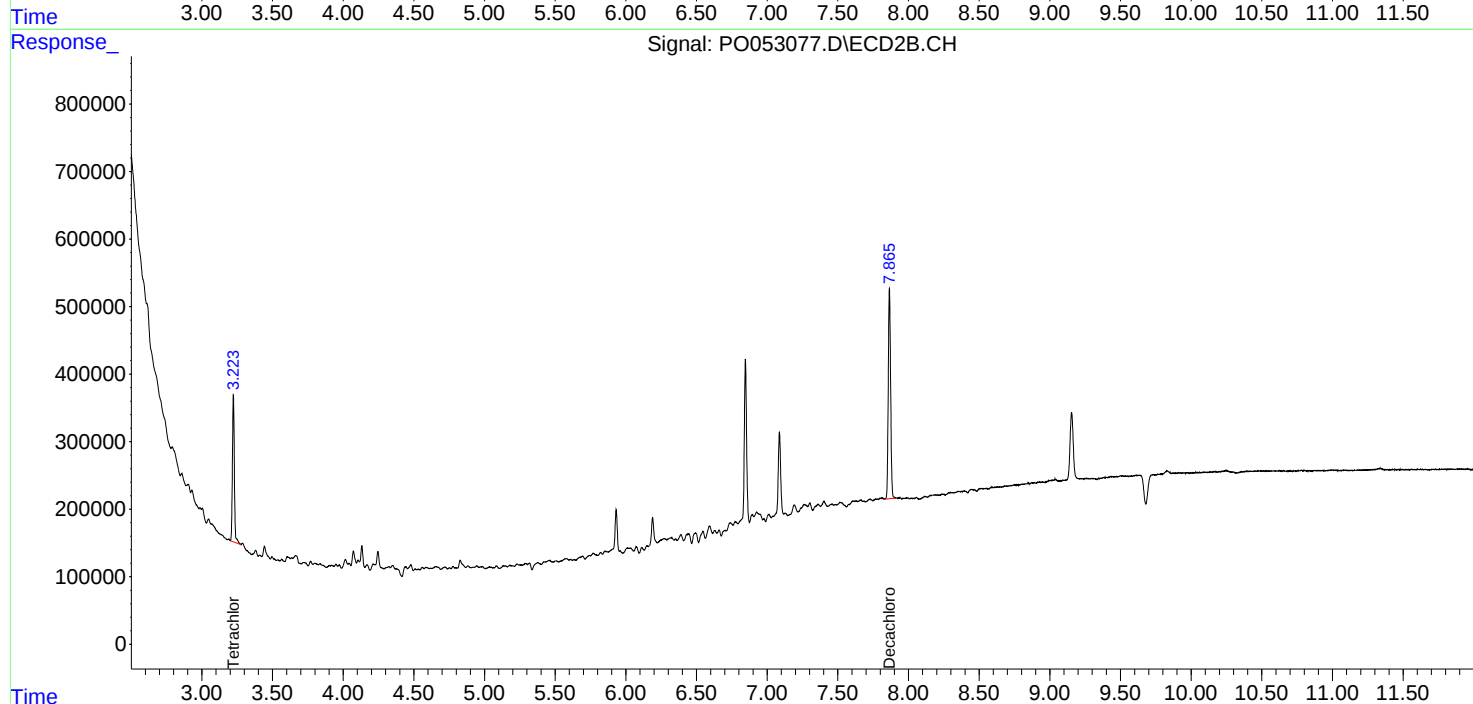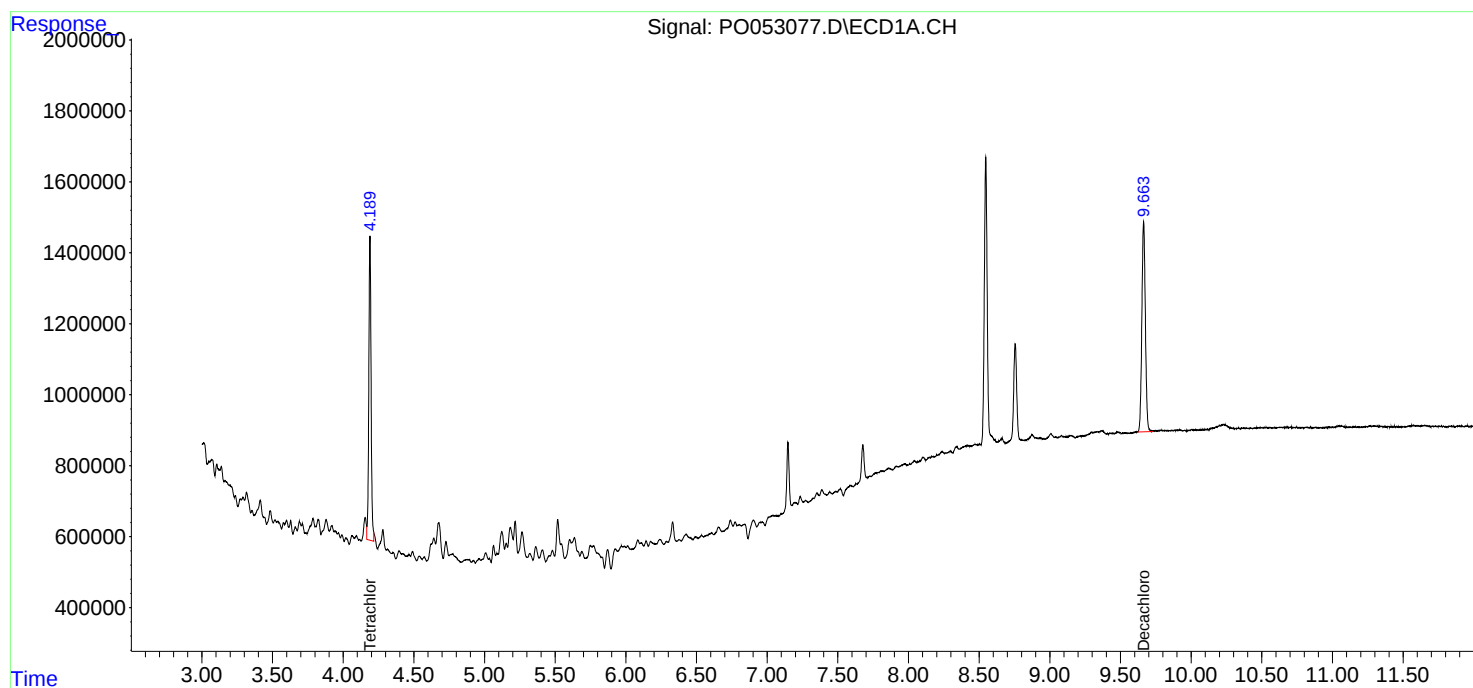

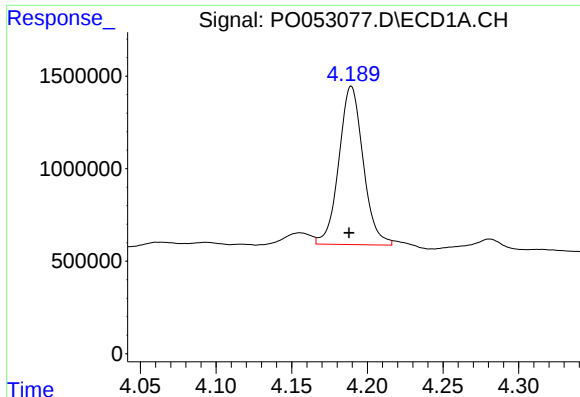


#1 Tetrachloro-m-xylene

R.T.: 4.189 min
Delta R.T.: 0.000 min
Response: 9552383
Conc: 9.85 ng/ml m

Instrument :
ECD_O
ClientSampleId :
50081


Manual Integrations
APPROVED

Sohil
1/2/2019 12:01:16 PM

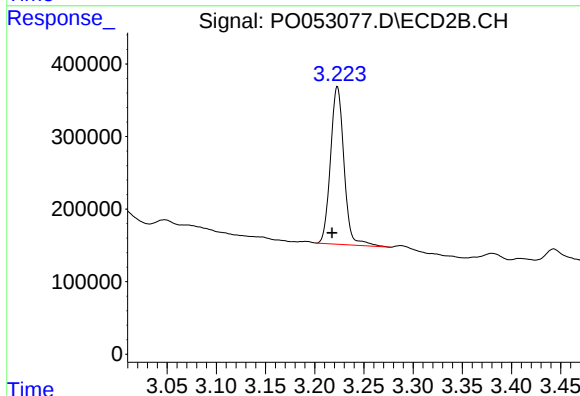


#1 Tetrachloro-m-xylene

R.T.: 3.223 min
Delta R.T.: 0.006 min
Response: 2075165
Conc: 10.69 ng/ml

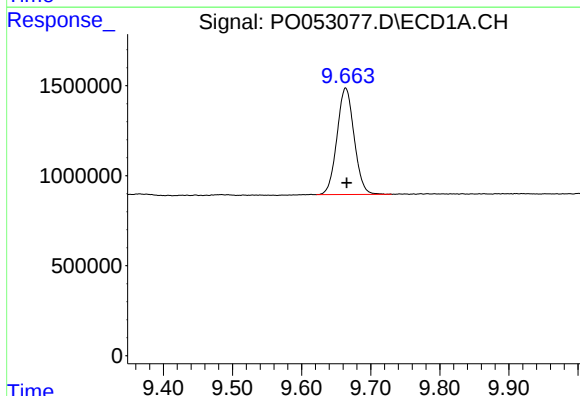

#2 Decachlorobiphenyl

R.T.: 9.664 min
Delta R.T.: -0.001 min
Response: 10192532
Conc: 16.53 ng/ml

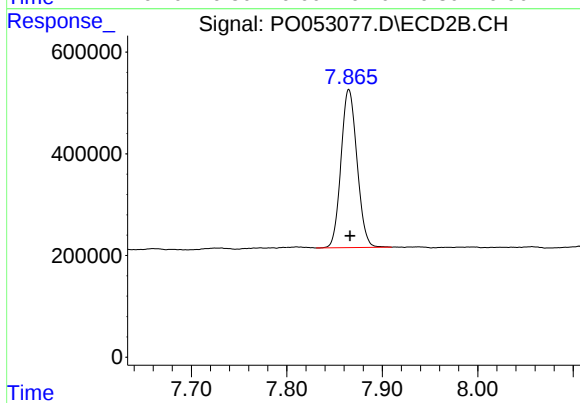

#2 Decachlorobiphenyl

R.T.: 7.865 min
Delta R.T.: -0.001 min
Response: 3620269
Conc: 16.79 ng/ml