

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122918\
 Data File : P0053088.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Dec 2018 3:51
 Operator : SM/SJ
 Sample : J6193-13
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CL-02-122718-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 29 04:57:43 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO122818.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 28 04:30:51 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.186	3.217	32232425	5010623	33.224	25.805
2) SA Decachlor...	9.663	7.866	10436421	2992046	16.921	13.874

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122918\
Data File : P0053088.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Dec 2018 3:51
Operator : SM/SJ
Sample : J6193-13
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CL-02-122718-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 29 04:57:43 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO122818.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 28 04:30:51 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

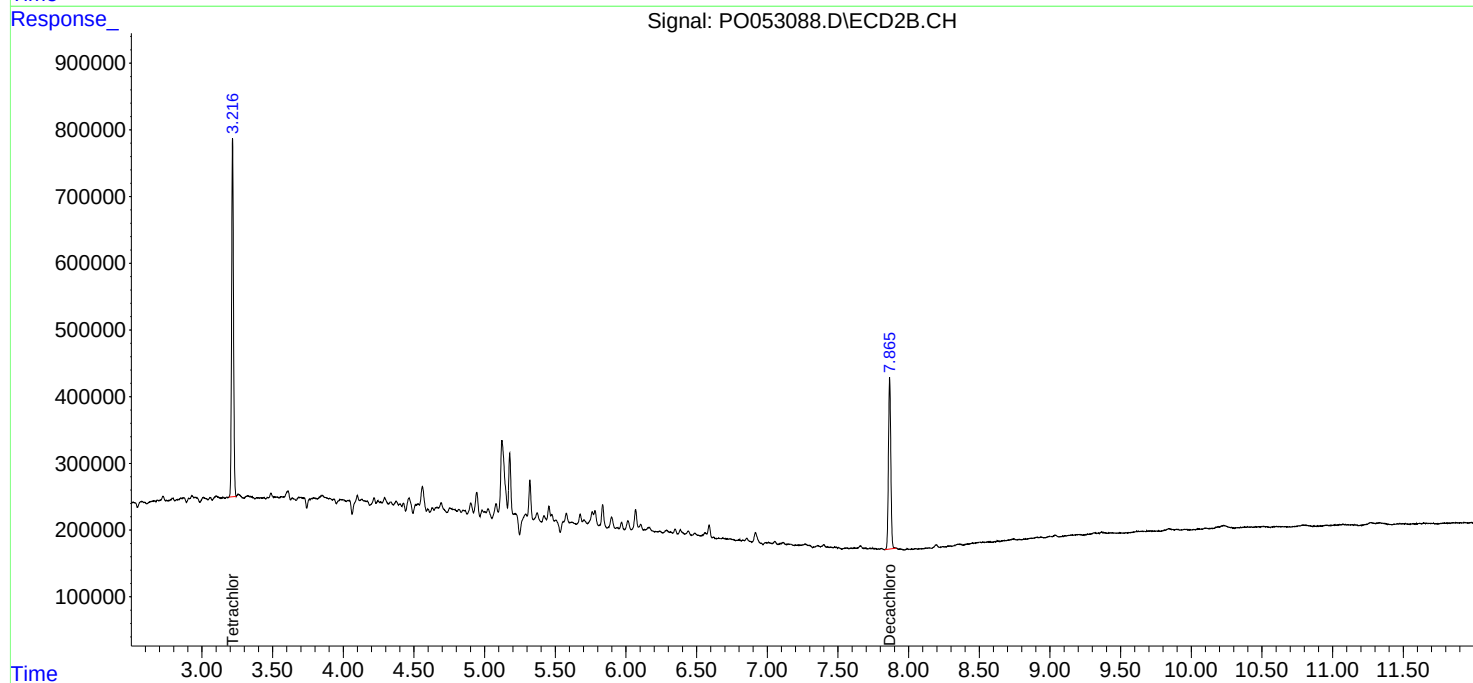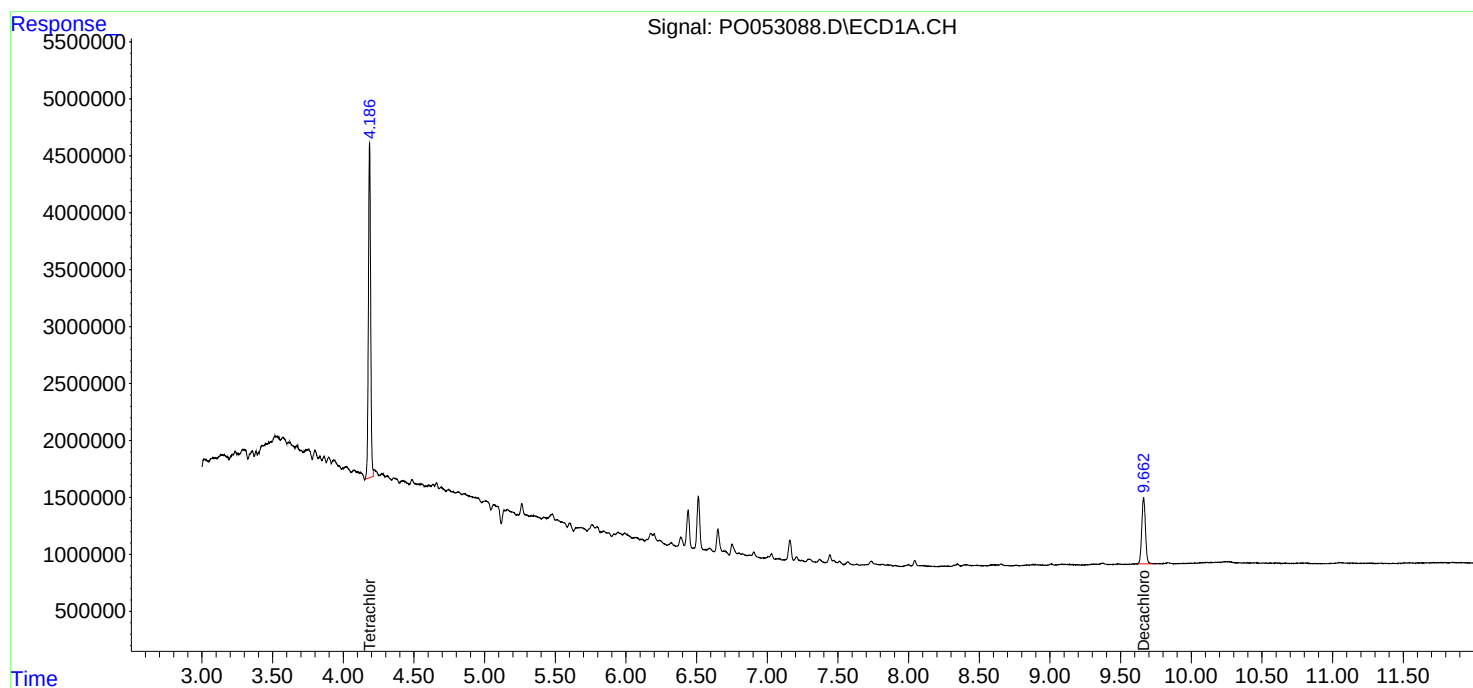


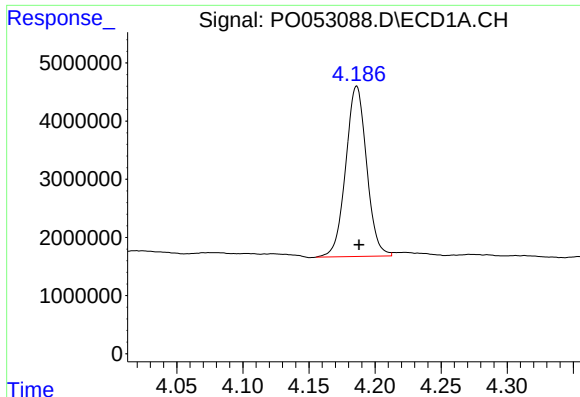

#1 Tetrachloro-m-xylene


R.T.: 4.186 min
Delta R.T.: -0.002 min
Response: 32232425
Conc: 33.22 ng/ml

Instrument :
ECD_O
ClientSampleId :
CL-02-122718-B

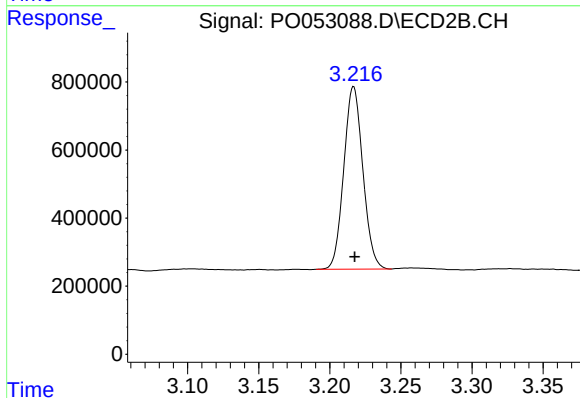


#1 Tetrachloro-m-xylene

R.T.: 3.217 min
Delta R.T.: 0.000 min
Response: 5010623
Conc: 25.80 ng/ml

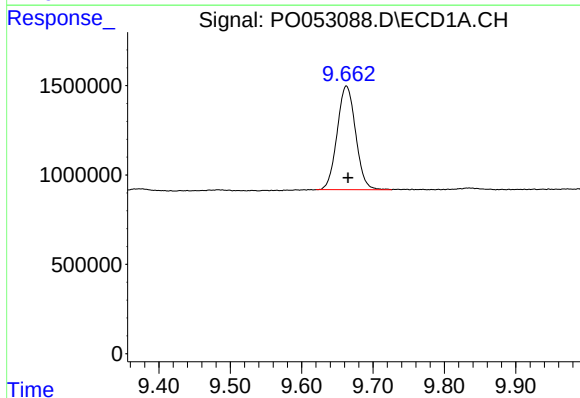

#2 Decachlorobiphenyl

R.T.: 9.663 min
Delta R.T.: -0.002 min
Response: 10436421
Conc: 16.92 ng/ml

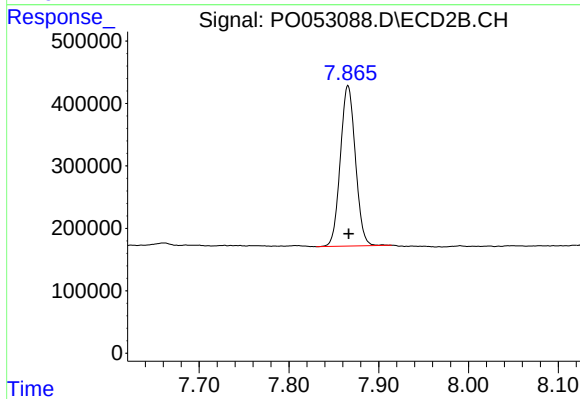

#2 Decachlorobiphenyl

R.T.: 7.866 min
Delta R.T.: 0.000 min
Response: 2992046
Conc: 13.87 ng/ml