

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0122920\
 Data File : P0074263.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Dec 2020 9:43
 Operator : DD\AJ
 Sample : PB133816BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 29 13:12:09 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0122320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Dec 24 01:16:32 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.932	3.989	2196235	1206614	21.540	21.032
2)	SA Decachlor...	10.949	9.247	2184901	1250967	22.435	23.269
Target Compounds							
20)	L4 AR-1242-5	0.000	6.125f	0	545617	N.D.	346.740 #
24)	L5 AR-1248-4	7.174f	0.000	1132063	0	282.079	N.D. #
25)	L5 AR-1248-5	0.000	6.125f	0	545617	N.D.	237.372 #
26)	L6 AR-1254-1	7.174	6.125f	1132063	545617	293.251	157.751 #
28)	L6 AR-1254-3	7.800f	0.000	577074	0	96.059	N.D. #
33)	L7 AR-1260-3	0.000	7.185f	0	53483	N.D.	13.650 #
38)	L8 AR-1262-3	0.000	8.166	0	536555	N.D.	148.970 #
41)	L9 AR-1268-1	0.000	8.166	0	536555	N.D.	50.491 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122920\
Data File : PO074263.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Dec 2020 9:43
Operator : DD\AJ
Sample : PB133816BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 29 13:12:09 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO122320.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Dec 24 01:16:32 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

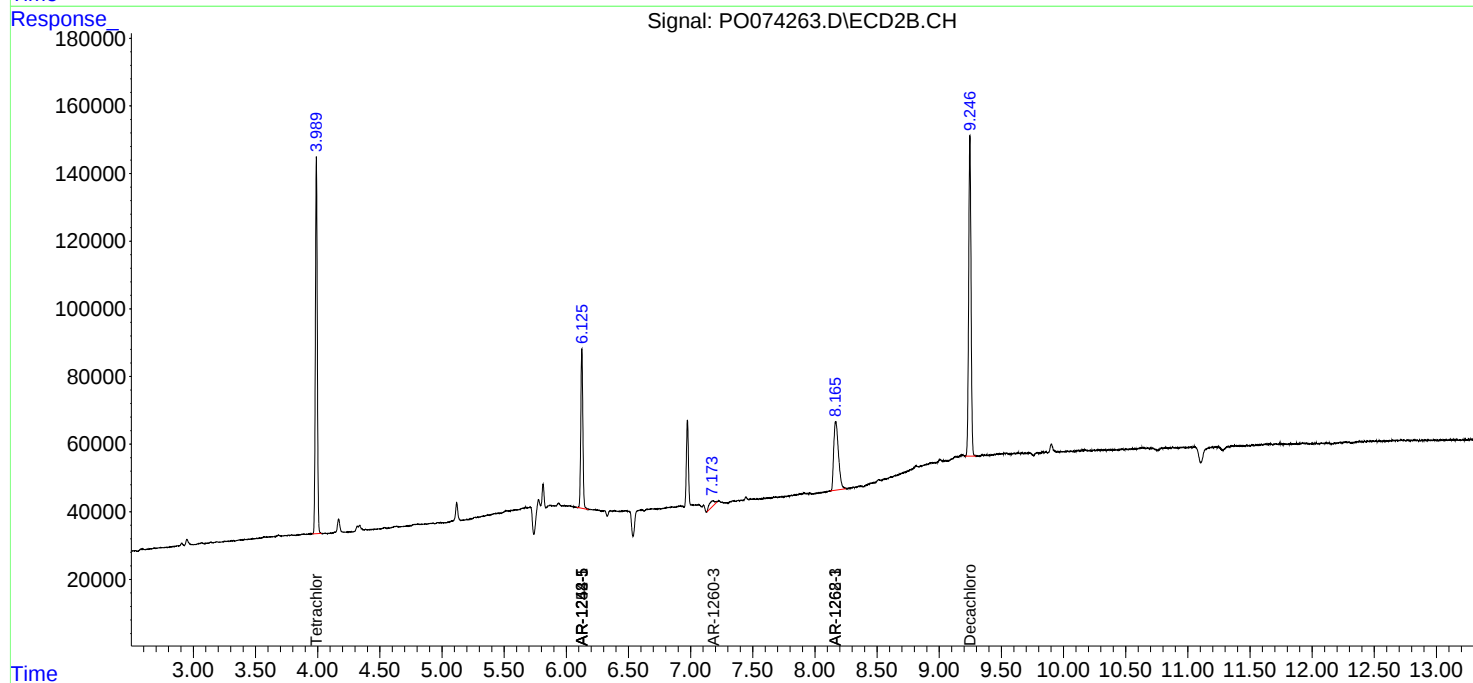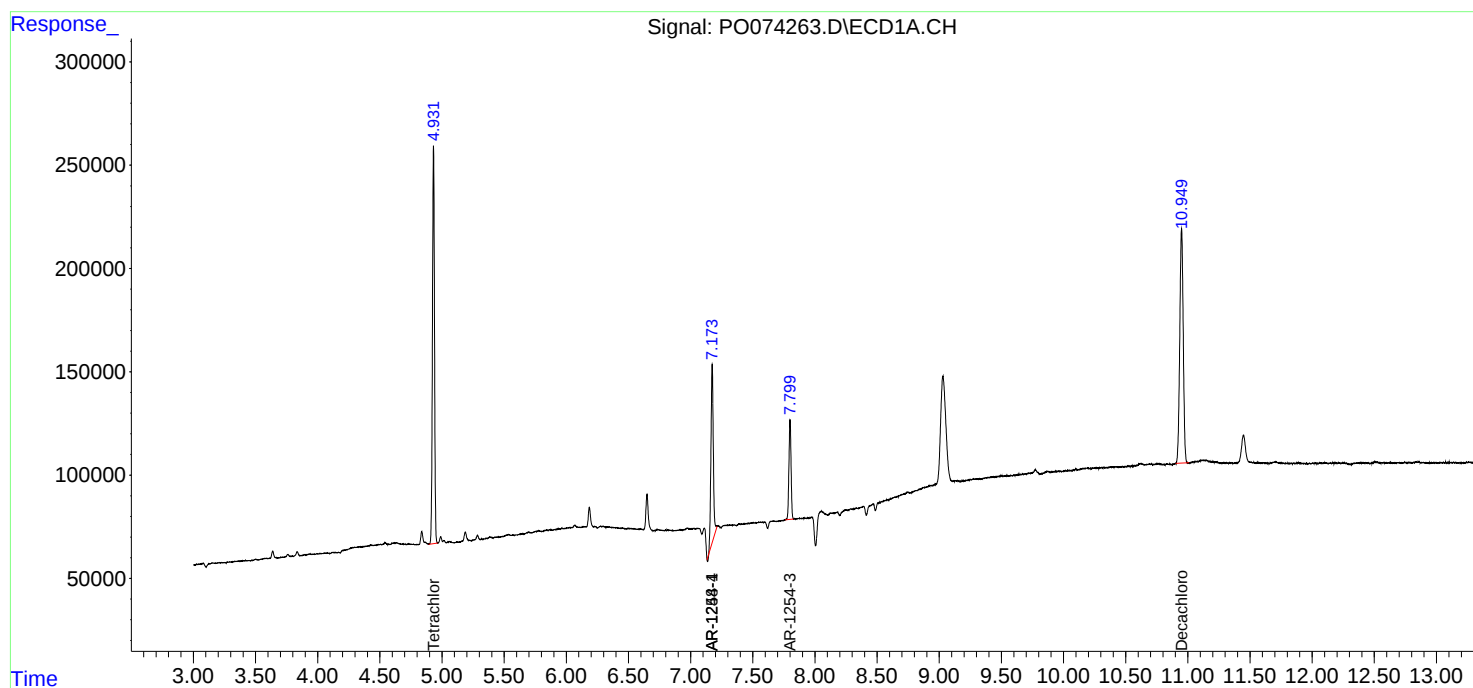


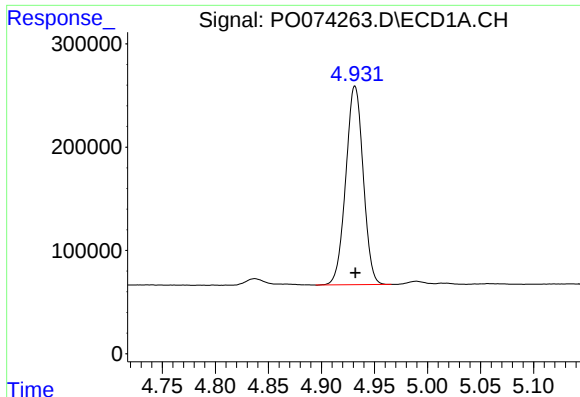

#1 Tetrachloro-m-xylene


R.T.: 4.932 min
Delta R.T.: 0.000 min
Response: 2196235
Conc: 21.54 ng/ml

Instrument :
ECD_O
ClientSampleId :

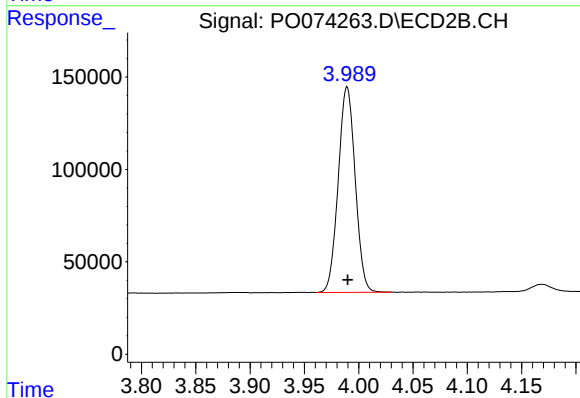


#1 Tetrachloro-m-xylene

R.T.: 3.989 min
Delta R.T.: 0.000 min
Response: 1206614
Conc: 21.03 ng/ml

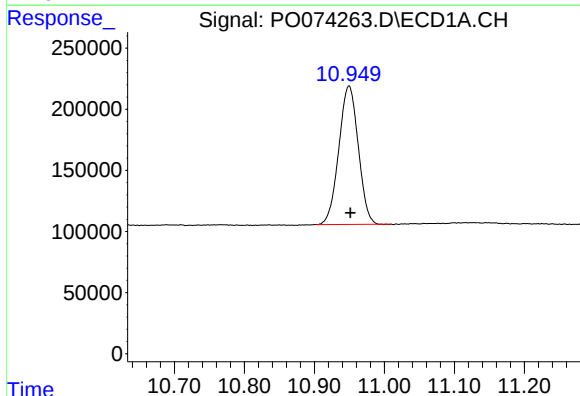


#2 Decachlorobiphenyl

R.T.: 10.949 min
Delta R.T.: -0.002 min
Response: 2184901
Conc: 22.44 ng/ml

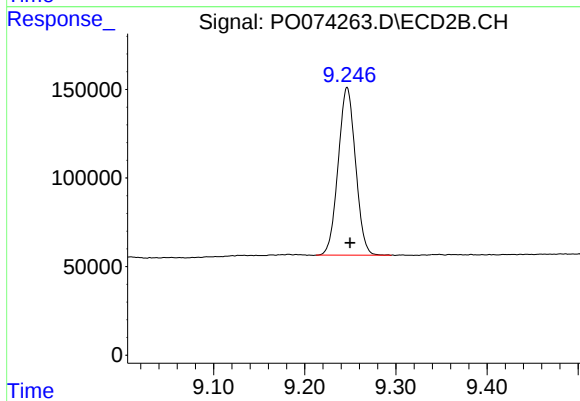

#2 Decachlorobiphenyl


R.T.: 9.247 min
Delta R.T.: -0.003 min
Response: 1250967
Conc: 23.27 ng/ml

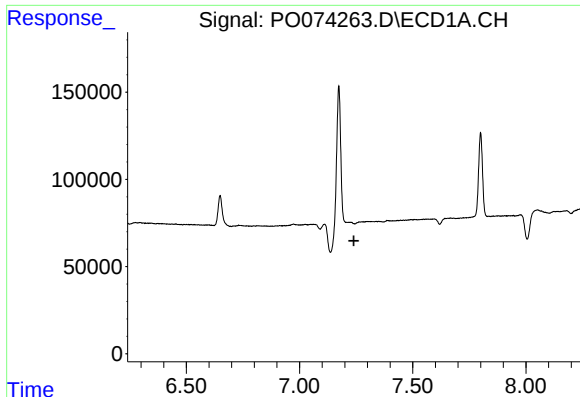

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T.: 7.240 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

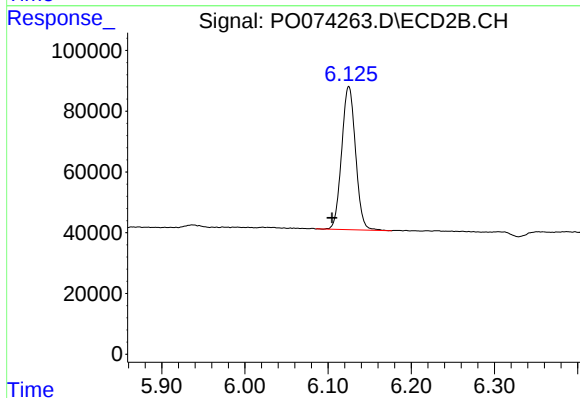


#20 AR-1242-5

R.T.: 6.125 min
Delta R.T.: 0.020 min
Response: 545617
Conc: 346.74 ng/ml

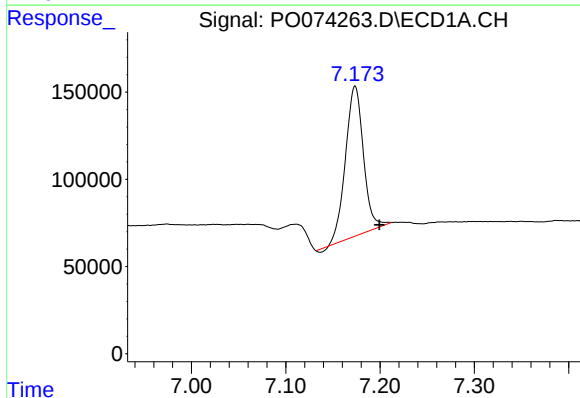


#24 AR-1248-4

R.T.: 7.174 min
Delta R.T.: -0.026 min
Response: 1132063
Conc: 282.08 ng/ml

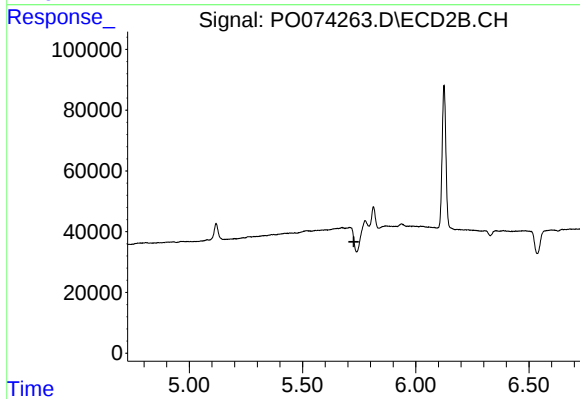

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T.: 5.727 min
Response: 0
Conc: N.D.

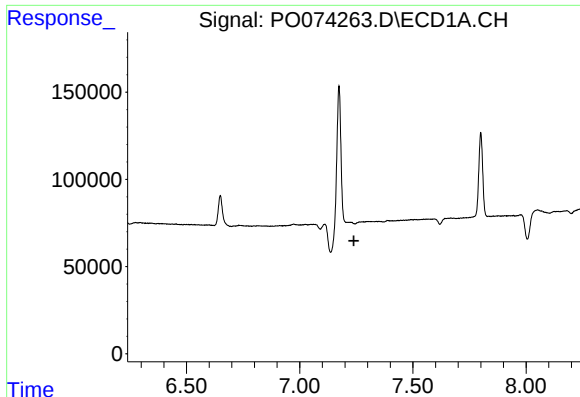

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T.: 7.239 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

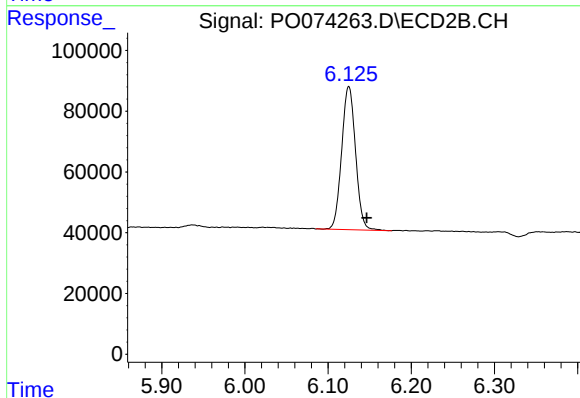


#25 AR-1248-5

R.T.: 6.125 min
Delta R.T.: -0.021 min
Response: 545617
Conc: 237.37 ng/ml

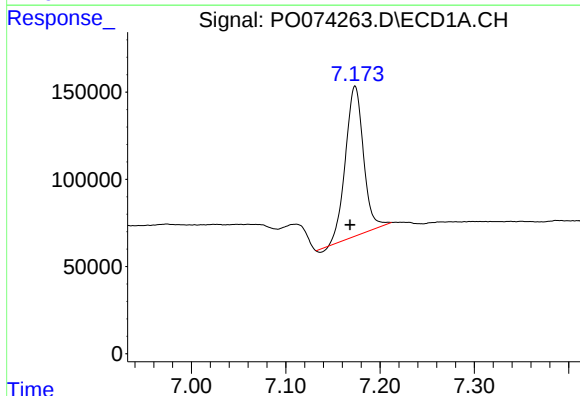


#26 AR-1254-1

R.T.: 7.174 min
Delta R.T.: 0.005 min
Response: 1132063
Conc: 293.25 ng/ml

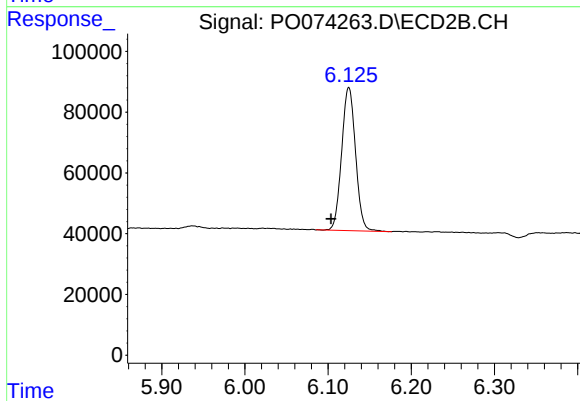

#26 AR-1254-1


R.T.: 6.125 min
Delta R.T.: 0.021 min
Response: 545617
Conc: 157.75 ng/ml

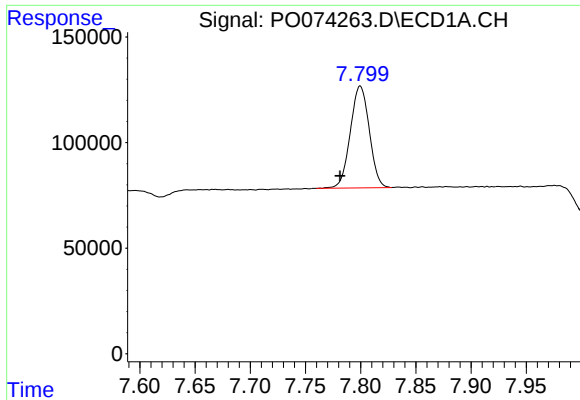

#28 AR-1254-3


R.T.: 7.800 min
Delta R.T.: 0.018 min
Response: 577074
Conc: 96.06 ng/ml

Instrument :
ECD_O
ClientSampleId :

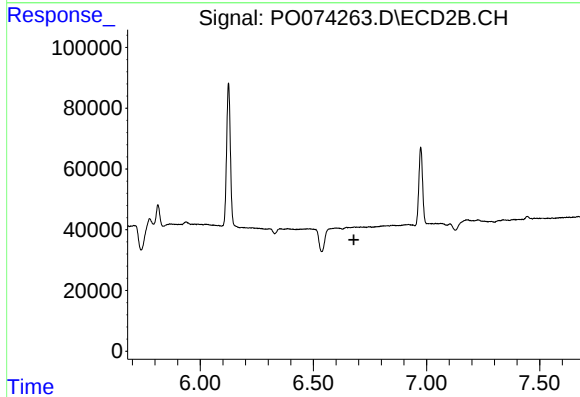


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.679 min
Response: 0
Conc: N.D.

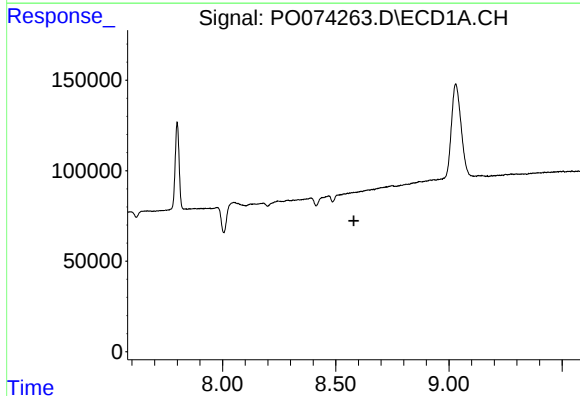


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 8.580 min
Response: 0
Conc: N.D.

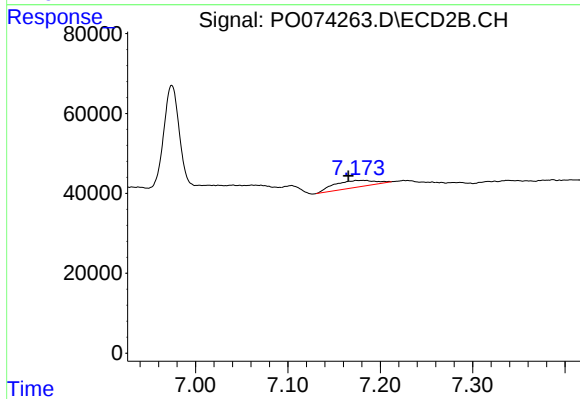

#33 AR-1260-3


R.T.: 7.185 min
Delta R.T.: 0.020 min
Response: 53483
Conc: 13.65 ng/ml

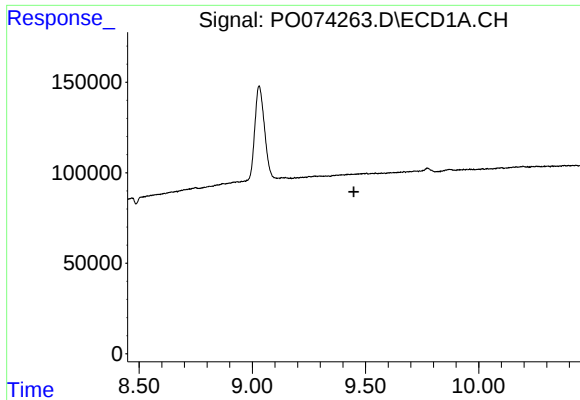

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T. : 9.449 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

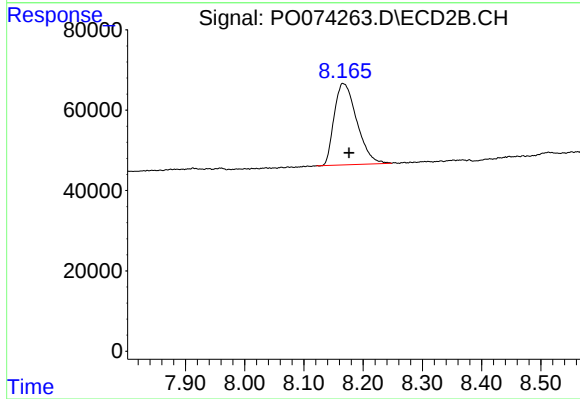


#38 AR-1262-3

R.T.: 8.166 min
Delta R.T.: -0.010 min
Response: 536555
Conc: 148.97 ng/ml

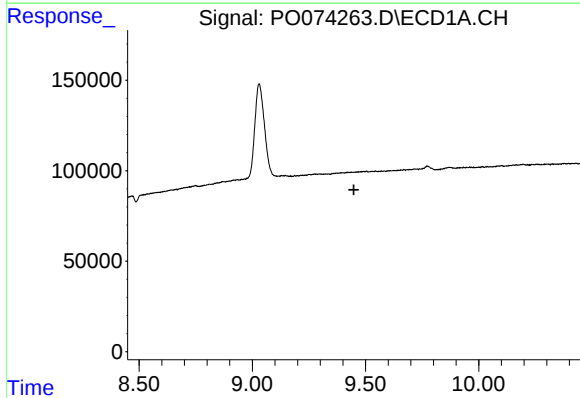

#41 AR-1268-1

R.T.: 0.000 min
Exp R.T. : 9.448 min
Response: 0
Conc: N.D.

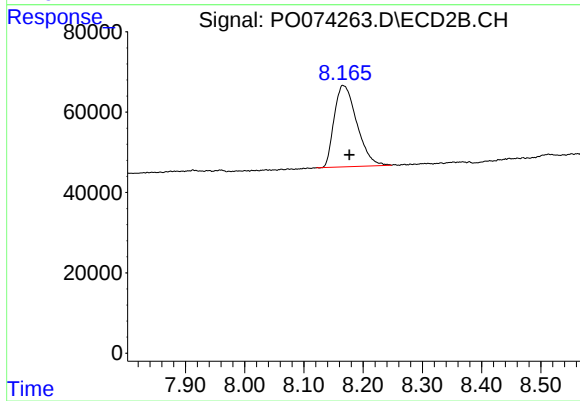

#41 AR-1268-1

R.T.: 8.166 min
Delta R.T.: -0.011 min
Response: 536555
Conc: 50.49 ng/ml