

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO122922\
 Data File : PO091727.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Dec 2022 10:21
 Operator : YP/AJ
 Sample : N6218-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 CHRT-26223

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/30/2022
 Supervised By :Ankita Jodhani 12/30/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 29 22:10:26 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO122122.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Dec 22 03:53:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.289	3.466	45900742	19646376	16.895	19.374
2) SA Decachlor...	10.024	8.459	29375604	15567696	15.611	17.844
Target Compounds						
31) L7 AR-1260-1	7.076	6.035	7335107	2985460	65.053	56.498m
32) L7 AR-1260-2	7.331	6.225	17439280	1742161	127.398	27.255m#
33) L7 AR-1260-3	7.698	6.378	4739853	3568710	58.031	53.432
34) L7 AR-1260-4	7.923	6.851	5466739	2655319	52.988m	62.725
35) L7 AR-1260-5	8.240	7.095	8514072	5165850	45.147	53.180

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122922\
Data File : PO091727.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Dec 2022 10:21
Operator : YP/AJ
Sample : N6218-03
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
CHRT-26223


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/30/2022
Supervised By :Ankita Jodhani 12/30/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 29 22:10:26 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO122122.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Dec 22 03:53:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

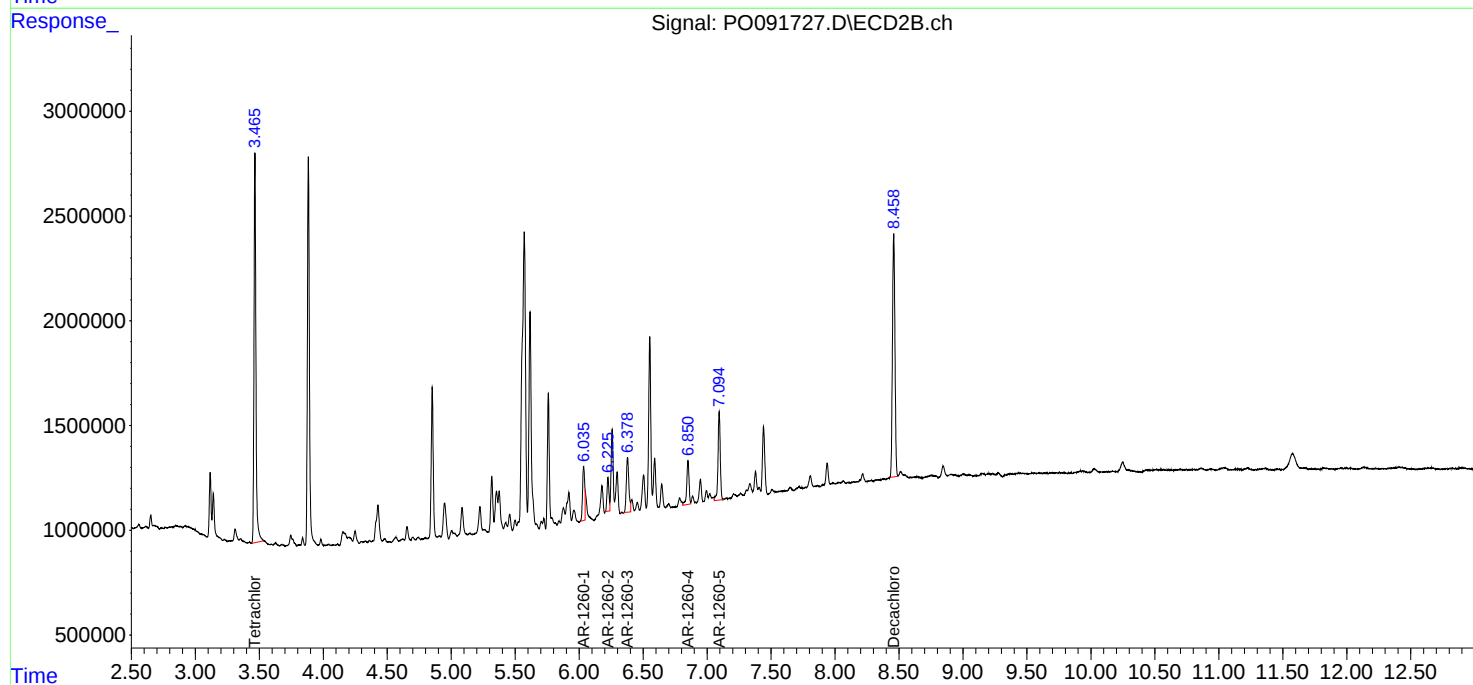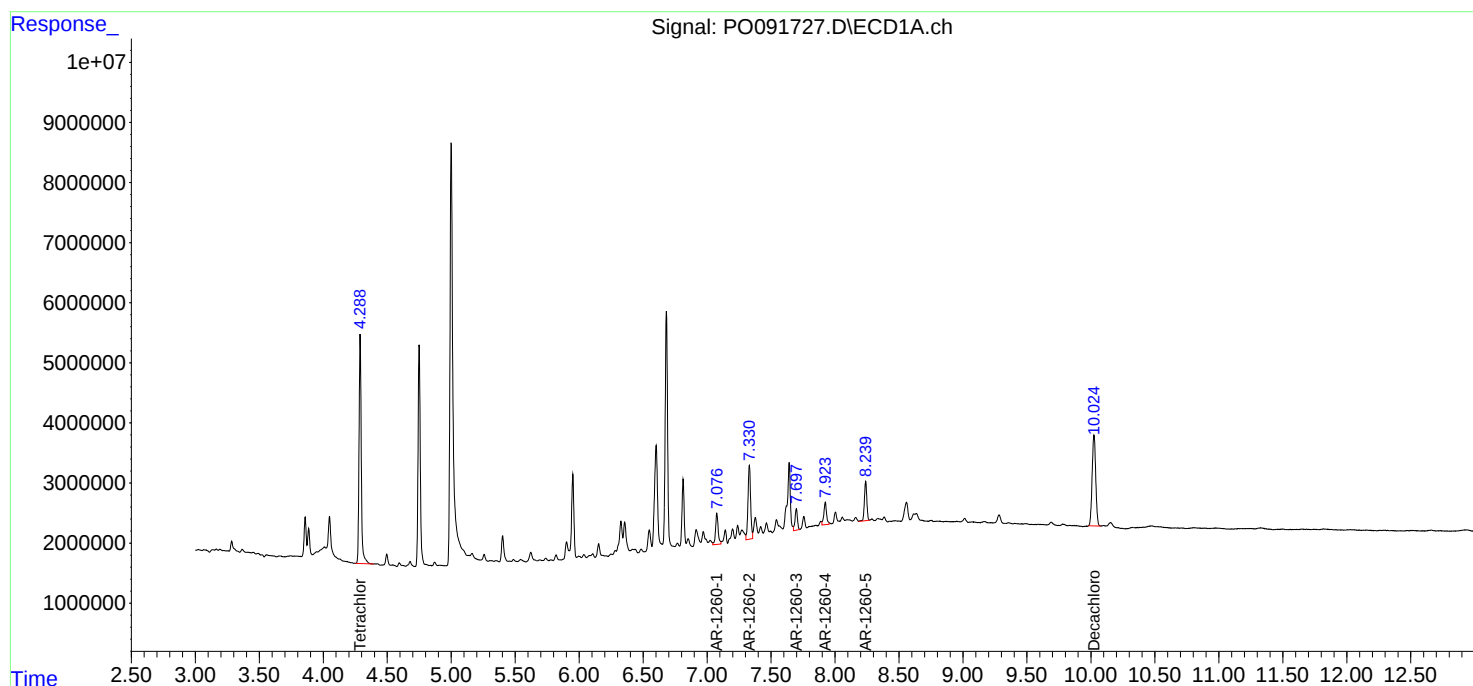

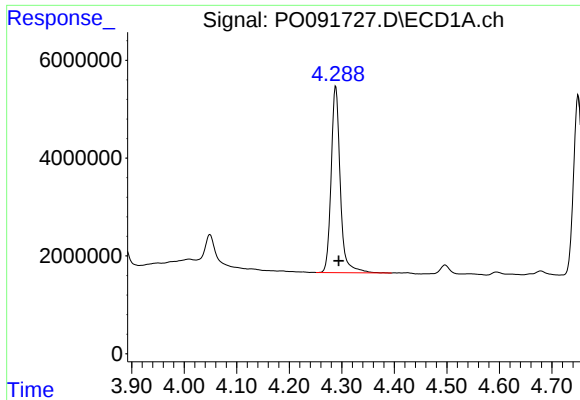


#1 Tetrachloro-m-xylene

R.T.: 4.289 min
Delta R.T.: -0.005 min
Response: 45900742
Conc: 16.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
CHRT-26223


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/30/2022
Supervised By :Ankita Jodhani 12/30/2022

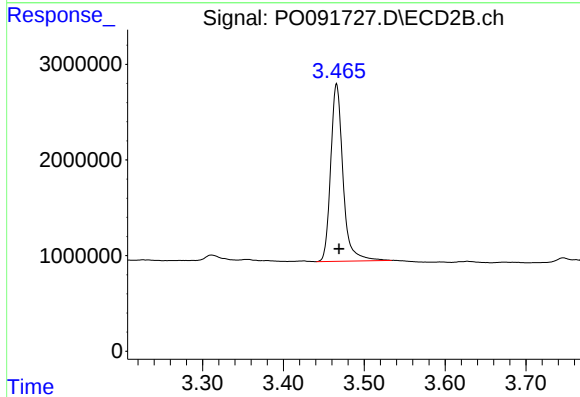


#1 Tetrachloro-m-xylene

R.T.: 3.466 min
Delta R.T.: -0.003 min
Response: 19646376
Conc: 19.37 ng/ml

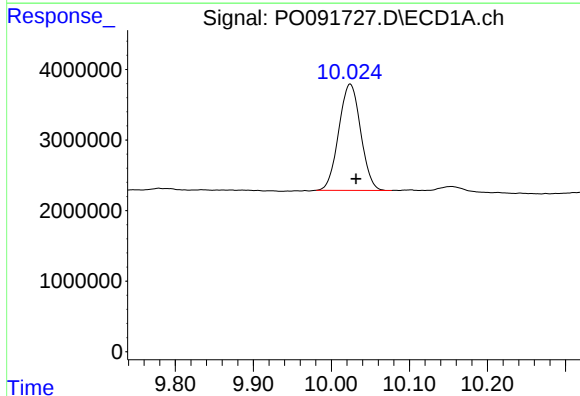


#2 Decachlorobiphenyl

R.T.: 10.024 min
Delta R.T.: -0.007 min
Response: 29375604
Conc: 15.61 ng/ml

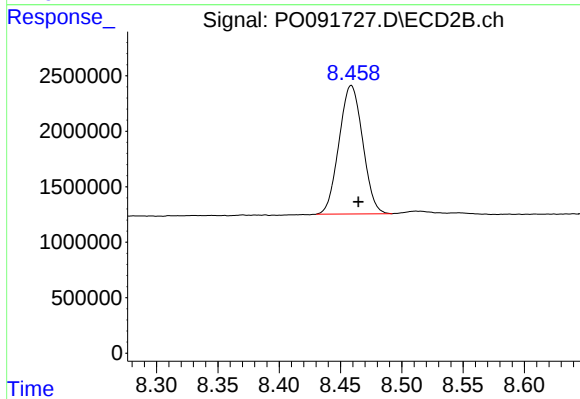

#2 Decachlorobiphenyl

R.T.: 8.459 min
Delta R.T.: -0.006 min
Response: 15567696
Conc: 17.84 ng/ml

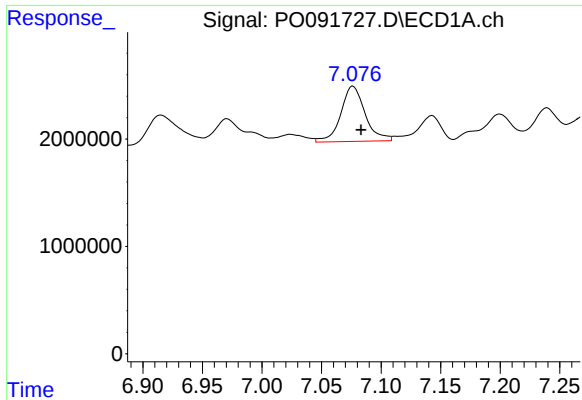


#31 AR-1260-1

R.T.: 7.076 min
Delta R.T.: -0.007 min
Response: 7335107
Conc: 65.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
CHRT-26223


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/30/2022
Supervised By :Ankita Jodhani 12/30/2022

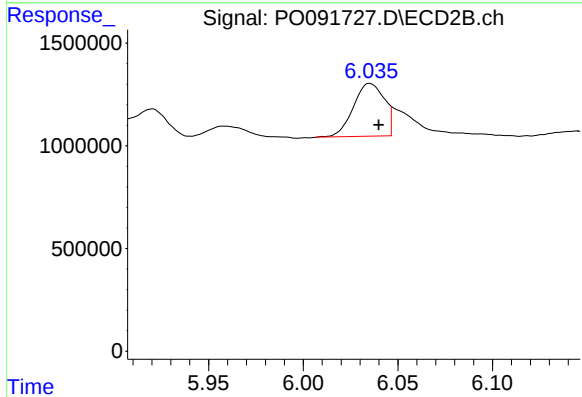


#31 AR-1260-1

R.T.: 6.035 min
Delta R.T.: -0.005 min
Response: 2985460
Conc: 56.50 ng/ml m

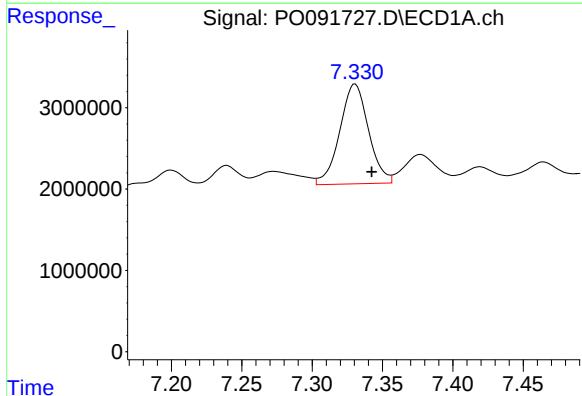


#32 AR-1260-2

R.T.: 7.331 min
Delta R.T.: -0.012 min
Response: 17439280
Conc: 127.40 ng/ml

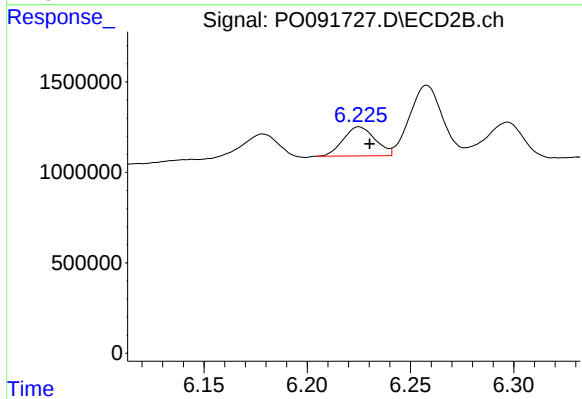

#32 AR-1260-2

R.T.: 6.225 min
Delta R.T.: -0.006 min
Response: 1742161
Conc: 27.26 ng/ml m

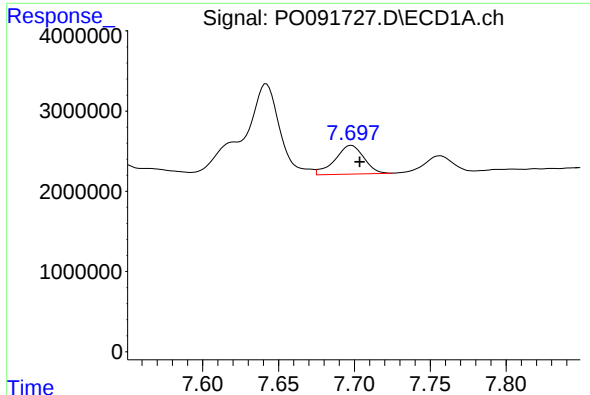


#33 AR-1260-3

R.T.: 7.698 min
Delta R.T.: -0.006 min
Response: 4739853
Conc: 58.03 ng/ml

Instrument :
ECD_O
ClientSampleId :
CHRT-26223


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/30/2022
Supervised By :Ankita Jodhani 12/30/2022

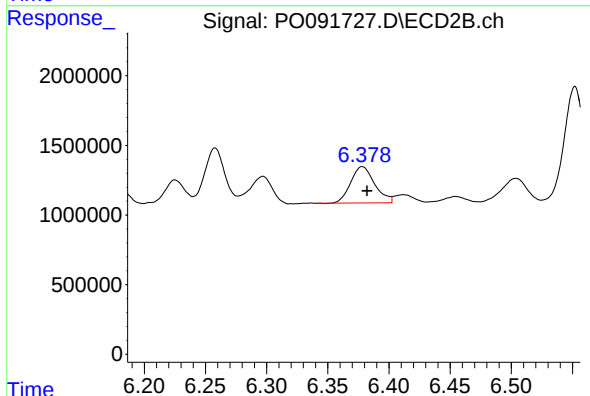


#33 AR-1260-3

R.T.: 6.378 min
Delta R.T.: -0.004 min
Response: 3568710
Conc: 53.43 ng/ml

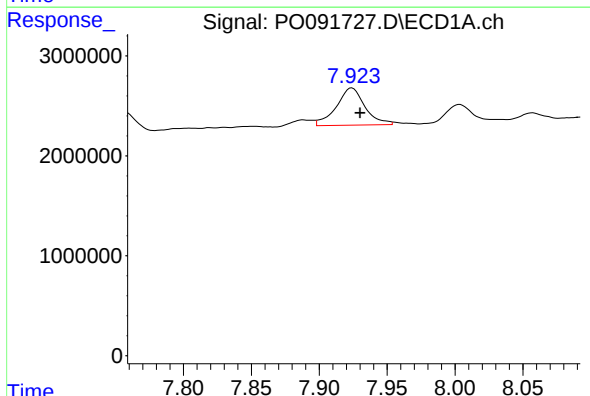


#34 AR-1260-4

R.T.: 7.923 min
Delta R.T.: -0.007 min
Response: 5466739
Conc: 52.99 ng/ml m

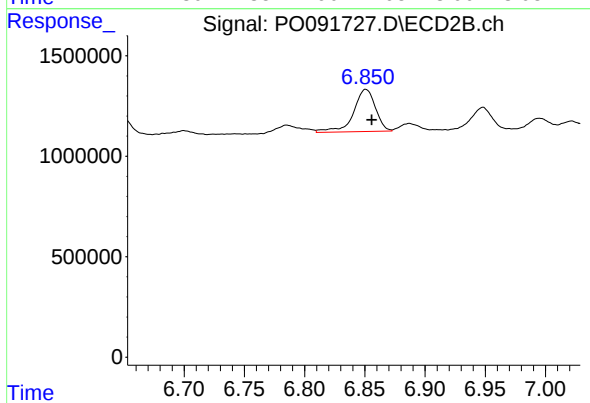

#34 AR-1260-4

R.T.: 6.851 min
Delta R.T.: -0.005 min
Response: 2655319
Conc: 62.73 ng/ml

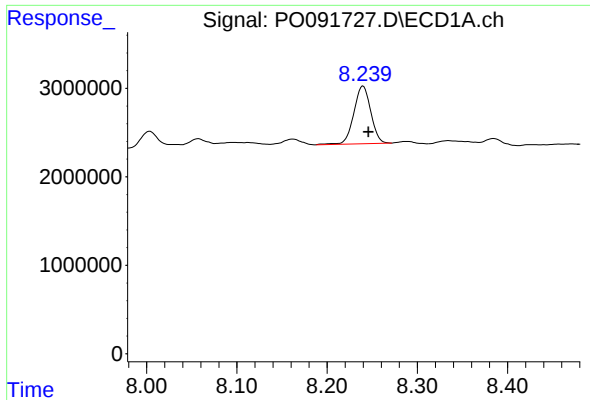


#35 AR-1260-5

R.T.: 8.240 min
Delta R.T.: -0.006 min
Response: 8514072
Conc: 45.15 ng/ml

Instrument :
ECD_O
ClientSampleId :
CHRT-26223

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/30/2022
Supervised By :Ankita Jodhani 12/30/2022

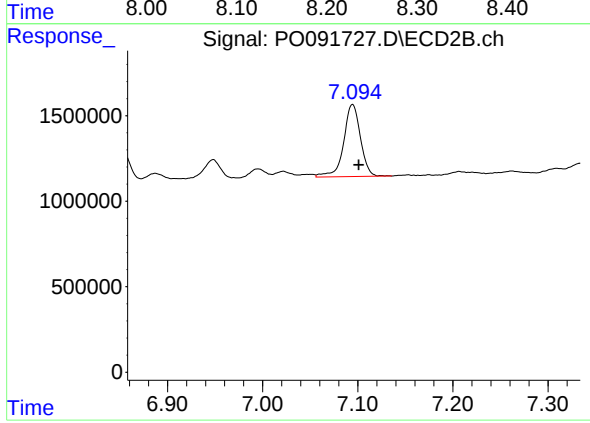

#35 AR-1260-5

R.T.: 7.095 min
Delta R.T.: -0.007 min
Response: 5165850
Conc: 53.18 ng/ml