

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO123019\
 Data File : P0065079.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Dec 2019 10:00
 Operator : AJ/MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 30 13:53:49 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO122619.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Dec 26 13:32:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.177	3.448	476873	558073	20.303	19.813
2)	SA Decachlor...	9.692	8.362	586094	723204	23.086	22.075
Target Compounds							
30)	L6 AR-1254-5	0.000	6.486	0	11644	N.D.	3.869 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO123019\
Data File : PO065079.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Dec 2019 10:00
Operator : AJ/MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 30 13:53:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO122619.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Dec 26 13:32:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

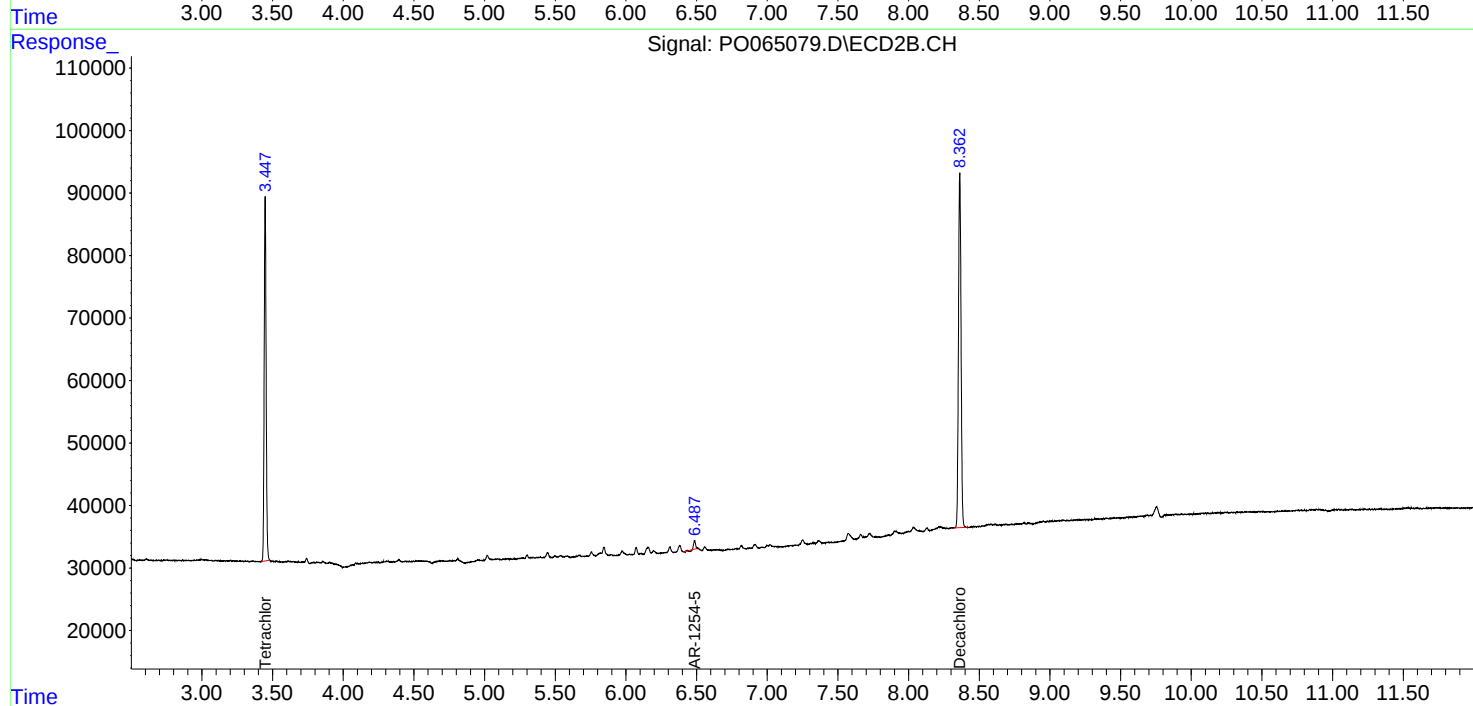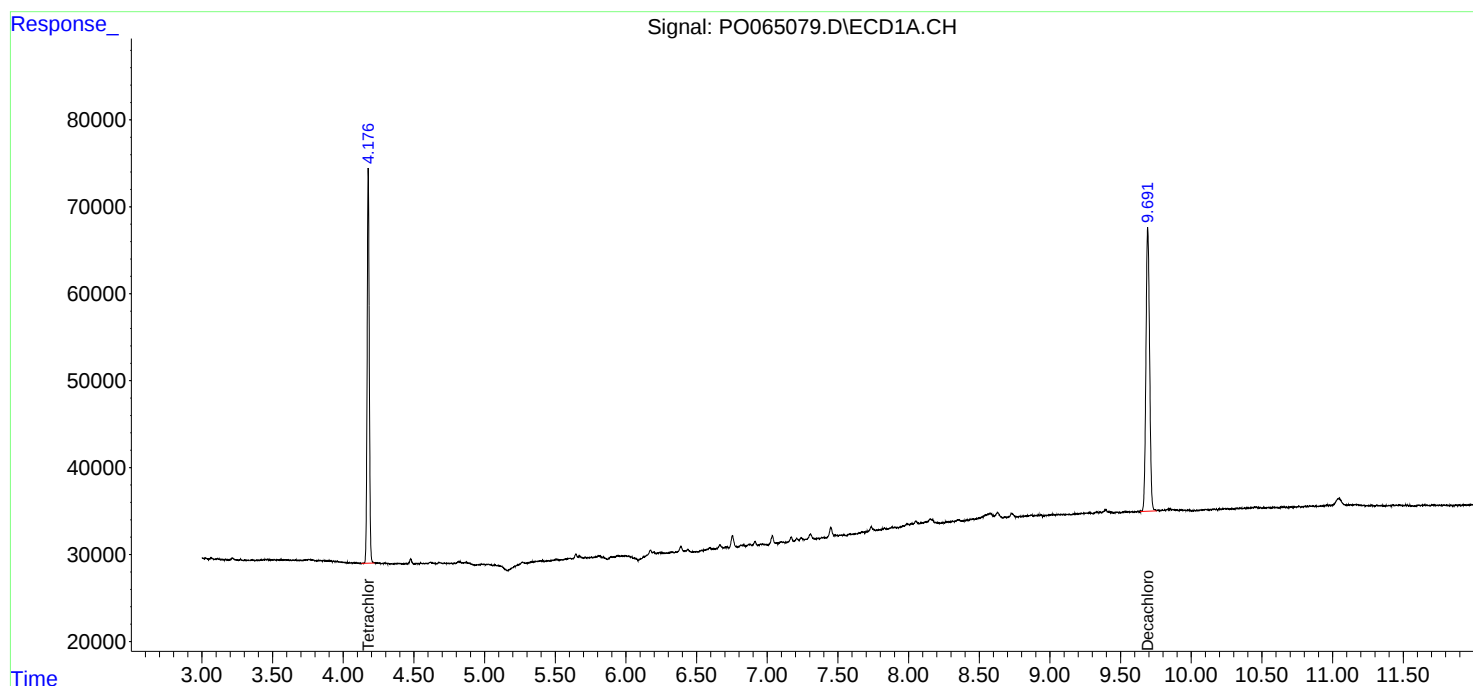


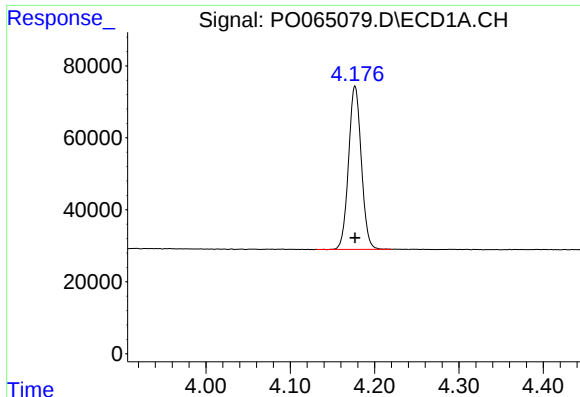

#1 Tetrachloro-m-xylene


R.T.: 4.177 min
Delta R.T.: 0.000 min
Response: 476873
Conc: 20.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

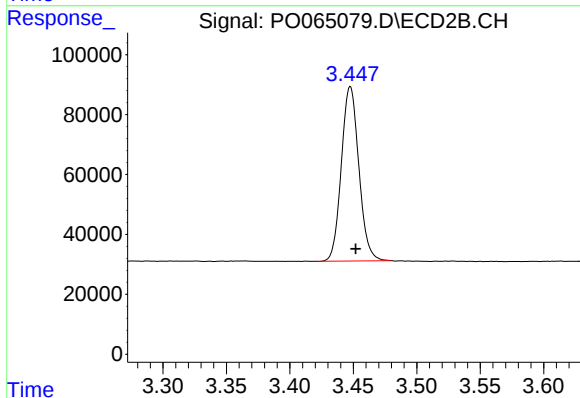


#1 Tetrachloro-m-xylene

R.T.: 3.448 min
Delta R.T.: -0.004 min
Response: 558073
Conc: 19.81 ng/ml

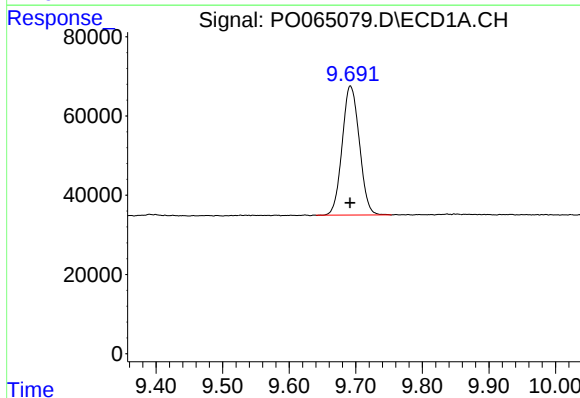


#2 Decachlorobiphenyl

R.T.: 9.692 min
Delta R.T.: 0.000 min
Response: 586094
Conc: 23.09 ng/ml

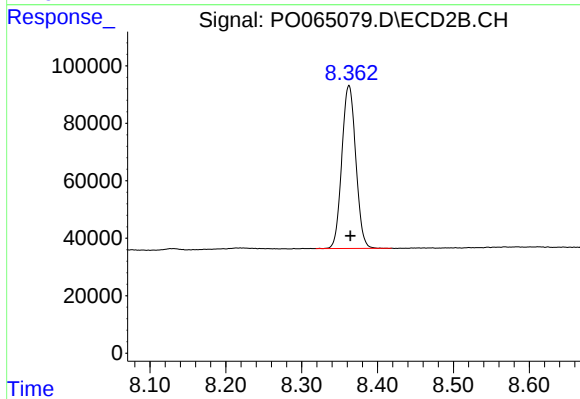

#2 Decachlorobiphenyl


R.T.: 8.362 min
Delta R.T.: -0.002 min
Response: 723204
Conc: 22.08 ng/ml

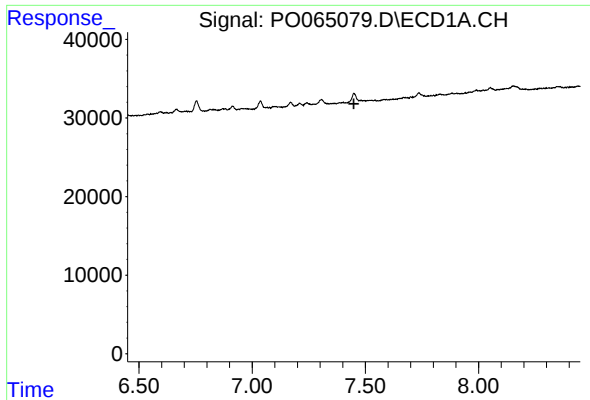

#30 AR-1254-5

R.T.: 0.000 min
Exp R.T.: 7.449 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

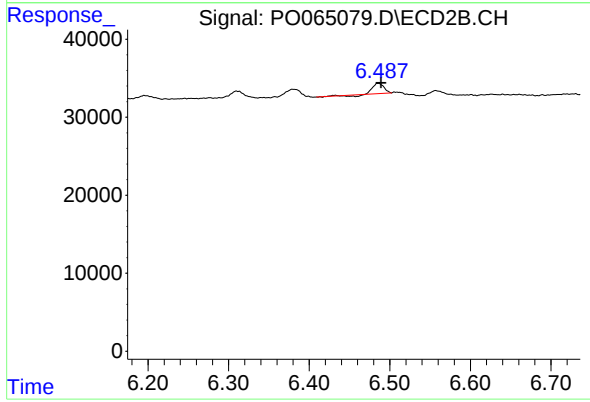

#30 AR-1254-5

R.T.: 6.486 min
Delta R.T.: -0.003 min
Response: 11644
Conc: 3.87 ng/ml