

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0123019\
 Data File : P0065095.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Dec 2019 16:31
 Operator : AJ/MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 30 17:53:01 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0122619.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Dec 26 13:32:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.175	3.452	286804	364758	12.211	12.950
2) SA Decachlor...	9.693	8.366	487484	619377	19.201	18.906
Target Compounds						
7) L1 AR-1016-5	0.000	5.022	0	23398	N.D.	20.961 #
15) L3 AR-1232-5	0.000	5.022	0	23398	N.D.	31.854 #
24) L5 AR-1248-4	0.000	5.022	0	23398	N.D.	17.886 #
27) L6 AR-1254-2	0.000	5.443	0	54576	N.D.	27.077 #
28) L6 AR-1254-3	6.757	0.000	41288	0	18.467	N.D. #
31) L7 AR-1260-1	6.901	0.000	16647	0	10.367	N.D. #
32) L7 AR-1260-2	0.000	6.151	0	10794	N.D.	3.906 #
34) L7 AR-1260-4	7.686	0.000	122365	0	71.987	N.D. #
43) L9 AR-1268-3	8.639	0.000	351768	0	108.031	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO123019\
Data File : P0065095.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Dec 2019 16:31
Operator : AJ/MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 30 17:53:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO122619.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Dec 26 13:32:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

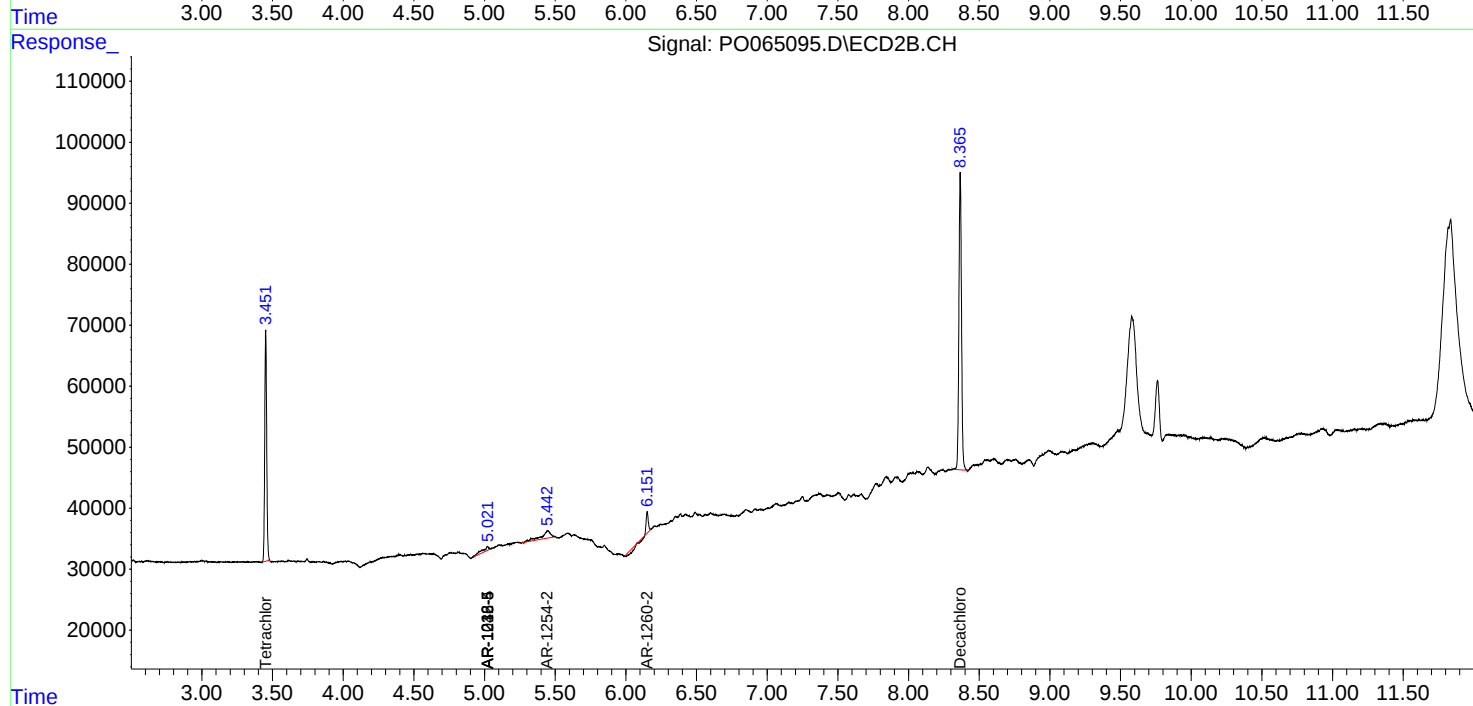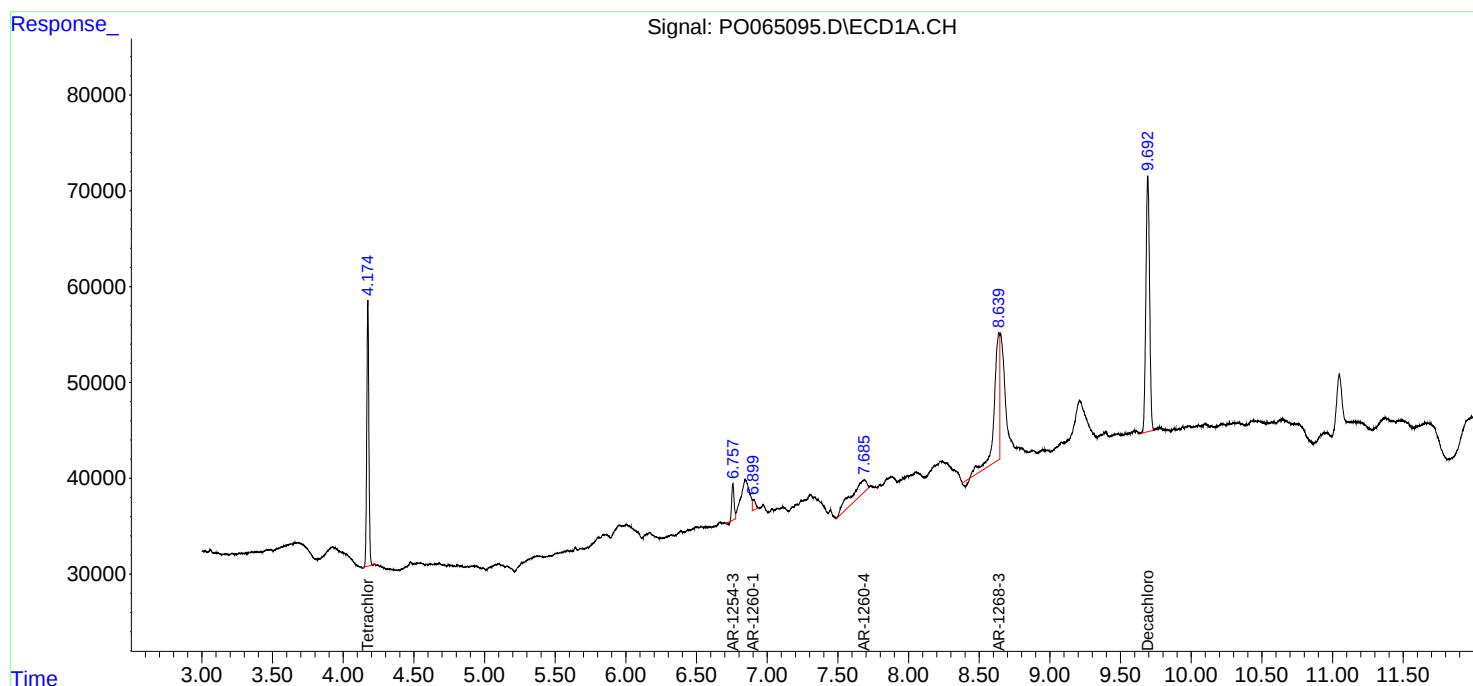


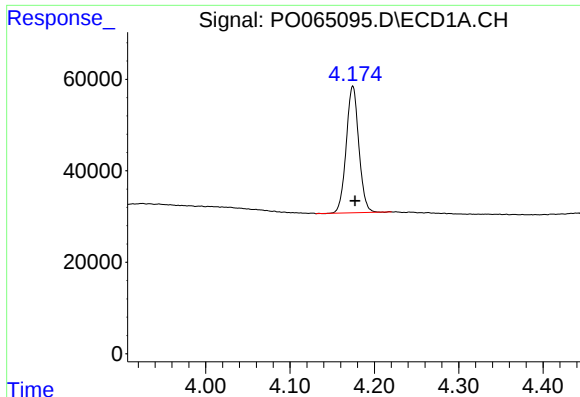

#1 Tetrachloro-m-xylene


R.T.: 4.175 min
Delta R.T.: -0.002 min
Response: 286804
Conc: 12.21 ng/ml

Instrument :
ECD_O
ClientSampleId :

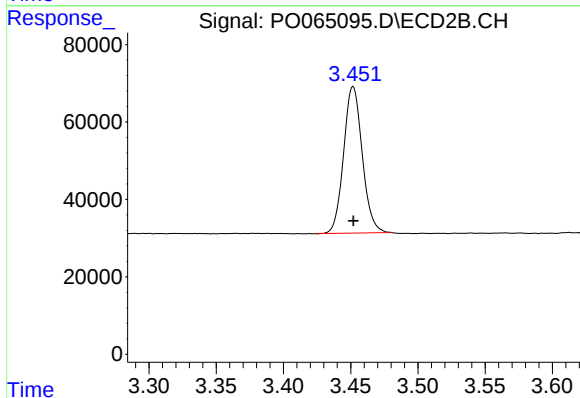


#1 Tetrachloro-m-xylene

R.T.: 3.452 min
Delta R.T.: 0.000 min
Response: 364758
Conc: 12.95 ng/ml

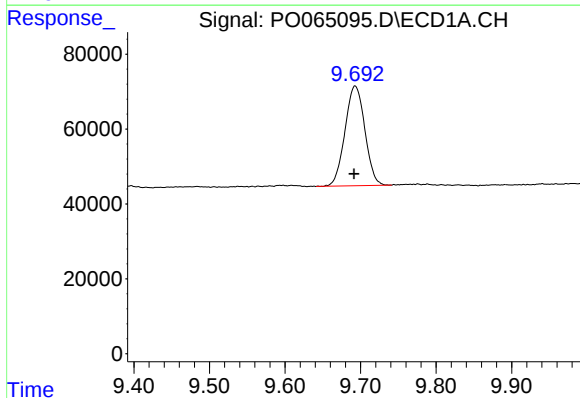


#2 Decachlorobiphenyl

R.T.: 9.693 min
Delta R.T.: 0.002 min
Response: 487484
Conc: 19.20 ng/ml

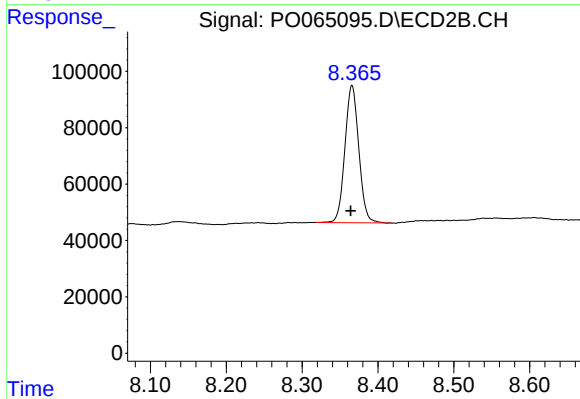

#2 Decachlorobiphenyl


R.T.: 8.366 min
Delta R.T.: 0.002 min
Response: 619377
Conc: 18.91 ng/ml

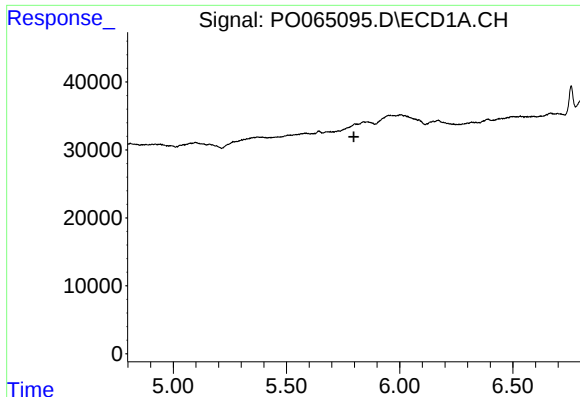

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T.: 5.798 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

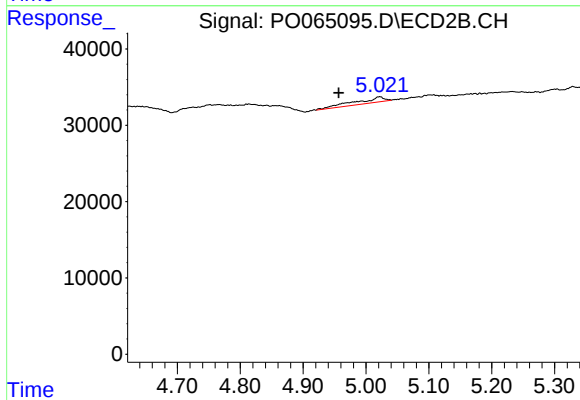


#7 AR-1016-5

R.T.: 5.022 min
Delta R.T.: 0.066 min
Response: 23398
Conc: 20.96 ng/ml

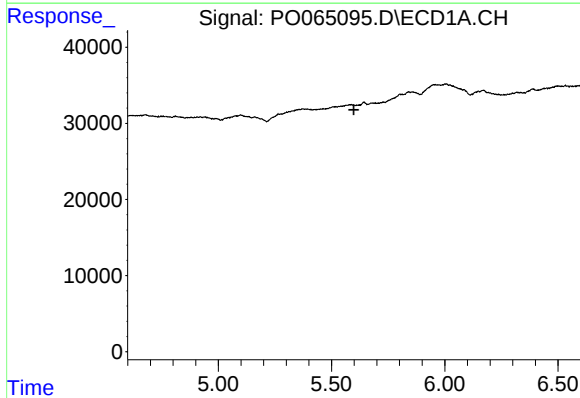


#15 AR-1232-5

R.T.: 0.000 min
Exp R.T.: 5.598 min
Response: 0
Conc: N.D.

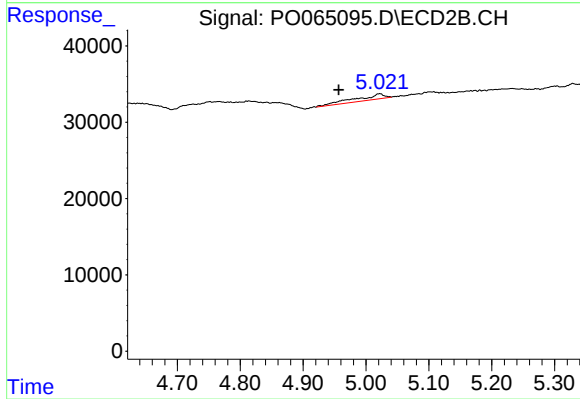

#15 AR-1232-5


R.T.: 5.022 min
Delta R.T.: 0.065 min
Response: 23398
Conc: 31.85 ng/ml

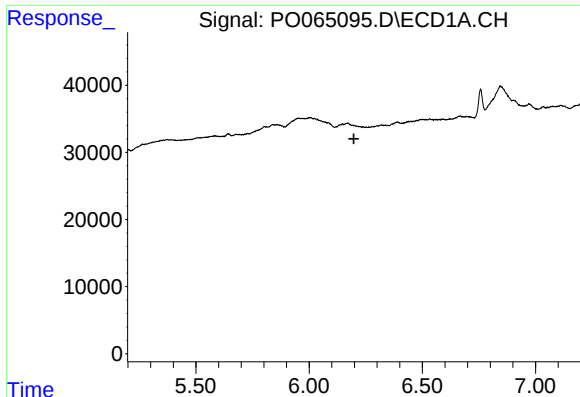

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T.: 6.198 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

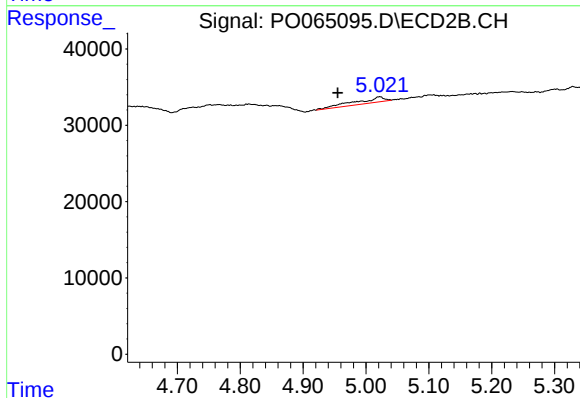


#24 AR-1248-4

R.T.: 5.022 min
Delta R.T.: 0.067 min
Response: 23398
Conc: 17.89 ng/ml

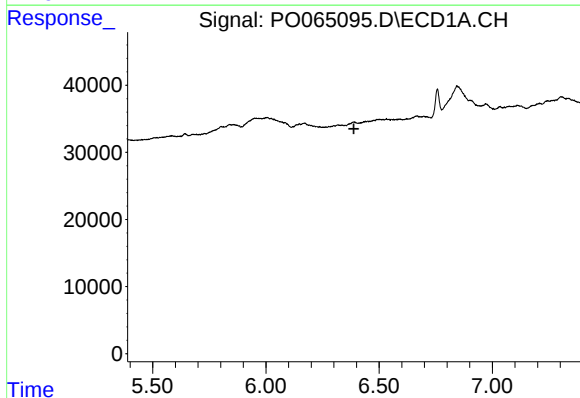


#27 AR-1254-2

R.T.: 0.000 min
Exp R.T.: 6.388 min
Response: 0
Conc: N.D.

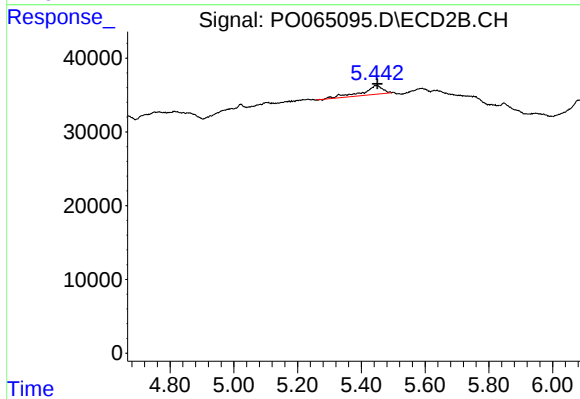

#27 AR-1254-2


R.T.: 5.443 min
Delta R.T.: -0.008 min
Response: 54576
Conc: 27.08 ng/ml

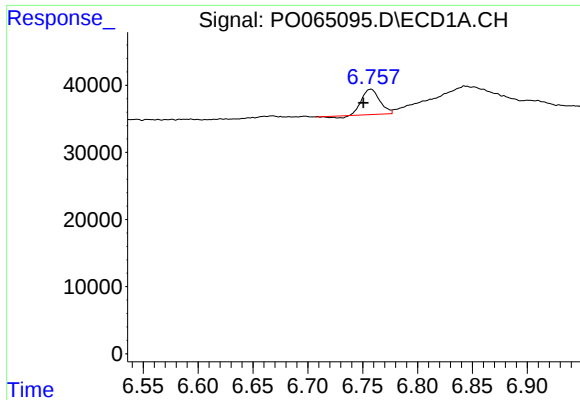

#28 AR-1254-3


R.T.: 6.757 min
Delta R.T.: 0.007 min
Response: 41288
Conc: 18.47 ng/ml

Instrument :
ECD_O
ClientSampleId :

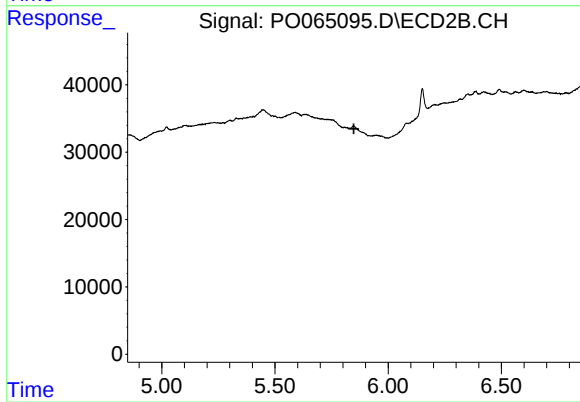


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 5.848 min
Response: 0
Conc: N.D.

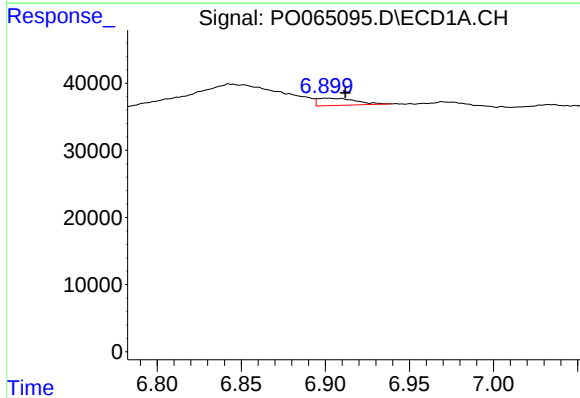


#31 AR-1260-1

R.T.: 6.901 min
Delta R.T.: -0.011 min
Response: 16647
Conc: 10.37 ng/ml

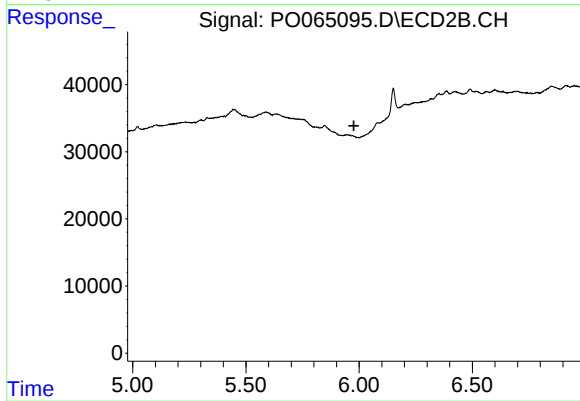

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T. : 5.977 min
Response: 0
Conc: N.D.

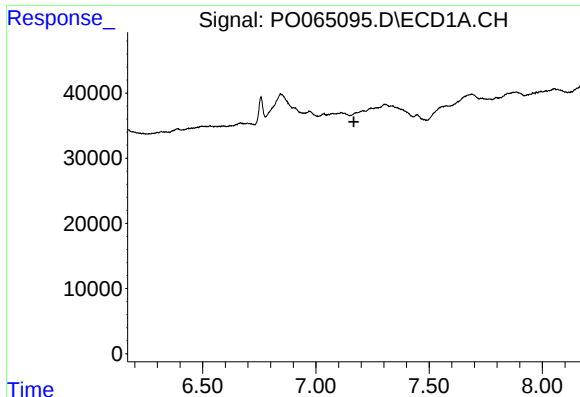

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T.: 7.168 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

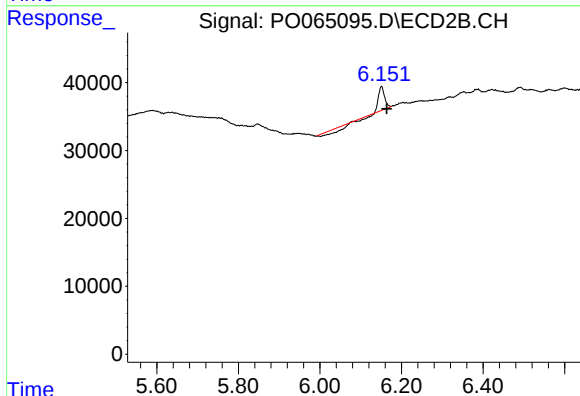


#32 AR-1260-2

R.T.: 6.151 min
Delta R.T.: -0.013 min
Response: 10794
Conc: 3.91 ng/ml

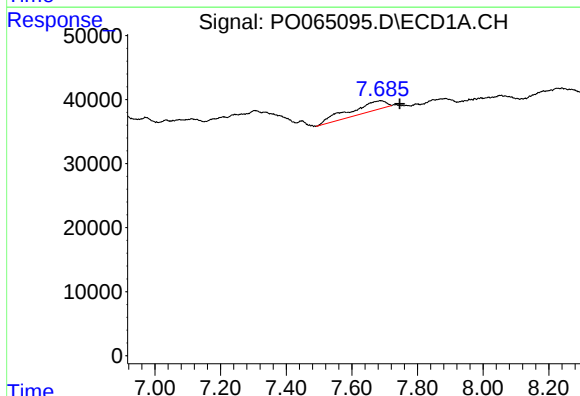


#34 AR-1260-4

R.T.: 7.686 min
Delta R.T.: -0.060 min
Response: 122365
Conc: 71.99 ng/ml

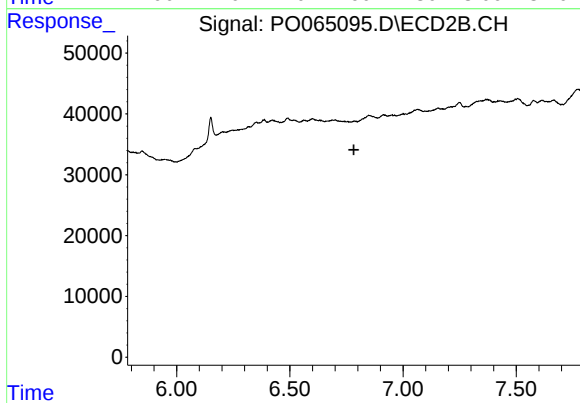

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T.: 6.782 min
Response: 0
Conc: N.D.

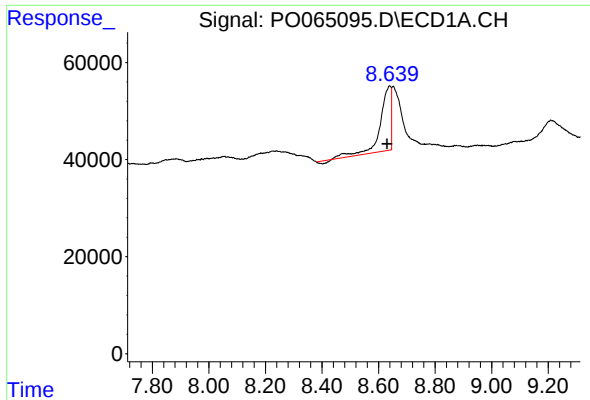

#43 AR-1268-3

R.T.: 8.639 min
Delta R.T.: 0.009 min
Response: 351768
Conc: 108.03 ng/ml

Instrument :
ECD_O
ClientSampleId :

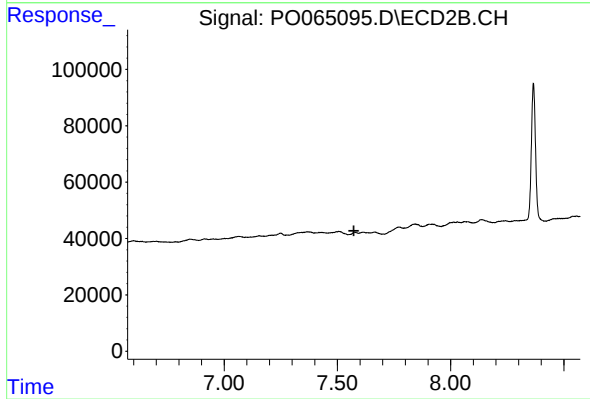

#43 AR-1268-3

R.T.: 0.000 min
Exp R.T. : 7.573 min
Response: 0
Conc: N.D.