

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0123119\
 Data File : P0065132.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 31 Dec 2019 4:43
 Operator : AJ/MA
 Sample : K6463-04
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 GP-7-(4-6)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 31 07:54:22 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0123119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Dec 31 07:42:34 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.179	3.451	509780	632919	24.170	25.053
2)	SA Decachlor...	9.697	8.367	703375	914224	23.049	23.756
Target Compounds							
3)	L1 AR-1016-1	0.000	4.456	0	27932	N.D.	21.774 #
9)	L2 AR-1221-2	0.000	3.745	0	8947	N.D.	39.954 #
16)	L4 AR-1242-1	0.000	4.456	0	27932	N.D.	29.531 #
21)	L5 AR-1248-1	0.000	4.456	0	27932	N.D.	37.078 #
30)	L6 AR-1254-5	0.000	6.492	0	9682	N.D.	2.871 #
31)	L7 AR-1260-1	0.000	5.976	0	48053	N.D.	20.247 #
33)	L7 AR-1260-3	0.000	6.382	0	11912	N.D.	4.435 #
43)	L9 AR-1268-3	0.000	7.576	0	883	N.D.	0.169 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO123119\
Data File : PO065132.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 31 Dec 2019 4:43
Operator : AJ/MA
Sample : K6463-04
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
GP-7-(4-6)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 31 07:54:22 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO123119.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Dec 31 07:42:34 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

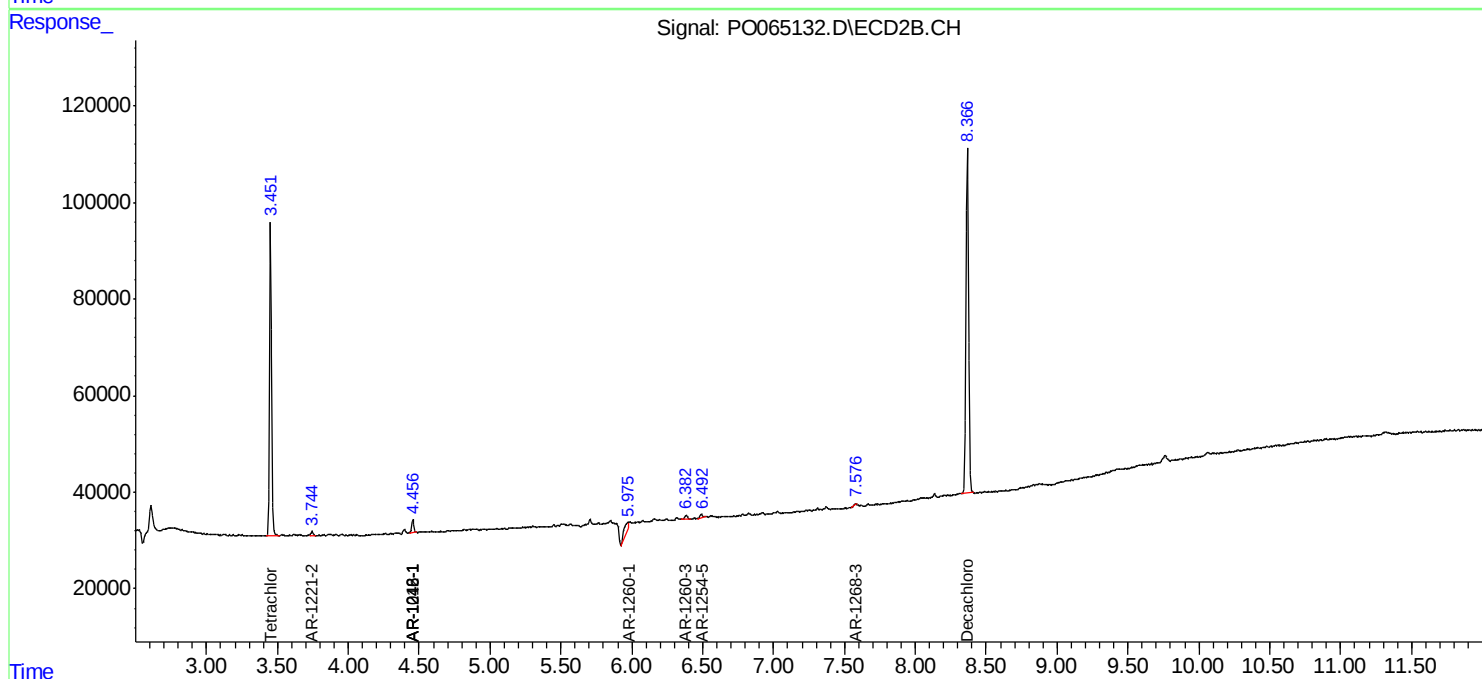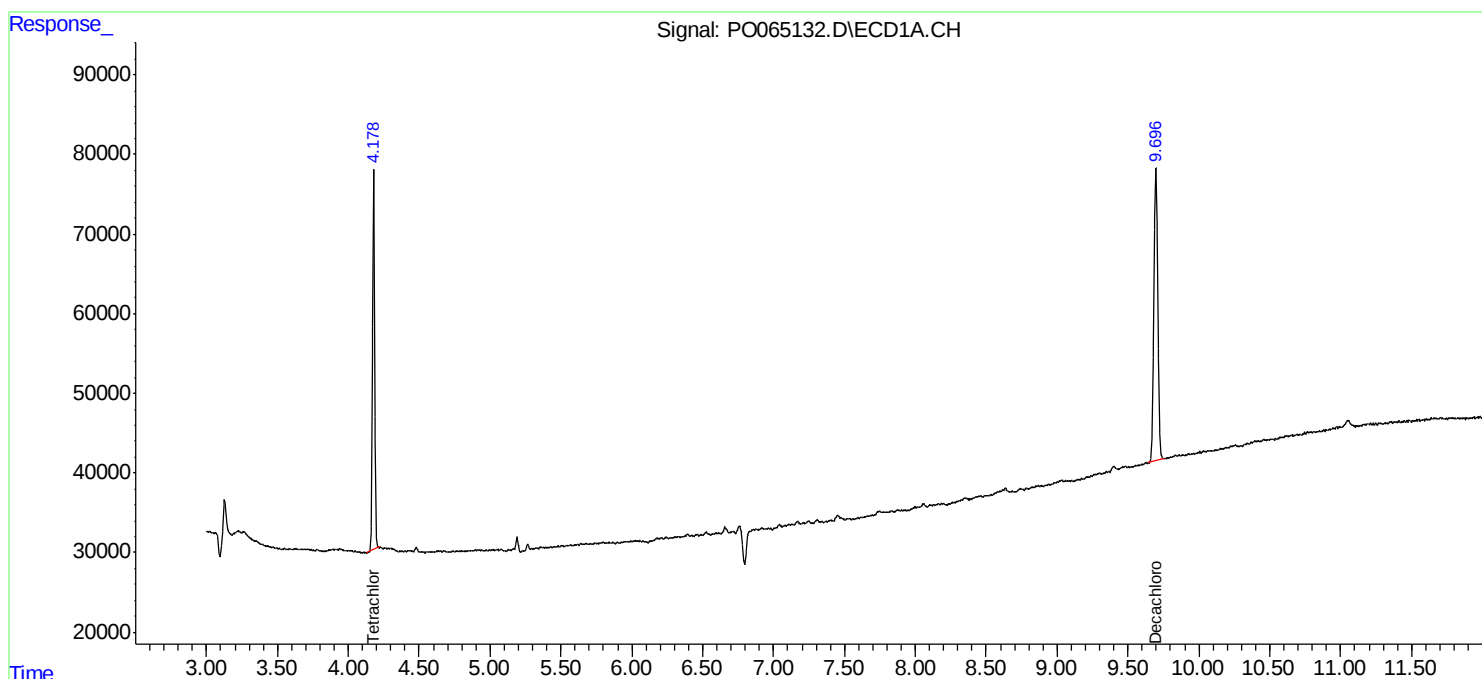


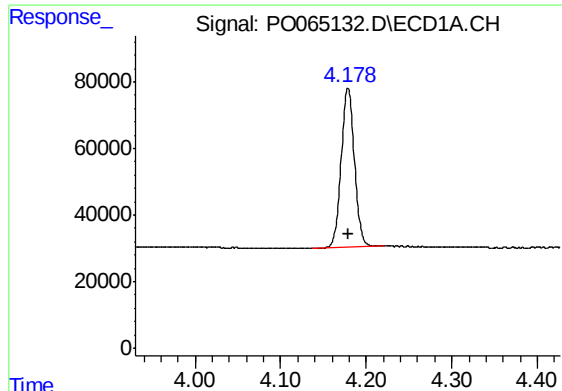

#1 Tetrachloro-m-xylene


R.T.: 4.179 min
Delta R.T.: 0.000 min
Response: 509780
Conc: 24.17 ng/ml

Instrument :
ECD_O
ClientSampleId :
GP-7-(4-6)

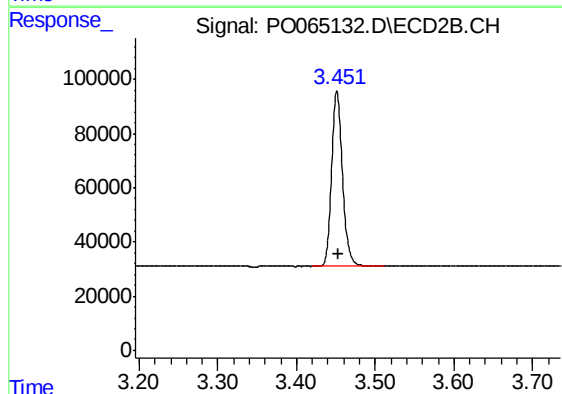


#1 Tetrachloro-m-xylene

R.T.: 3.451 min
Delta R.T.: -0.001 min
Response: 632919
Conc: 25.05 ng/ml

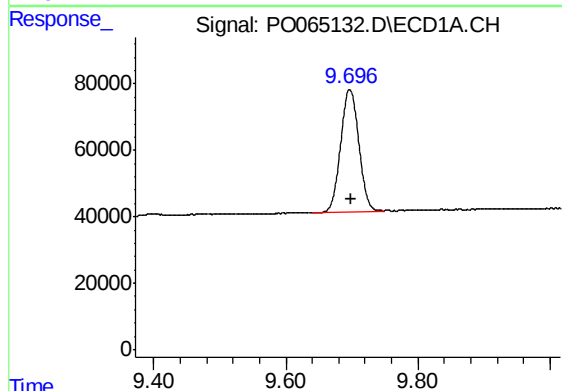


#2 Decachlorobiphenyl

R.T.: 9.697 min
Delta R.T.: -0.002 min
Response: 703375
Conc: 23.05 ng/ml

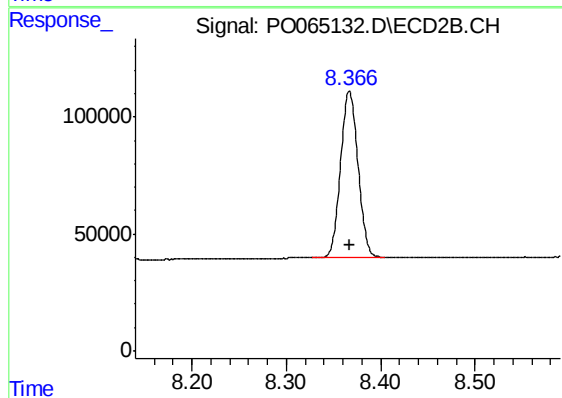

#2 Decachlorobiphenyl


R.T.: 8.367 min
Delta R.T.: 0.000 min
Response: 914224
Conc: 23.76 ng/ml

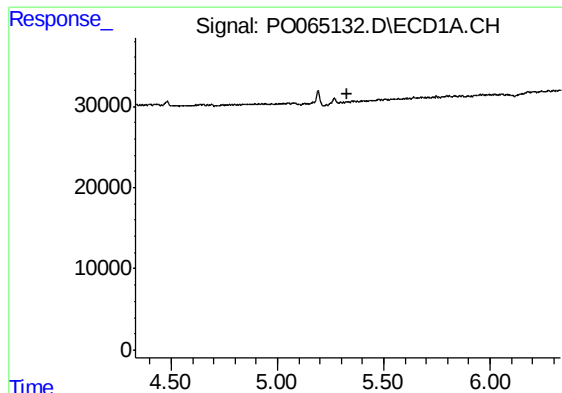

#3 AR-1016-1


R.T.: 0.000 min
Exp R.T. : 5.331 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
GP-7-(4-6)

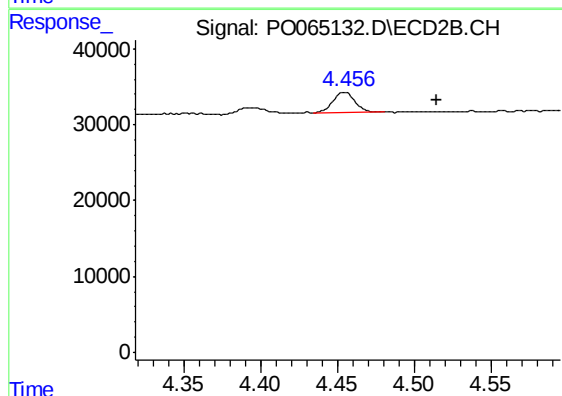


#3 AR-1016-1

R.T.: 4.456 min
Delta R.T.: -0.059 min
Response: 27932
Conc: 21.77 ng/ml

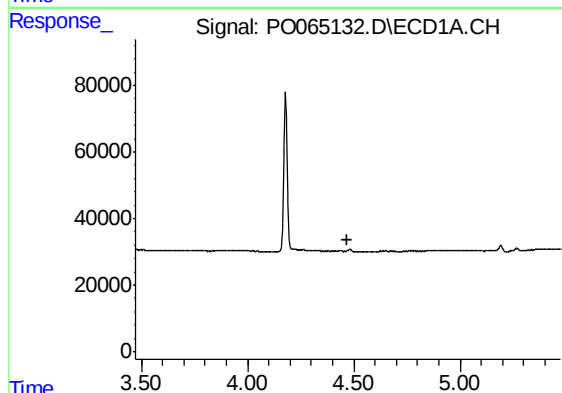


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 4.472 min
Response: 0
Conc: N.D.

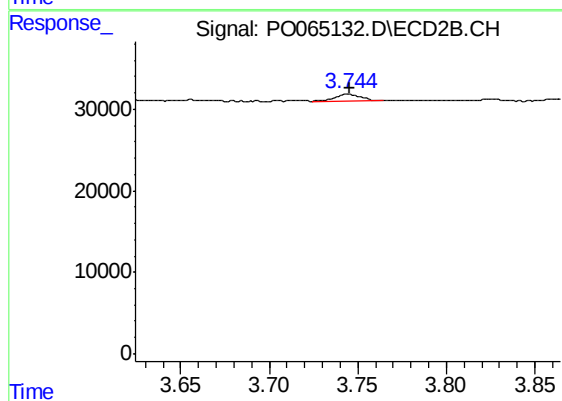

#9 AR-1221-2


R.T.: 3.745 min
Delta R.T.: 0.000 min
Response: 8947
Conc: 39.95 ng/ml

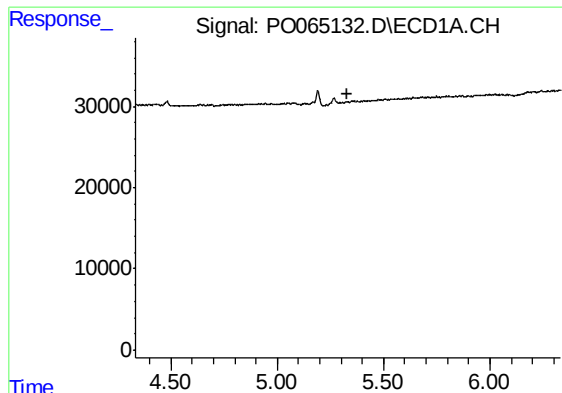

#16 AR-1242-1


R.T.: 0.000 min
Exp R.T. : 5.332 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
GP-7-(4-6)

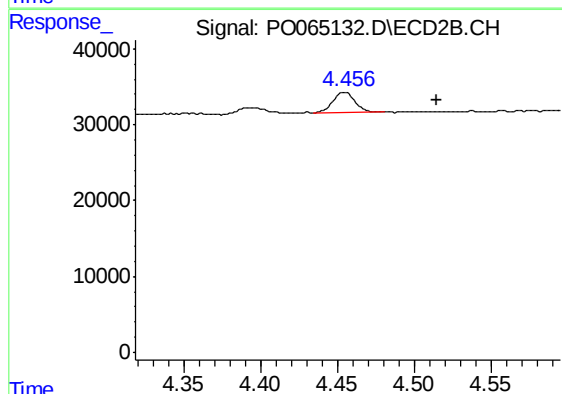


#16 AR-1242-1

R.T.: 4.456 min
Delta R.T.: -0.060 min
Response: 27932
Conc: 29.53 ng/ml

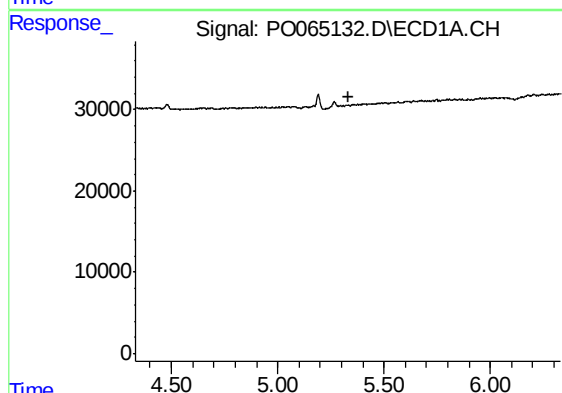


#21 AR-1248-1

R.T.: 0.000 min
Exp R.T. : 5.331 min
Response: 0
Conc: N.D.

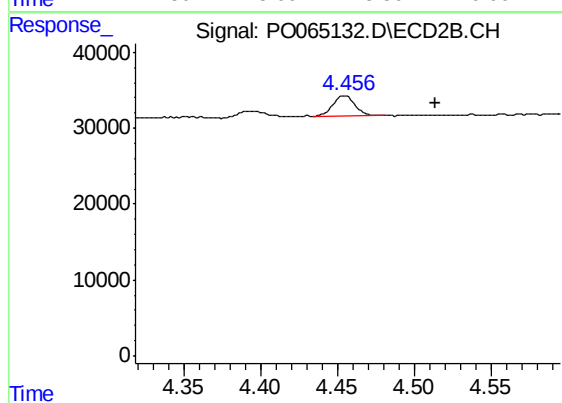

#21 AR-1248-1


R.T.: 4.456 min
Delta R.T.: -0.058 min
Response: 27932
Conc: 37.08 ng/ml

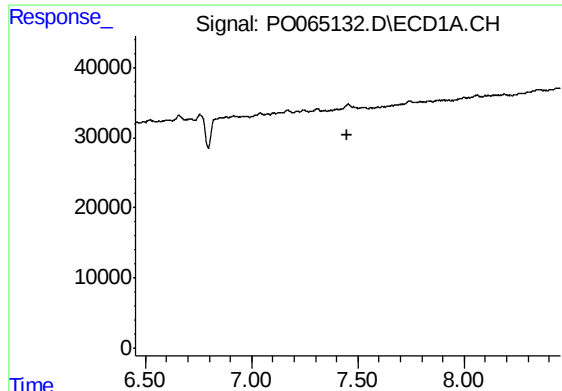

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T. : 7.453 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
GP-7-(4-6)

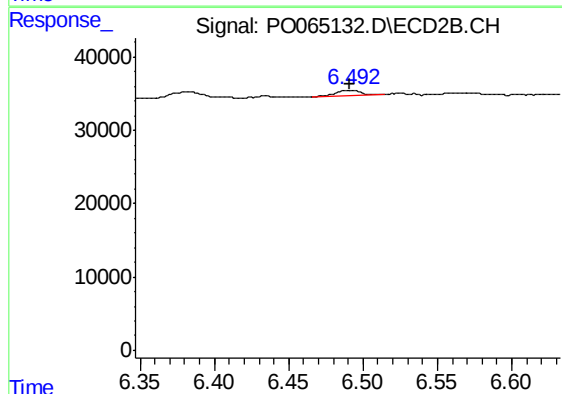


#30 AR-1254-5

R.T.: 6.492 min
Delta R.T.: 0.001 min
Response: 9682
Conc: 2.87 ng/ml

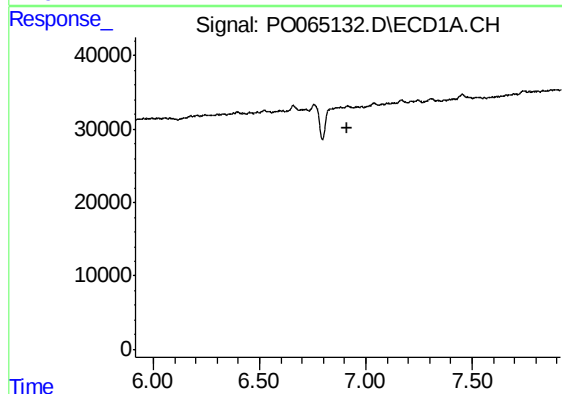


#31 AR-1260-1

R.T.: 0.000 min
Exp R.T. : 6.916 min
Response: 0
Conc: N.D.

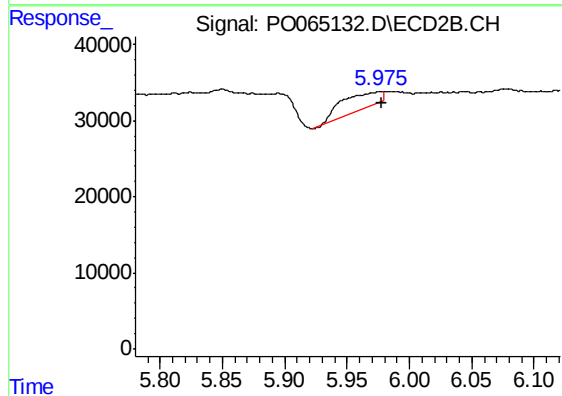

#31 AR-1260-1


R.T.: 5.976 min
Delta R.T.: -0.002 min
Response: 48053
Conc: 20.25 ng/ml

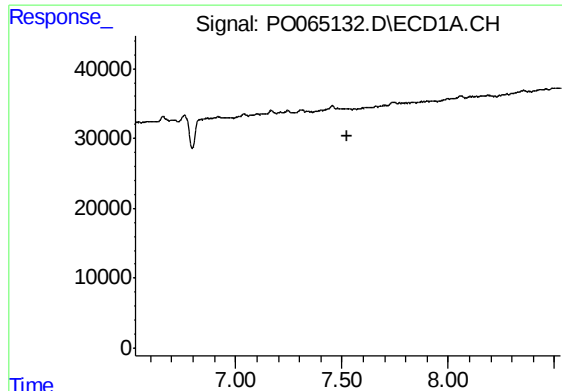

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T. : 7.528 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
GP-7-(4-6)

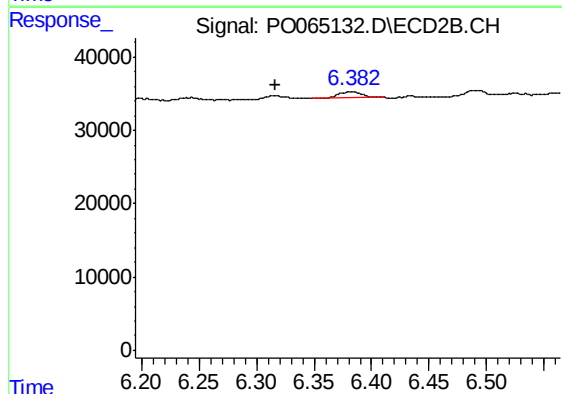


#33 AR-1260-3

R.T.: 6.382 min
Delta R.T.: 0.065 min
Response: 11912
Conc: 4.44 ng/ml

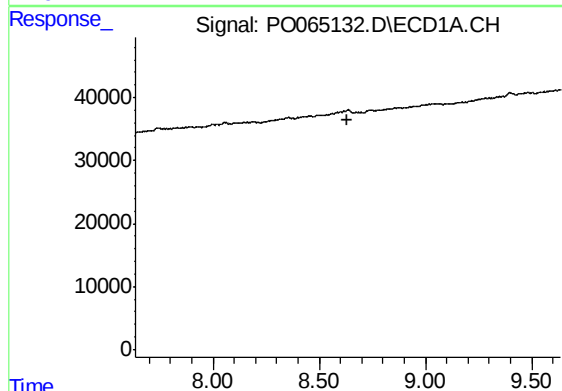

#43 AR-1268-3

R.T.: 0.000 min
Exp R.T. : 8.635 min
Response: 0
Conc: N.D.

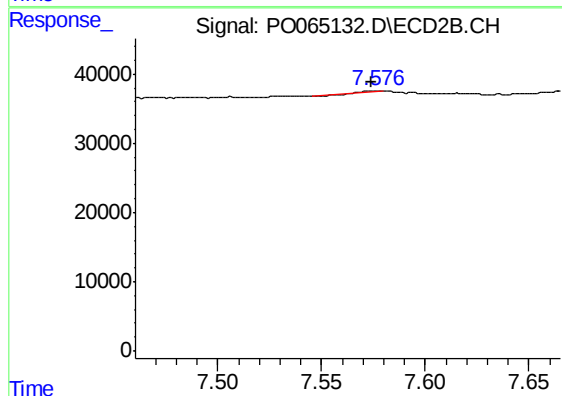

#43 AR-1268-3

R.T.: 7.576 min
Delta R.T.: 0.002 min
Response: 883
Conc: 0.17 ng/ml