

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0123119\
 Data File : P0065121.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 31 Dec 2019 1:22
 Operator : AJ/MA
 Sample : K6456-01
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-03

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 31 07:49:07 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0123119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Dec 31 07:42:34 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.179	3.452	472160	578815	22.386	22.912
2) SA Decachlor...	9.697	8.367	531305	687484	17.410	17.864

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO123119\
Data File : P0065121.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 31 Dec 2019 1:22
Operator : AJ/MA
Sample : K6456-01
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SB-03

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 31 07:49:07 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO123119.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Dec 31 07:42:34 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

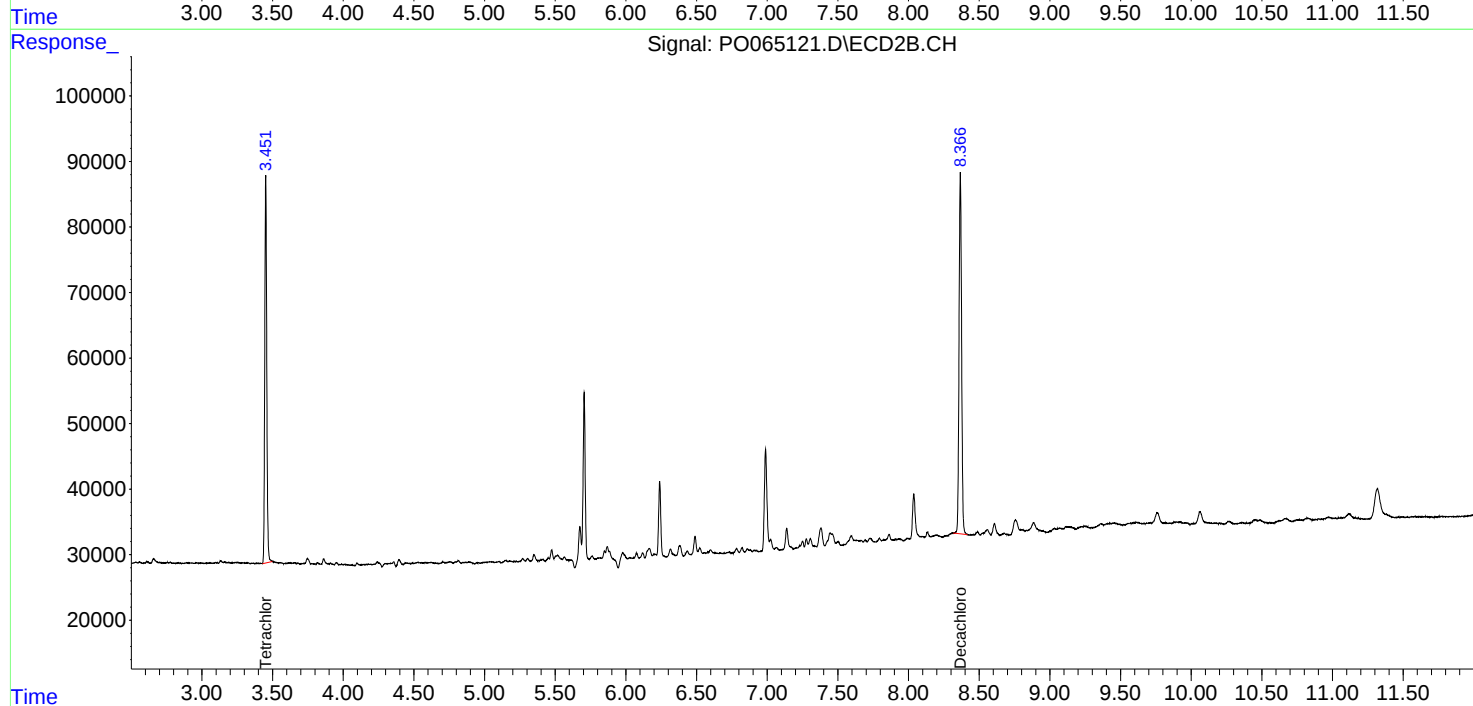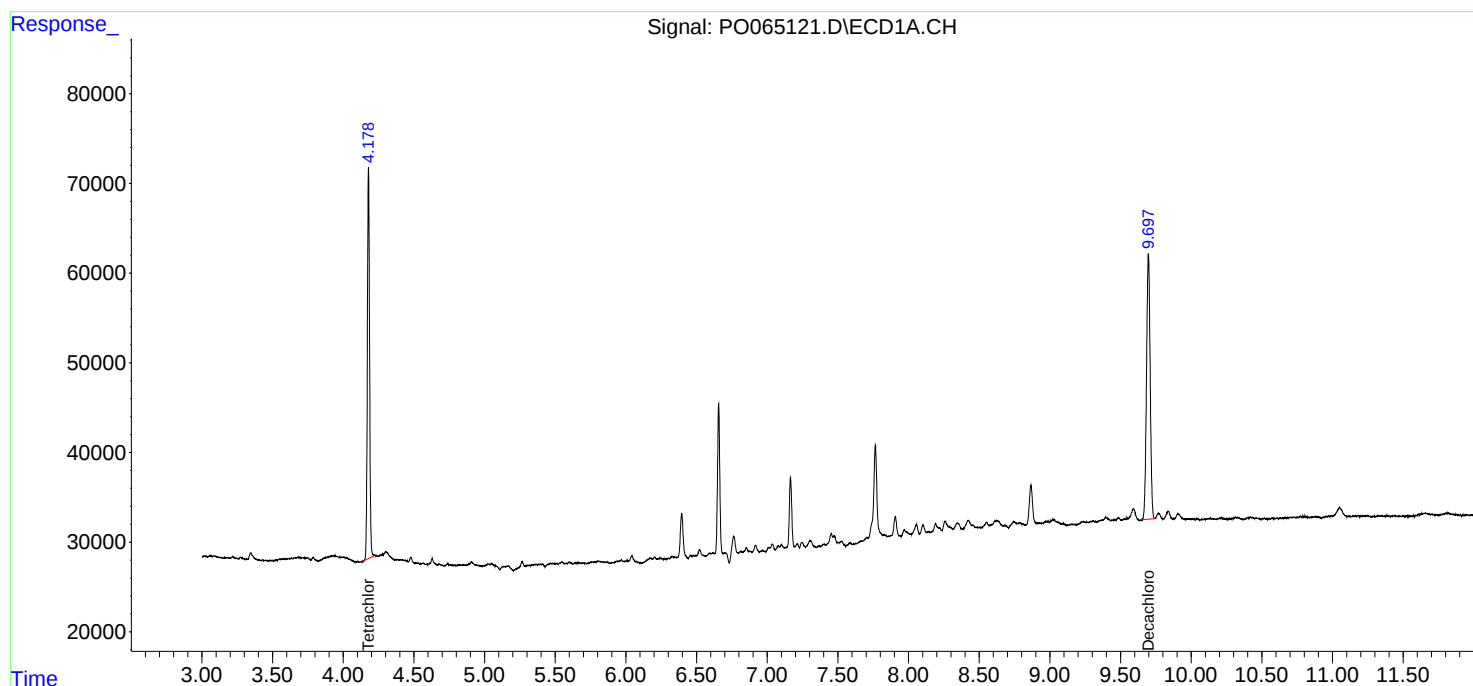


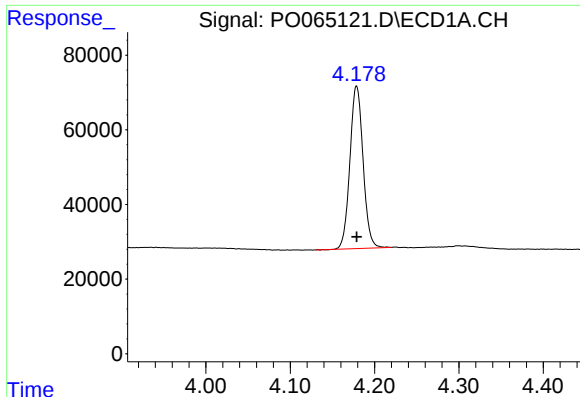

#1 Tetrachloro-m-xylene


R.T.: 4.179 min
Delta R.T.: 0.000 min
Response: 472160
Conc: 22.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-03

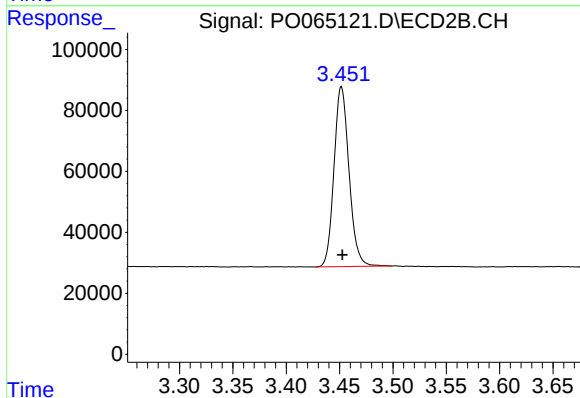


#1 Tetrachloro-m-xylene

R.T.: 3.452 min
Delta R.T.: -0.001 min
Response: 578815
Conc: 22.91 ng/ml

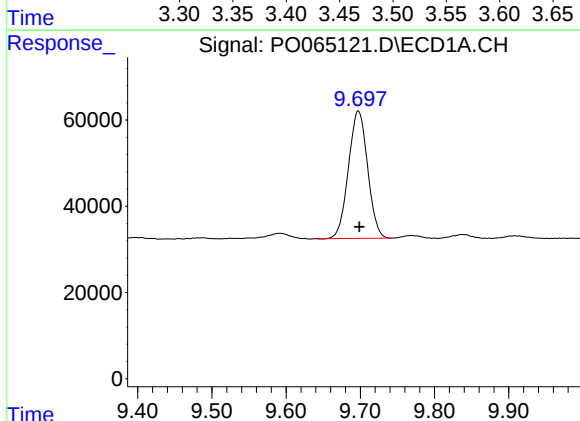

#2 Decachlorobiphenyl

R.T.: 9.697 min
Delta R.T.: -0.002 min
Response: 531305
Conc: 17.41 ng/ml

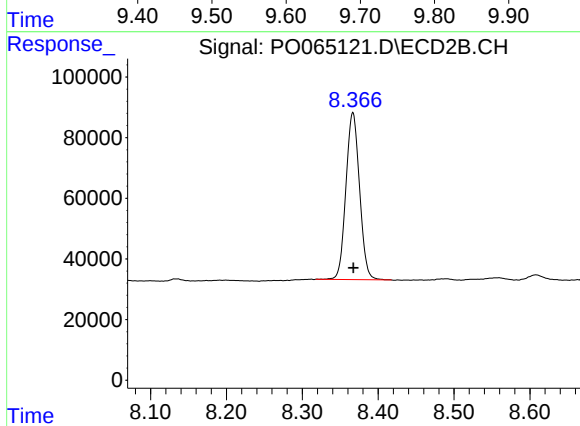

#2 Decachlorobiphenyl

R.T.: 8.367 min
Delta R.T.: 0.000 min
Response: 687484
Conc: 17.86 ng/ml