

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0123119\
 Data File : P0065134.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 31 Dec 2019 5:17
 Operator : AJ/MA
 Sample : K6464-02
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-5-(8-10)

Manual Integrations
 APPROVED

mohammad
 12/31/2019 2:48:41 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 31 07:55:27 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0123119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Dec 31 07:42:34 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.179	3.451	514296	975951	24.384m	38.632m#
2) SA Decachlor...	9.697	8.366	479496	600359	15.712	15.600

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO123119\
Data File : P0065134.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 31 Dec 2019 5:17
Operator : AJ/MA
Sample : K6464-02
Misc :
ALS Vial : 35 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SB-5-(8-10)


Manual Integrations
APPROVED

mohammad
12/31/2019 2:48:41 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 31 07:55:27 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO123119.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Dec 31 07:42:34 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

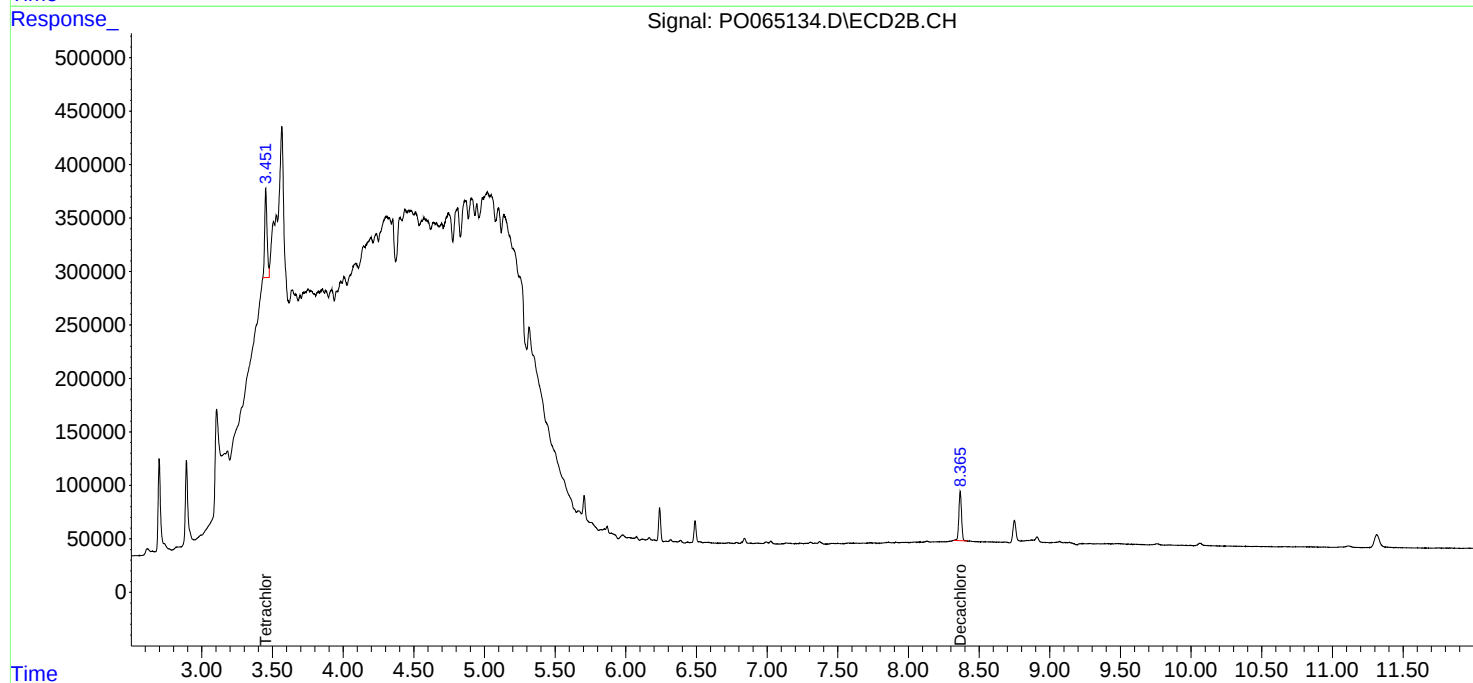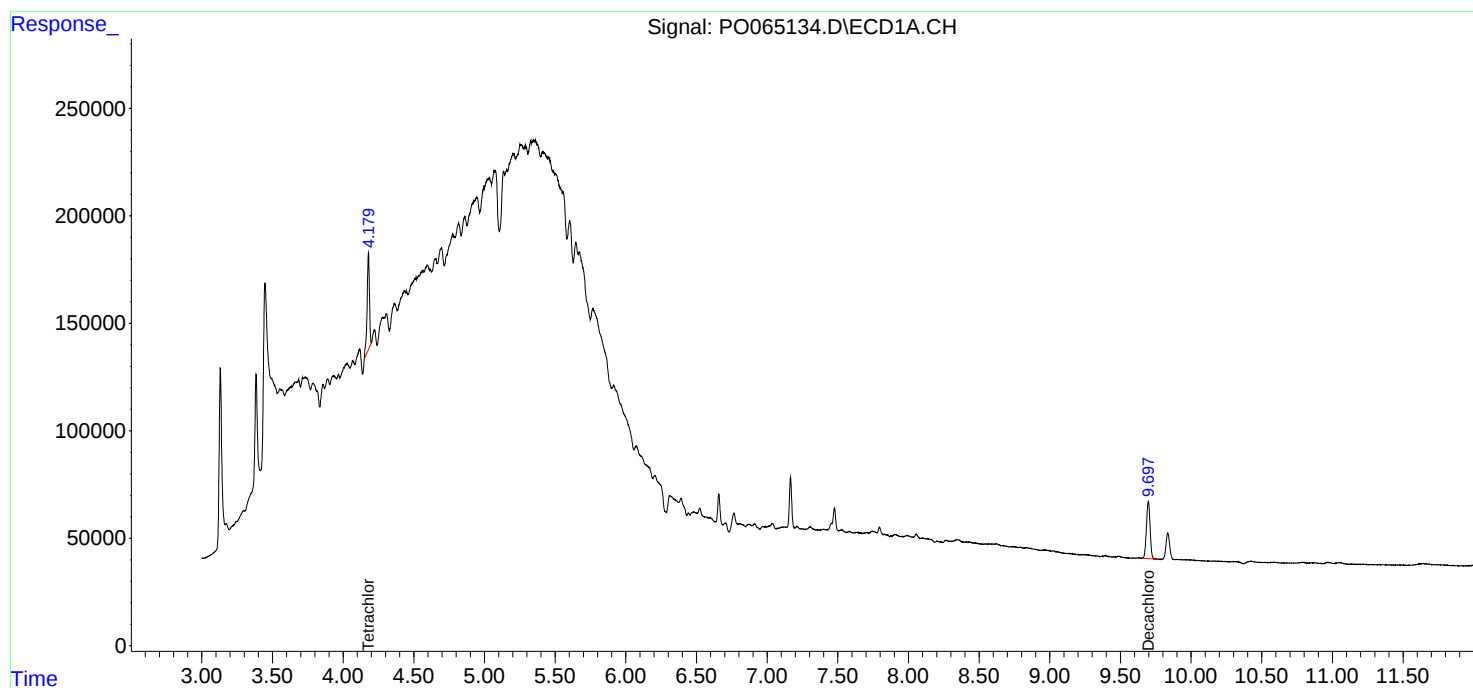

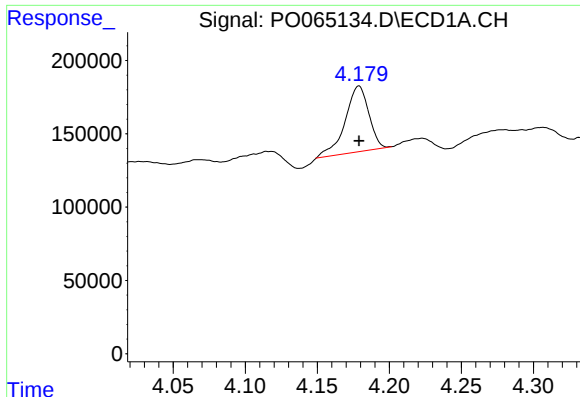


#1 Tetrachloro-m-xylene

R.T.: 4.179 min
Delta R.T.: 0.000 min
Response: 514296
Conc: 24.38 ng/ml m

Instrument :
ECD_O
ClientSampleId :
SB-5-(8-10)


Manual Integrations
APPROVED

mohammad
12/31/2019 2:48:41 PM

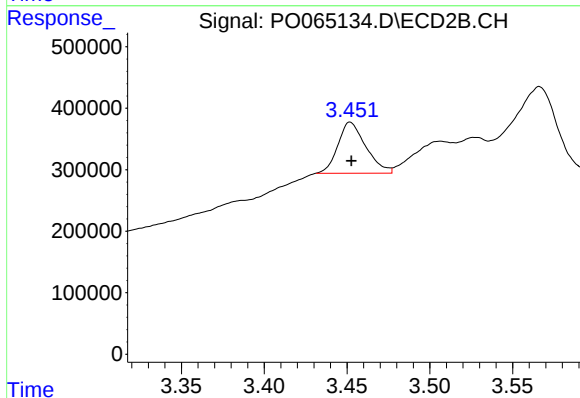


#1 Tetrachloro-m-xylene

R.T.: 3.451 min
Delta R.T.: -0.001 min
Response: 975951
Conc: 38.63 ng/ml m

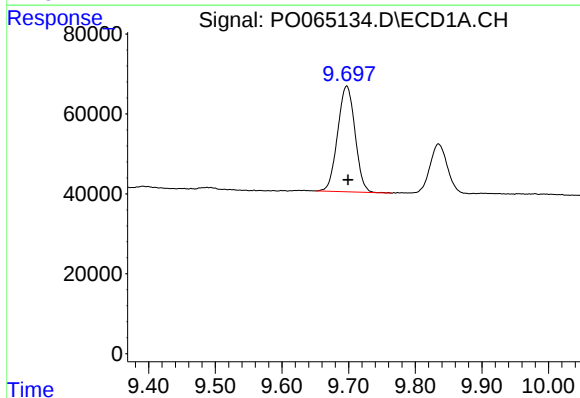

#2 Decachlorobiphenyl

R.T.: 9.697 min
Delta R.T.: -0.002 min
Response: 479496
Conc: 15.71 ng/ml

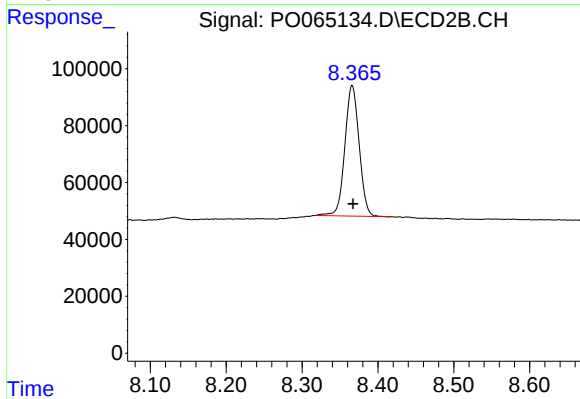

#2 Decachlorobiphenyl

R.T.: 8.366 min
Delta R.T.: -0.001 min
Response: 600359
Conc: 15.60 ng/ml