

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0123120\
 Data File : P0074316.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 31 Dec 2020 11:25
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Manual Integrations
 APPROVED

mohammad
 12/31/2020 2:37:57 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 31 11:46:34 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0122320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Dec 24 01:16:32 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.945	3.990	2475401	1343026	24.278m	23.409
2) SA Decachlor...	10.967	9.250	2274236	1285624	23.353	23.914

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO123120\
Data File : PO074316.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 31 Dec 2020 11:25
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

mohammad
12/31/2020 2:37:57 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 31 11:46:34 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO122320.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Dec 24 01:16:32 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

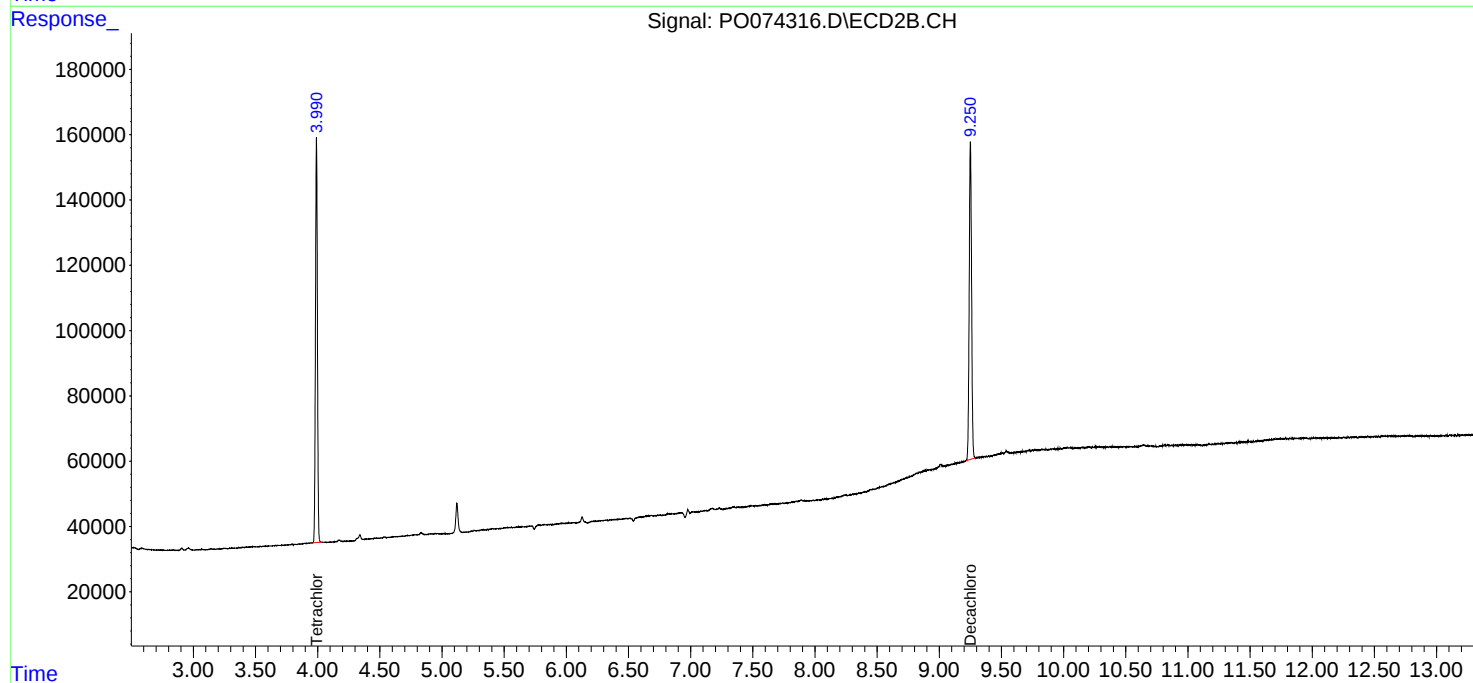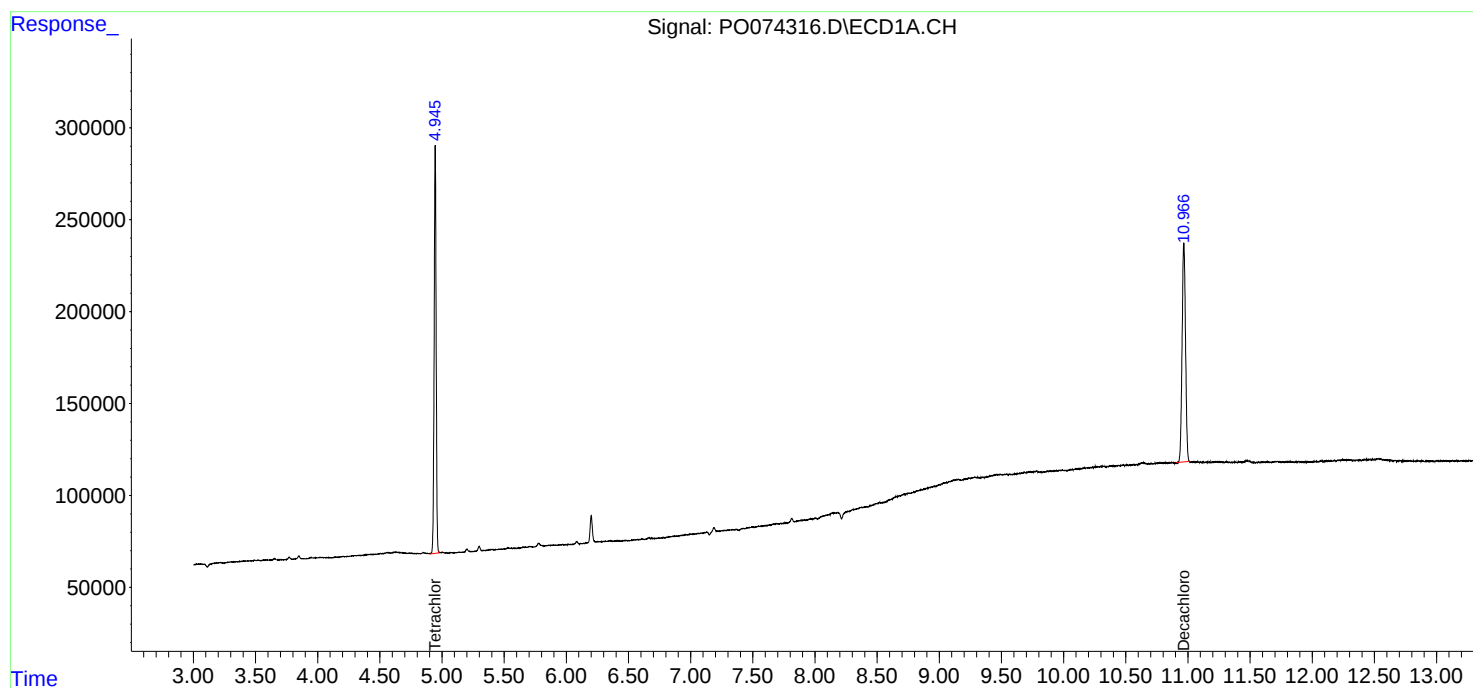

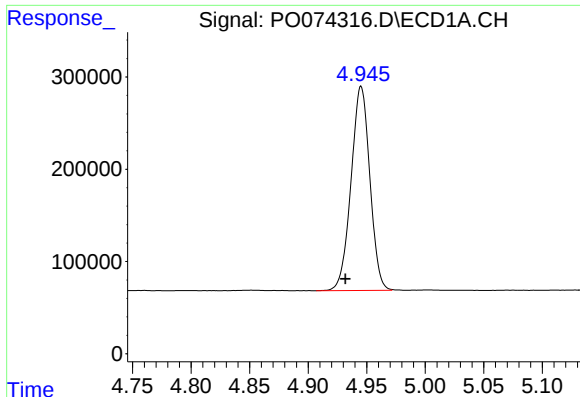


#1 Tetrachloro-m-xylene

R.T.: 4.945 min
Delta R.T.: 0.013 min
Response: 2475401
Conc: 24.28 ng/ml m

Instrument :
ECD_O
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

mohammad
12/31/2020 2:37:57 PM

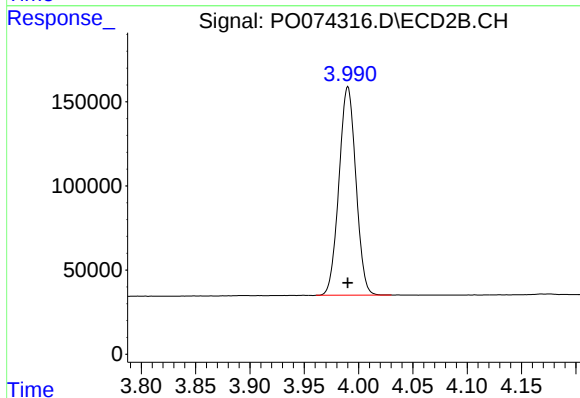


#1 Tetrachloro-m-xylene

R.T.: 3.990 min
Delta R.T.: 0.000 min
Response: 1343026
Conc: 23.41 ng/ml

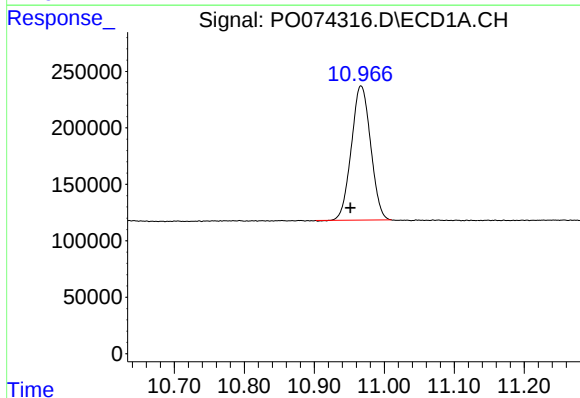

#2 Decachlorobiphenyl

R.T.: 10.967 min
Delta R.T.: 0.015 min
Response: 2274236
Conc: 23.35 ng/ml

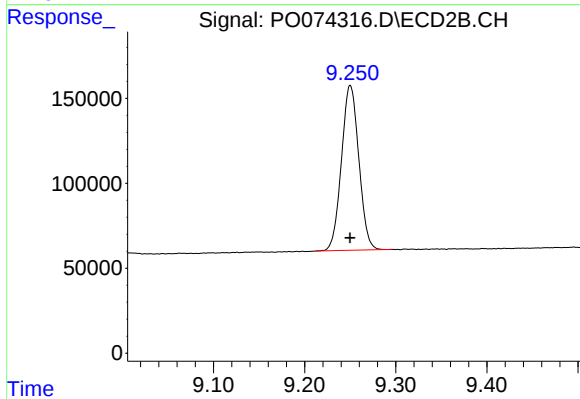

#2 Decachlorobiphenyl

R.T.: 9.250 min
Delta R.T.: 0.000 min
Response: 1285624
Conc: 23.91 ng/ml