

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0123124\
 Data File : P0108854.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Dec 2024 13:13
 Operator : YP/AJ
 Sample : P5402-01 10X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 0827

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 01/02/2025
 Supervised By :Ankita Jodhani 01/02/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 01 02:29:43 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0120624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 07 05:58:15 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.704	3.701	11119286	6605592	1.278m	1.303m
2) SA Decachlor...	8.769	8.719	20440278	10058468	2.798	2.596

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO123124\
Data File : PO108854.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Dec 2024 13:13
Operator : YP/AJ
Sample : P5402-01 10X
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
0827


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/02/2025
Supervised By :Ankita Jodhani 01/02/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 01 02:29:43 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 07 05:58:15 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

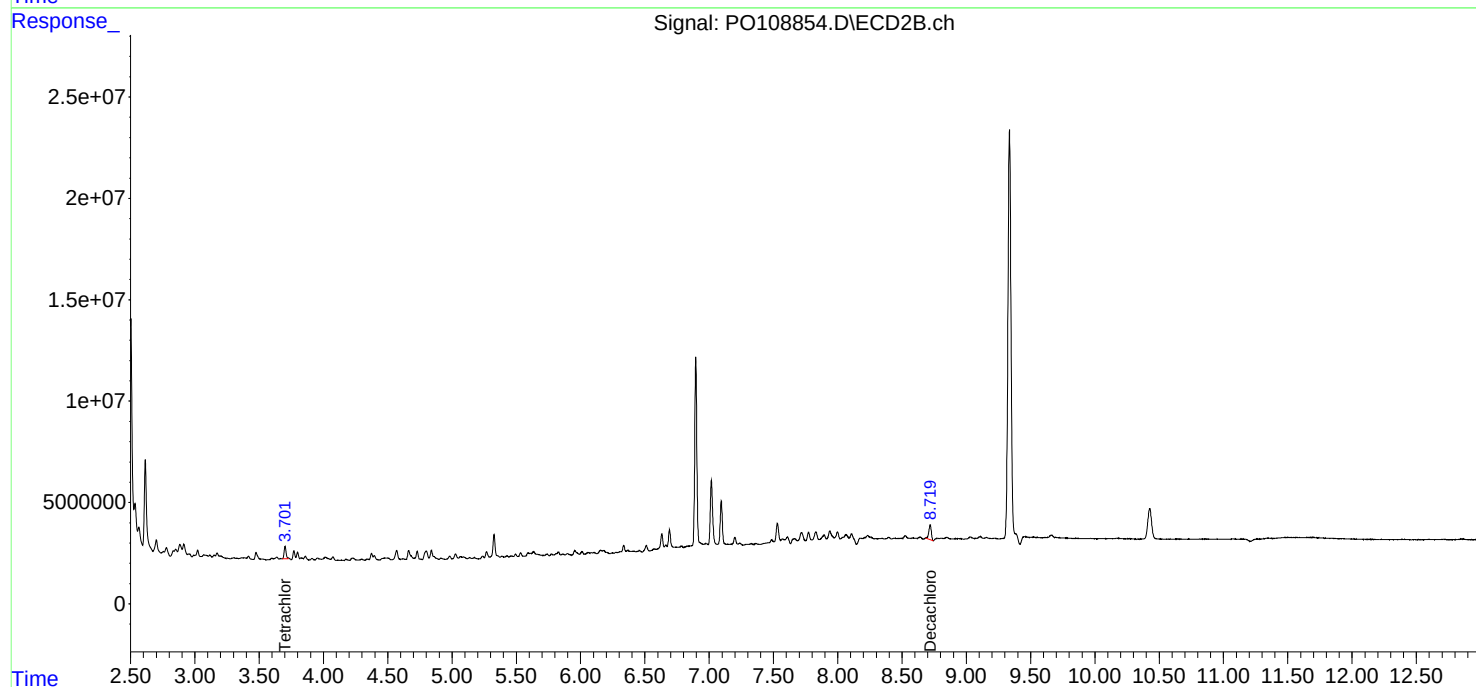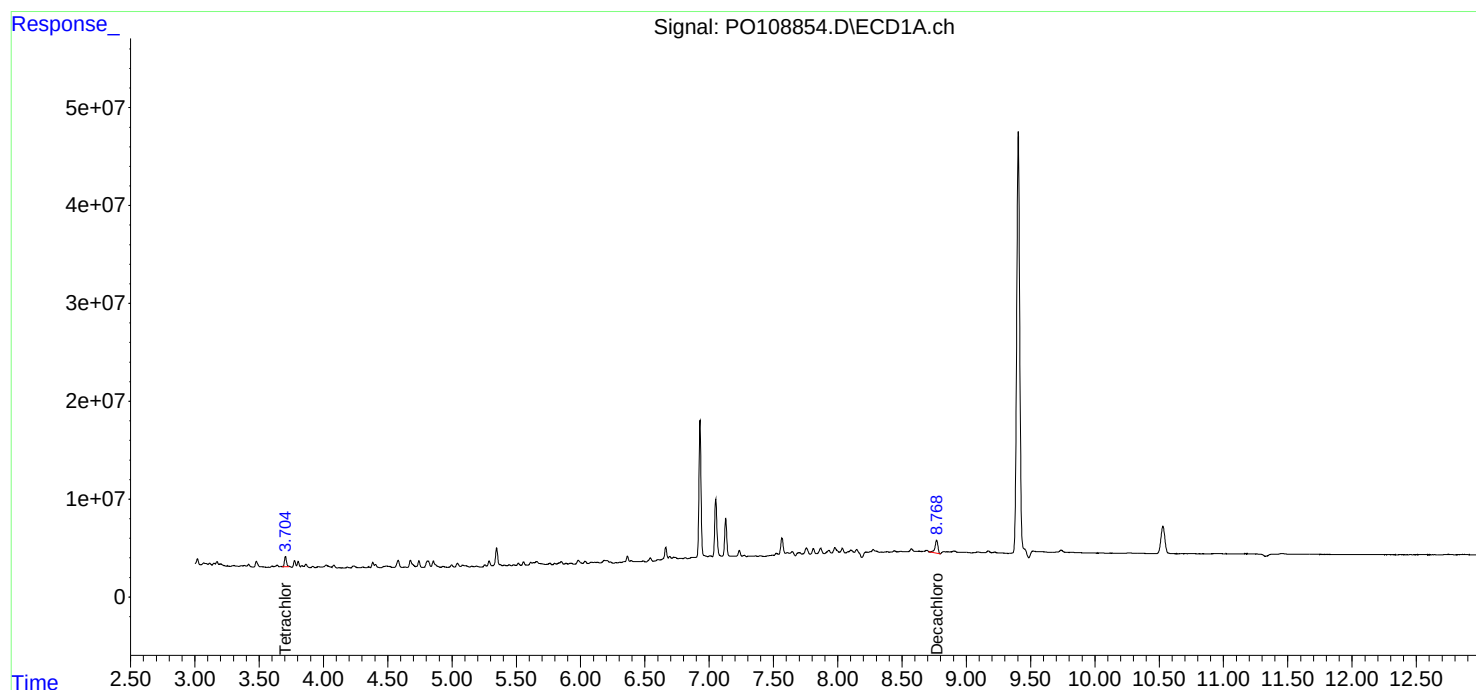

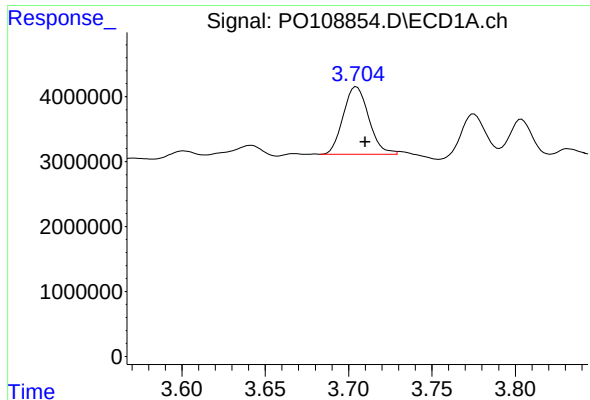


#1 Tetrachloro-m-xylene

R.T.: 3.704 min
Delta R.T.: -0.006 min
Response: 11119286
Conc: 1.28 ng/ml

Instrument :
ECD_O
ClientSampleId :
0827


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/02/2025
Supervised By :Ankita Jodhani 01/02/2025

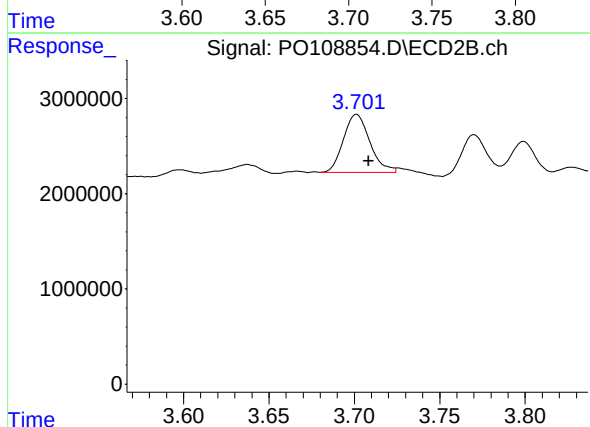


#1 Tetrachloro-m-xylene

R.T.: 3.701 min
Delta R.T.: -0.007 min
Response: 6605592
Conc: 1.30 ng/ml

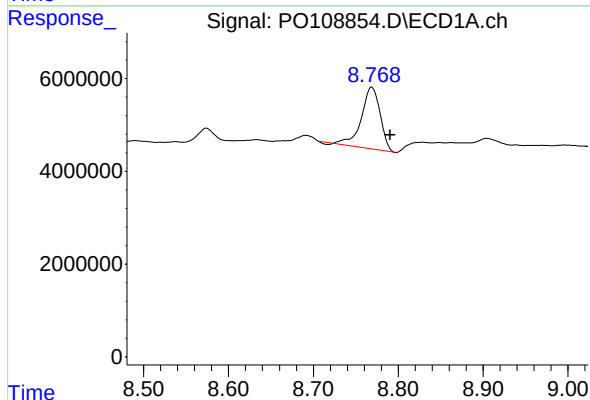

#2 Decachlorobiphenyl

R.T.: 8.769 min
Delta R.T.: -0.022 min
Response: 20440278
Conc: 2.80 ng/ml

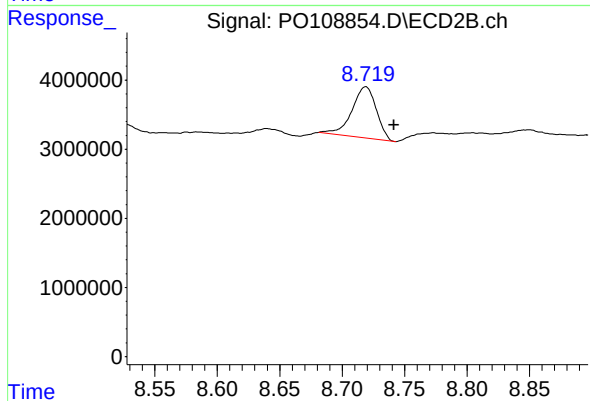

#2 Decachlorobiphenyl

R.T.: 8.719 min
Delta R.T.: -0.022 min
Response: 10058468
Conc: 2.60 ng/ml