

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071519\
 Data File : P0057960.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Jul 2019 10:43
 Operator : SM/AJ
 Sample : K3801-11
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S12-16-B

Manual Integrations
 APPROVED

Ankita
 7/17/2019 9:53:01 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 15 13:42:43 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 24 14:02:43 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.203	3.542	1103722	911125	28.098m	25.912
2)	SA Decachlor...	9.721	8.446	1393118	942603	24.774m	25.199

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071519\
Data File : P0057960.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Jul 2019 10:43
Operator : SM/AJ
Sample : K3801-11
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
S12-16-B


Manual Integrations
APPROVED

Ankita
7/17/2019 9:53:01 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 15 13:42:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062419.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 24 14:02:43 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

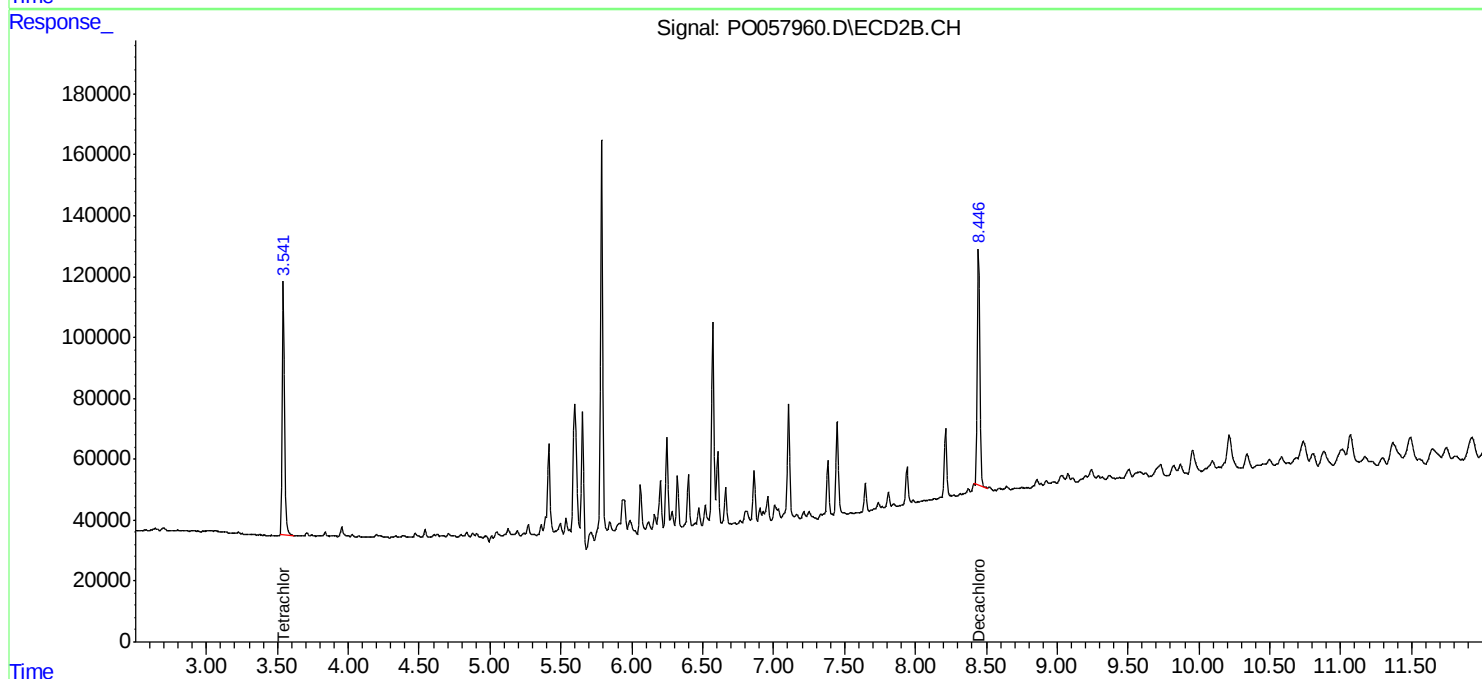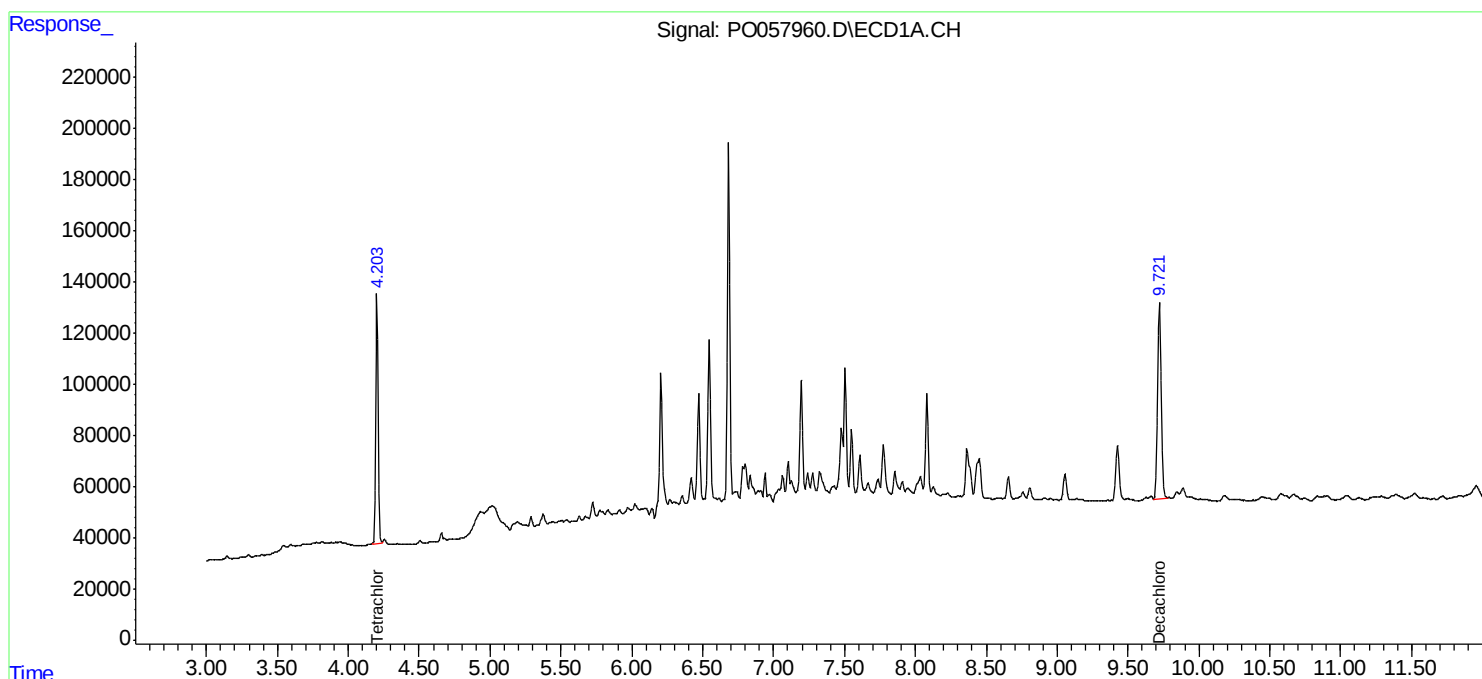

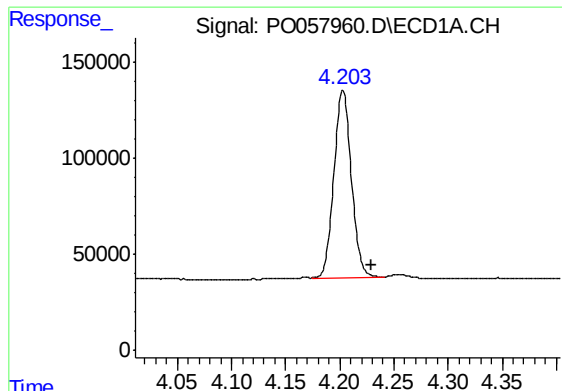


#1 Tetrachloro-m-xylene

R.T.: 4.203 min
Delta R.T.: -0.027 min
Response: 1103722
Conc: 28.10 ng/ml m

Instrument :
ECD_O
ClientSampleId :
S12-16-B


Manual Integrations
APPROVED

Ankita
7/17/2019 9:53:01 AM

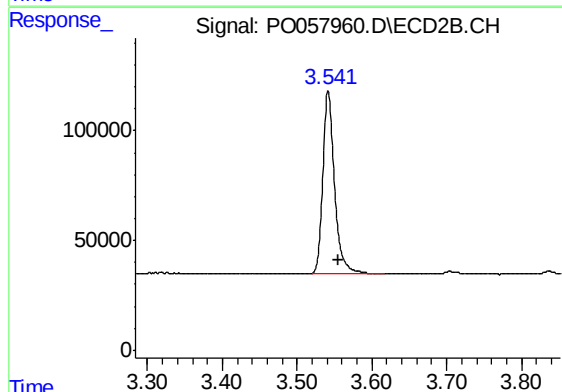


#1 Tetrachloro-m-xylene

R.T.: 3.542 min
Delta R.T.: -0.014 min
Response: 911125
Conc: 25.91 ng/ml

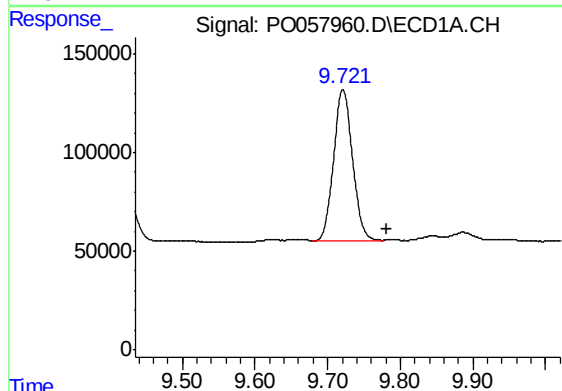

#2 Decachlorobiphenyl

R.T.: 9.721 min
Delta R.T.: -0.061 min
Response: 1393118
Conc: 24.77 ng/ml m

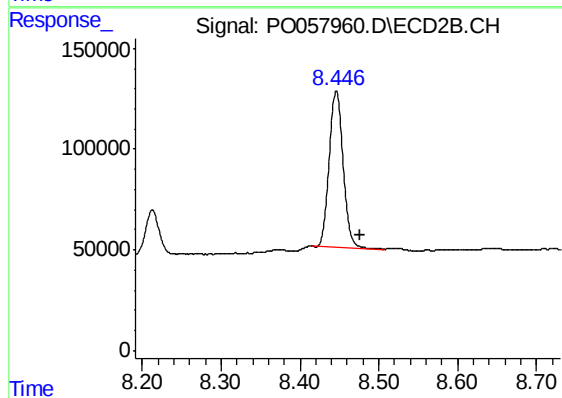

#2 Decachlorobiphenyl

R.T.: 8.446 min
Delta R.T.: -0.031 min
Response: 942603
Conc: 25.20 ng/ml