

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071519\
 Data File : P0057968.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Jul 2019 14:07
 Operator : SM/AJ
 Sample : K3782-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 KY0300F003-SW-190711

Manual Integrations
 APPROVED

Ankita
 7/17/2019 9:53:16 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 16 01:26:06 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 24 14:02:43 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.204	3.544	915921	772989	23.317m	21.983
2)	SA Decachlor...	9.720	8.447	1116878	775895	19.862m	20.742

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO071519\
Data File : PO057968.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Jul 2019 14:07
Operator : SM/AJ
Sample : K3782-03
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
KY030OF003-SW-190711


Manual Integrations
APPROVED

Ankita
7/17/2019 9:53:16 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 16 01:26:06 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO062419.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 24 14:02:43 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

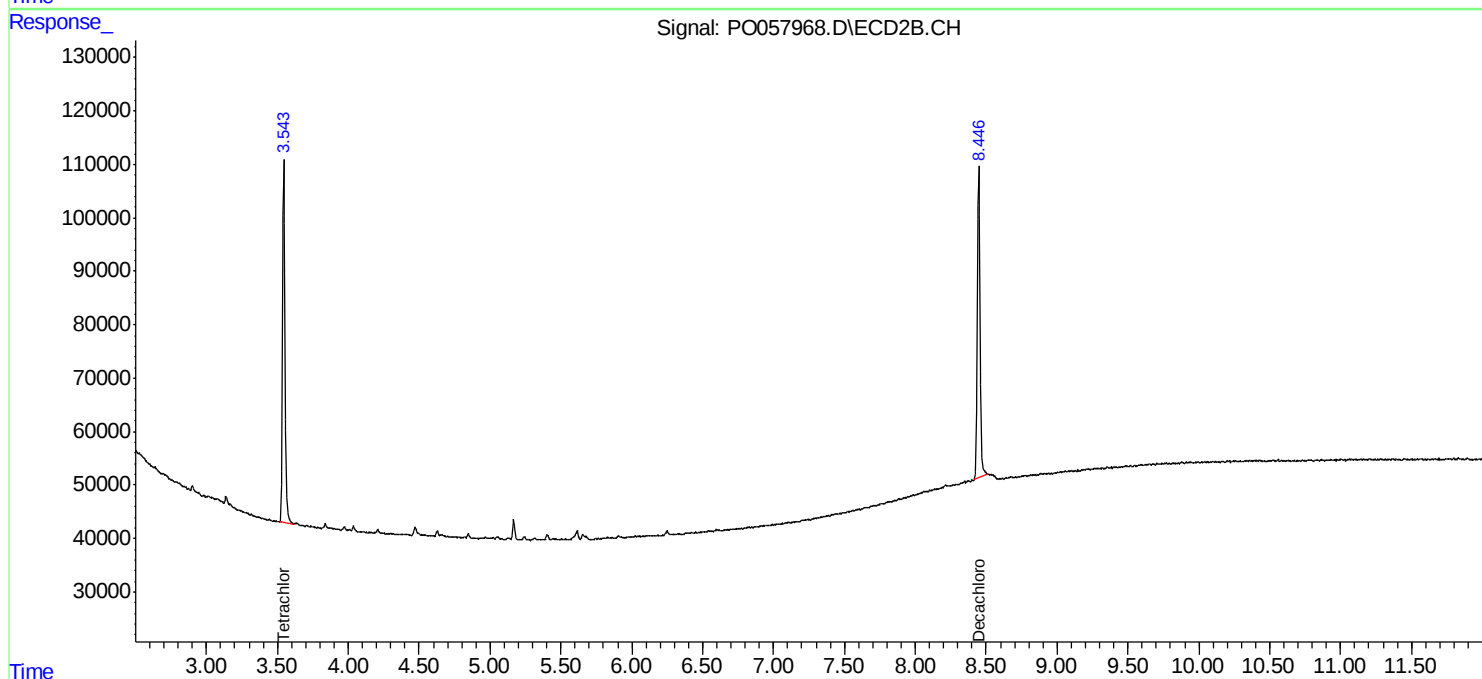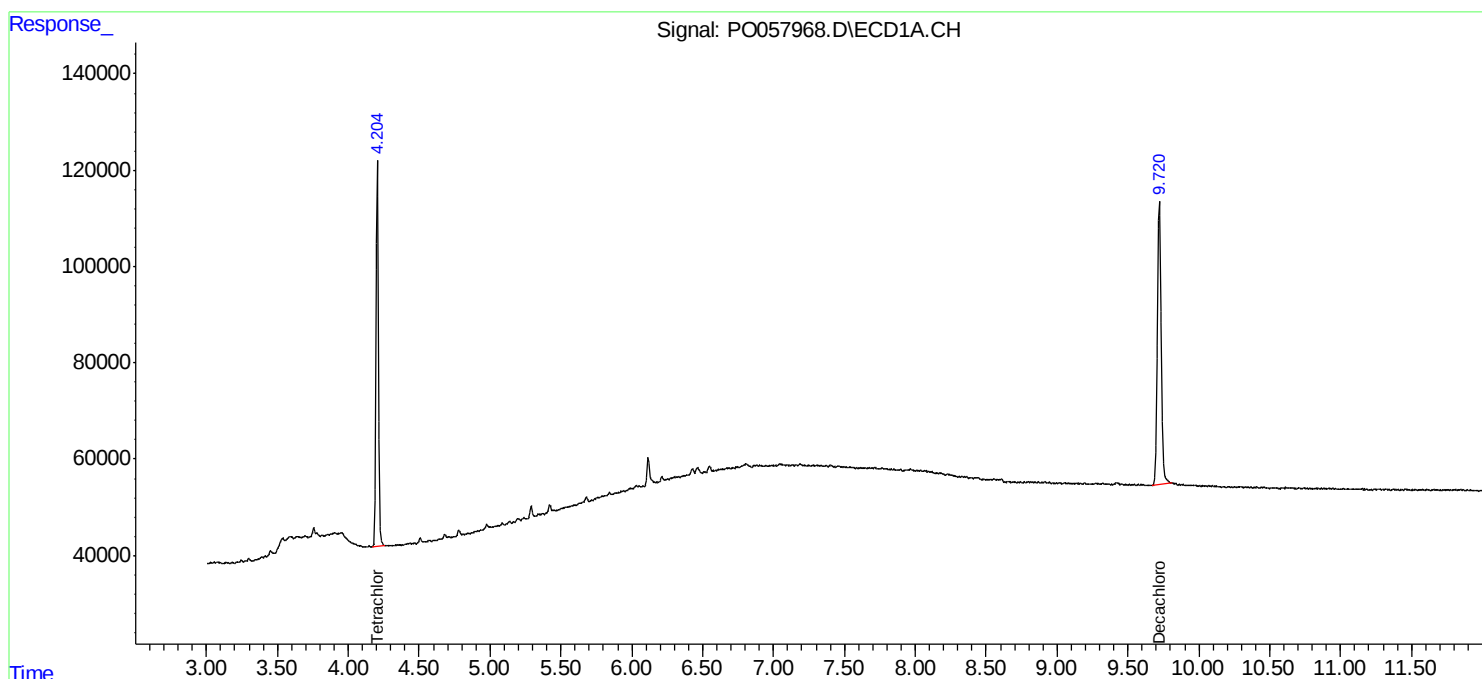

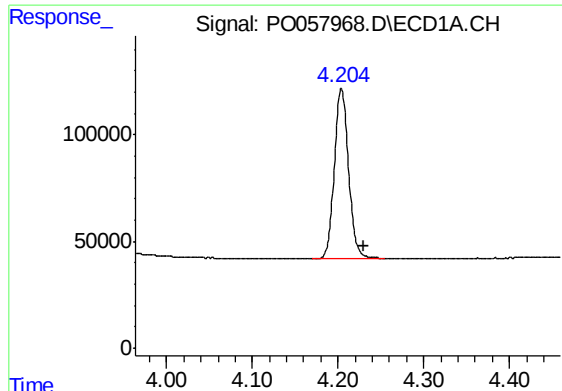


#1 Tetrachloro-m-xylene

R.T.: 4.204 min
Delta R.T.: -0.026 min
Response: 915921
Conc: 23.32 ng/ml m

Instrument :
ECD_O
ClientSampleId :
KY0300F003-SW-190711


Manual Integrations
APPROVED

Ankita
7/17/2019 9:53:16 AM

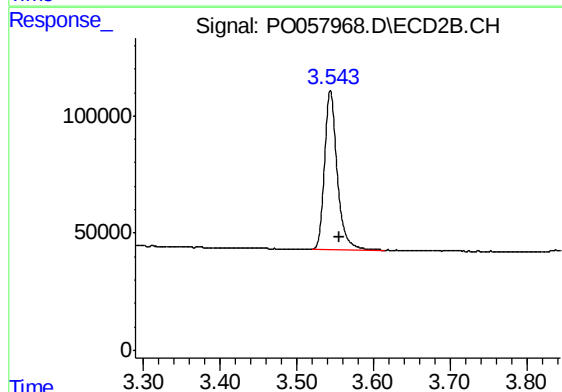


#1 Tetrachloro-m-xylene

R.T.: 3.544 min
Delta R.T.: -0.011 min
Response: 772989
Conc: 21.98 ng/ml

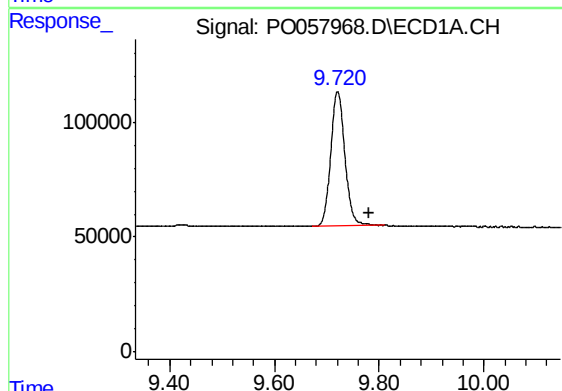

#2 Decachlorobiphenyl

R.T.: 9.720 min
Delta R.T.: -0.061 min
Response: 1116878
Conc: 19.86 ng/ml m

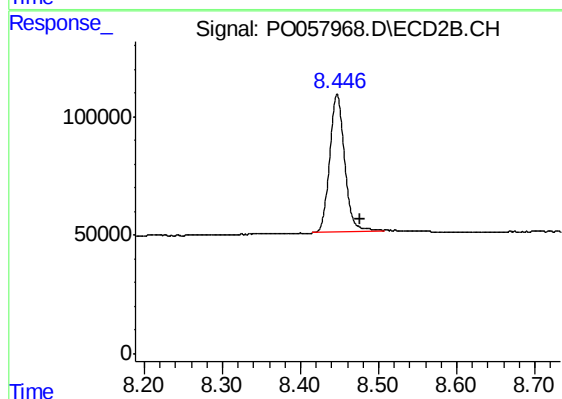

#2 Decachlorobiphenyl

R.T.: 8.447 min
Delta R.T.: -0.030 min
Response: 775895
Conc: 20.74 ng/ml