

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071519\
 Data File : P0057970.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Jul 2019 14:48
 Operator : SM/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Manual Integrations
 APPROVED

Ankita

7/17/2019 9:53:19 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 16 01:26:39 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 24 14:02:43 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.211	3.542	839198	733236	21.364	20.853
2) SA Decachlor...	9.733	8.450	1015740	714821	18.063m	19.109

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO071519\
Data File : PO057970.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Jul 2019 14:48
Operator : SM/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK



Manual Integrations
APPROVED


Ankita

7/17/2019 9:53:19 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 16 01:26:39 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO062419.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 24 14:02:43 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

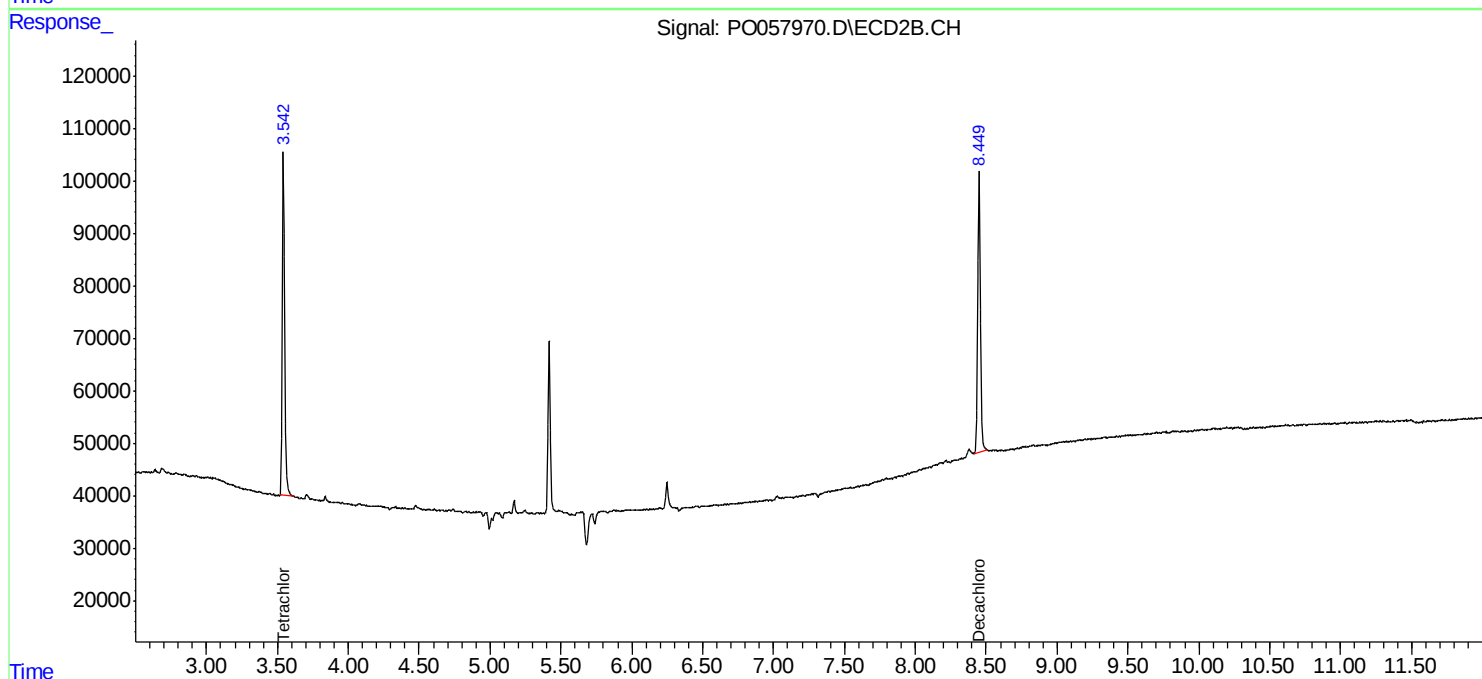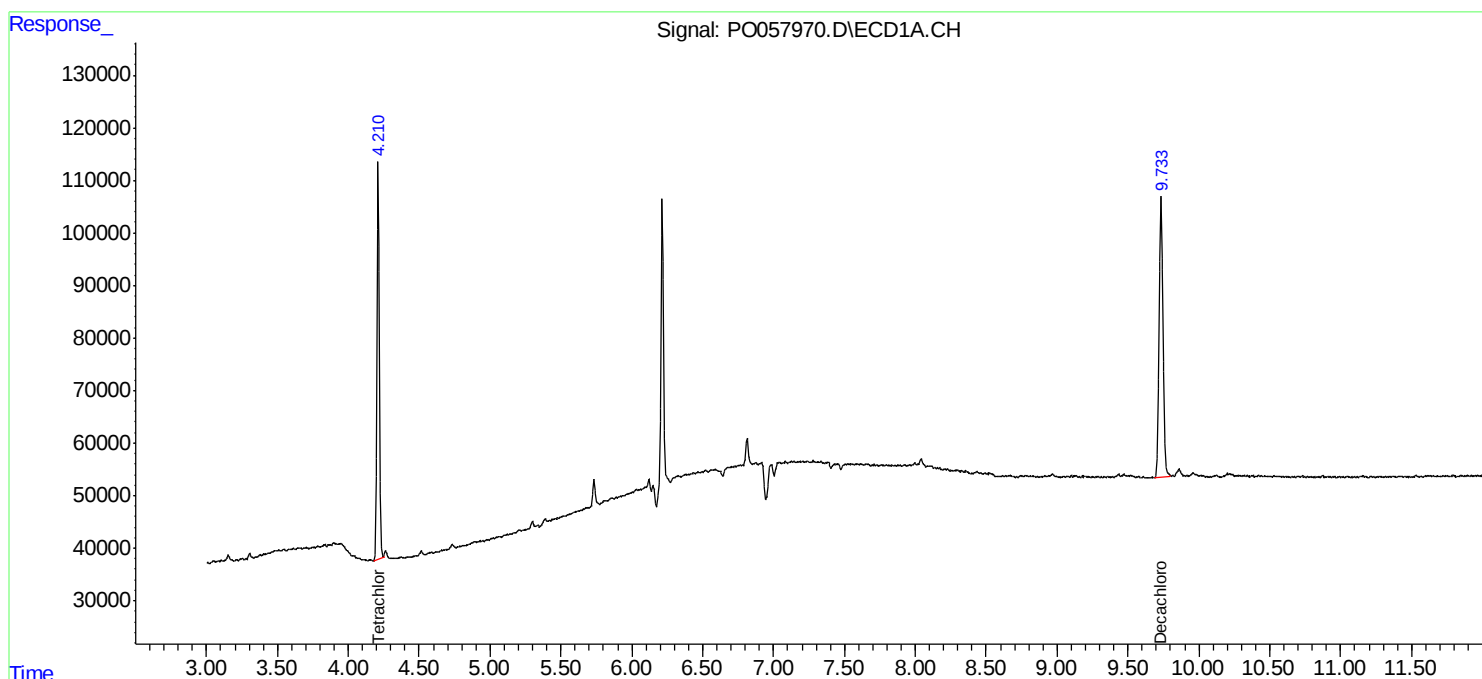

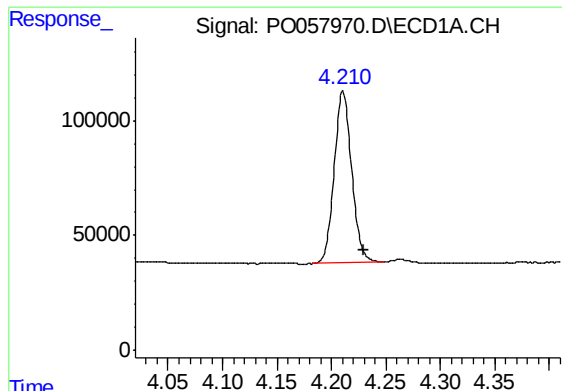

#1 Tetrachloro-m-xylene


R.T.: 4.211 min
Delta R.T.: -0.019 min
Response: 839198
Conc: 21.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

Manual Integrations
APPROVED


Ankita

7/17/2019 9:53:19 AM

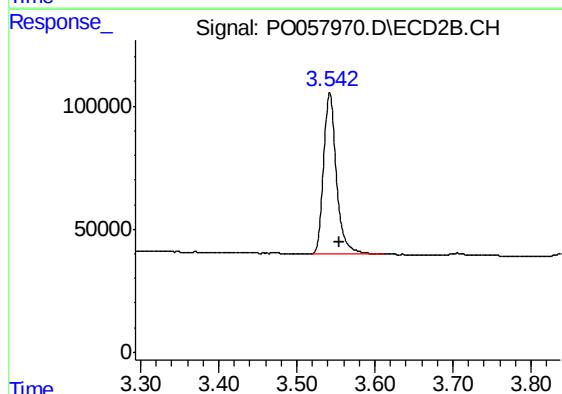


#1 Tetrachloro-m-xylene

R.T.: 3.542 min
Delta R.T.: -0.013 min
Response: 733236
Conc: 20.85 ng/ml

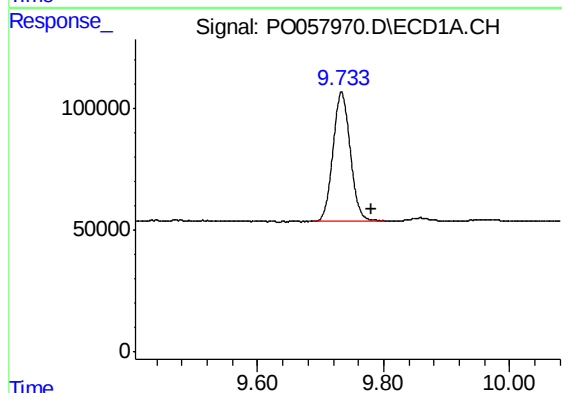

#2 Decachlorobiphenyl

R.T.: 9.733 min
Delta R.T.: -0.049 min
Response: 1015740
Conc: 18.06 ng/ml m

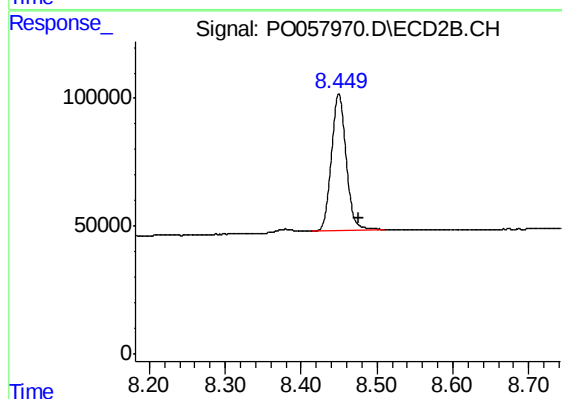

#2 Decachlorobiphenyl

R.T.: 8.450 min
Delta R.T.: -0.027 min
Response: 714821
Conc: 19.11 ng/ml