

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071519\
 Data File : P0057981.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Jul 2019 18:47
 Operator : SM/AJ
 Sample : K3776-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-SF-01-006-A

Manual Integrations
 APPROVED

Ankita

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 16 01:30:14 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 24 14:02:43 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

7/17/2019 9:53:39 AM

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.204	3.544	991132	821659	25.231m	23.367
2)	SA Decachlor...	9.724	8.449	1018374	599850	18.110m	16.036m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO071519\
Data File : PO057981.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Jul 2019 18:47
Operator : SM/AJ
Sample : K3776-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FK-SF-01-006-A



Manual Integrations
APPROVED


Ankita

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 16 01:30:14 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO062419.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 24 14:02:43 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

7/17/2019 9:53:39 AM

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

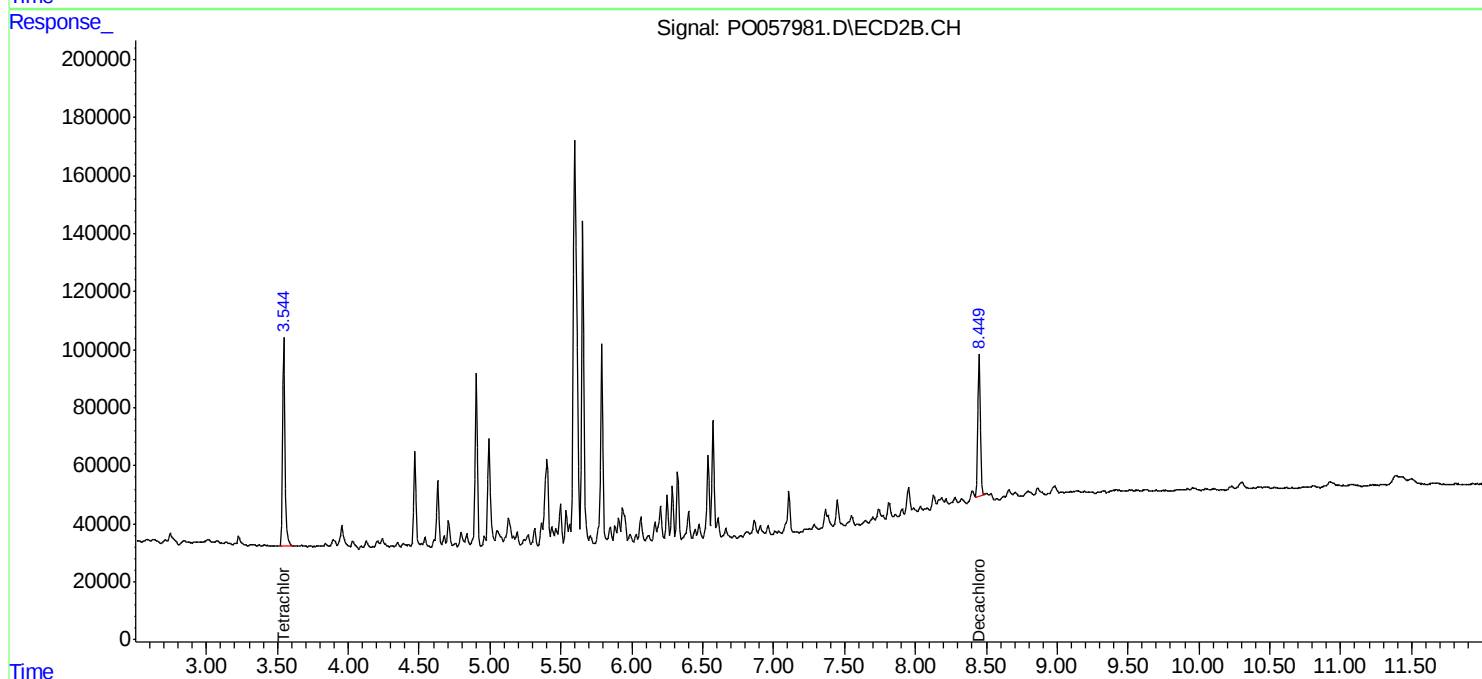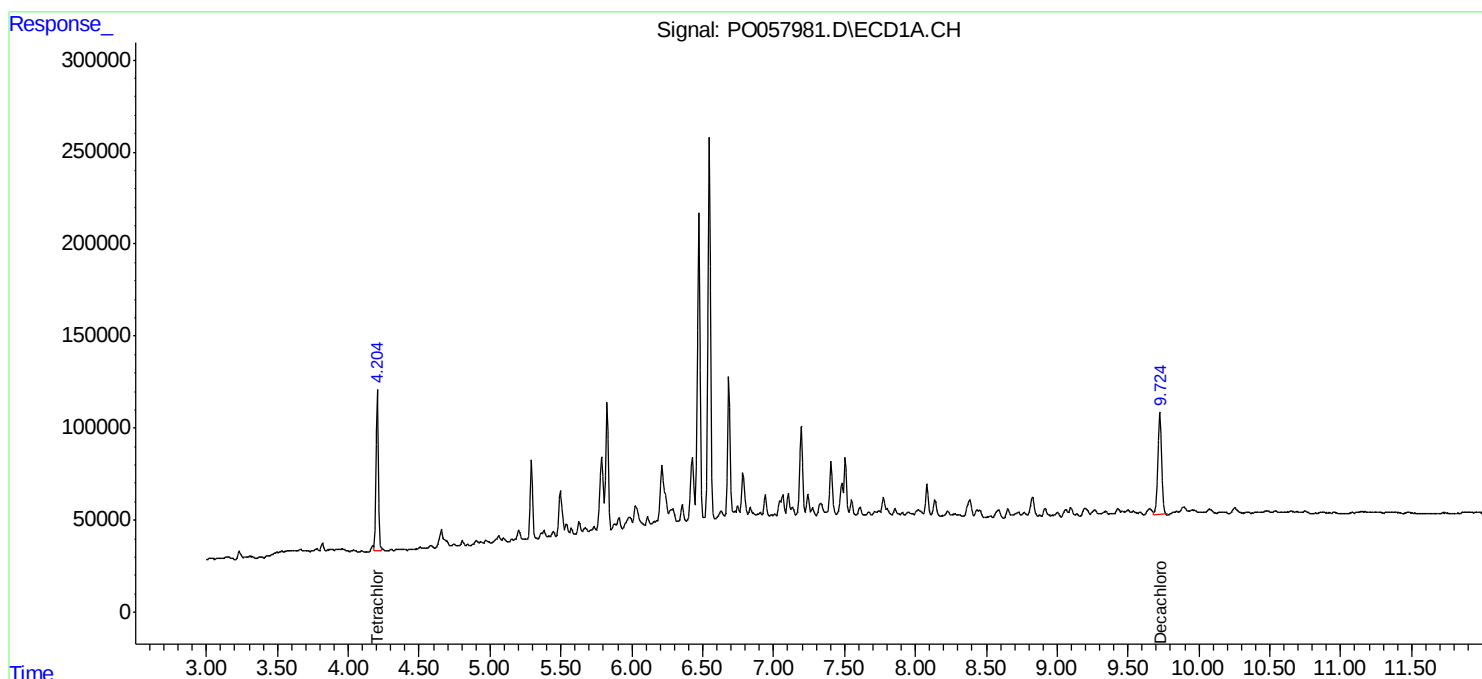

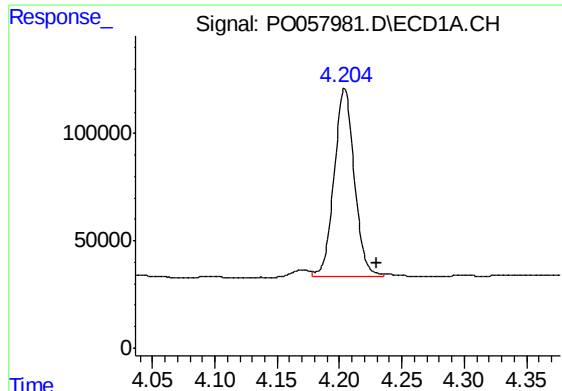

#1 Tetrachloro-m-xylene


R.T.: 4.204 min
Delta R.T.: -0.026 min
Response: 991132
Conc: 25.23 ng/ml m

Instrument :
ECD_O
ClientSampleId :
FK-SF-01-006-A

Manual Integrations
APPROVED


Ankita

7/17/2019 9:53:39 AM

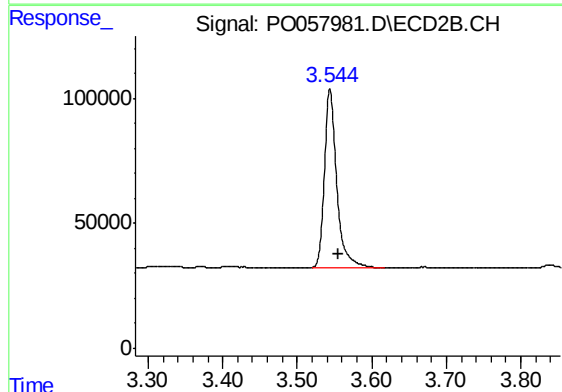


#1 Tetrachloro-m-xylene

R.T.: 3.544 min
Delta R.T.: -0.011 min
Response: 821659
Conc: 23.37 ng/ml

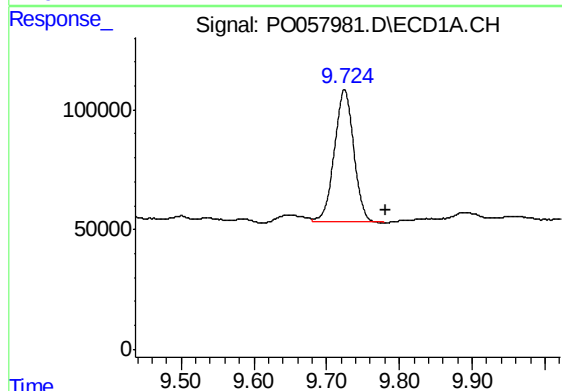

#2 Decachlorobiphenyl

R.T.: 9.724 min
Delta R.T.: -0.057 min
Response: 1018374
Conc: 18.11 ng/ml m

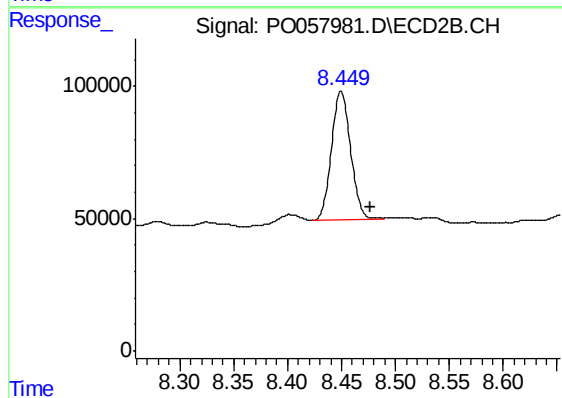

#2 Decachlorobiphenyl

R.T.: 8.449 min
Delta R.T.: -0.028 min
Response: 599850
Conc: 16.04 ng/ml m