

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071924\
 Data File : P0104855.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jul 2024 10:53
 Operator : YP/AJ
 Sample : P3282-04RE
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 IDW-T1-01RE

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/22/2024
 Supervised By :Ankita Jodhani 07/22/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 19 12:44:25 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070224.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 02 16:29:20 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.425	3.540	88415699	33766322	9.875m	10.350
2) SA Decachlor...	10.211	8.435	28888642	10475876	4.711m	4.995

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071924\
Data File : P0104855.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jul 2024 10:53
Operator : YP/AJ
Sample : P3282-04RE
Misc :
ALS Vial : 7 Sample Multiplier: 1


Instrument :
ECD_O
ClientSampleId :
IDW-T1-01RE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/22/2024
Supervised By :Ankita Jodhani 07/22/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 19 12:44:25 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070224.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 02 16:29:20 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

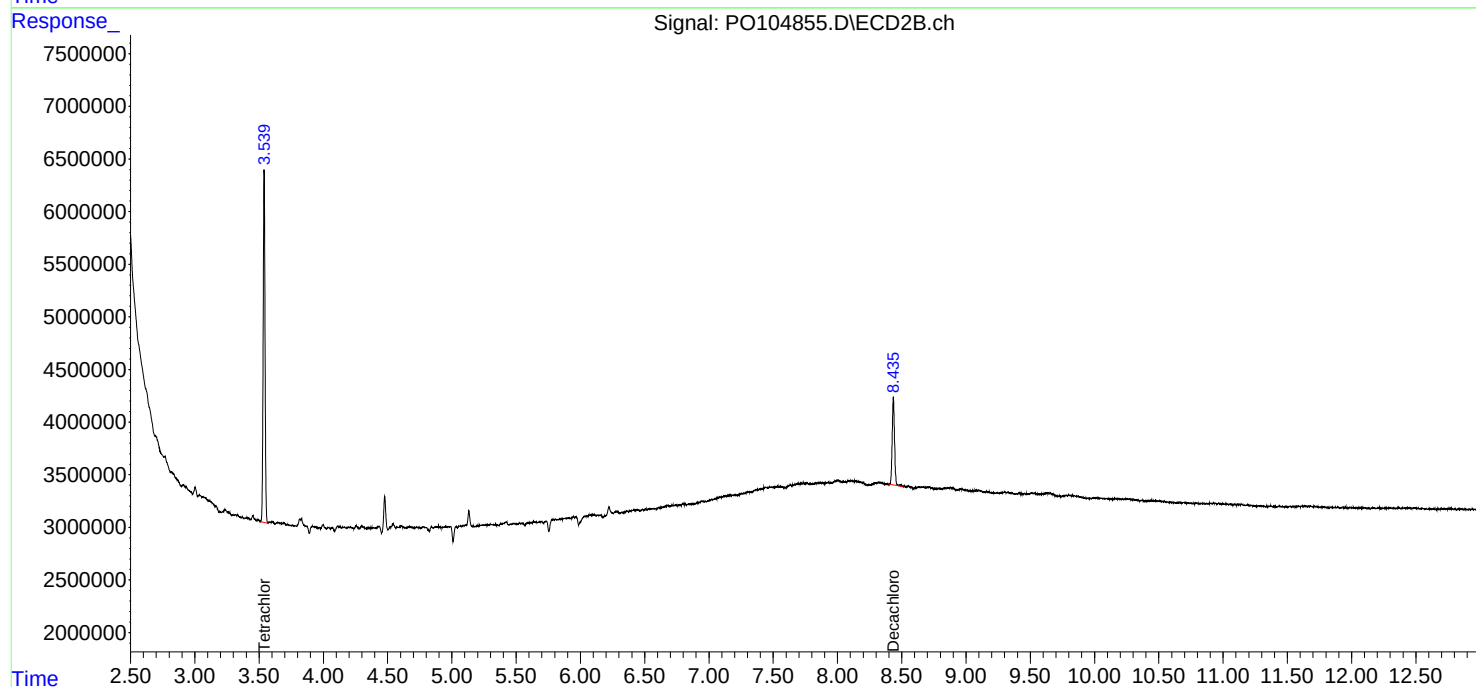

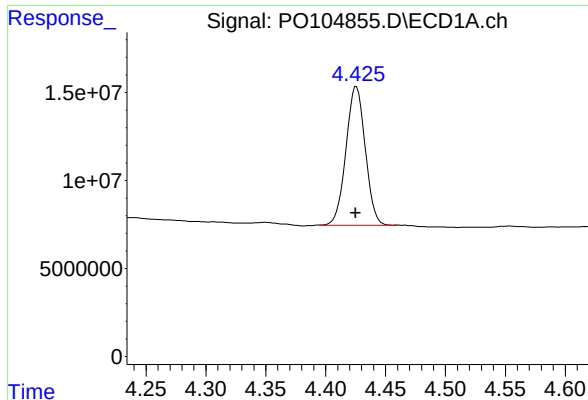


#1 Tetrachloro-m-xylene

R.T.: 4.425 min
Delta R.T.: 0.000 min
Response: 88415699
Conc: 9.88 ng/ml

Instrument :
ECD_O
ClientSampleId :
IDW-T1-01RE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/22/2024
Supervised By :Ankita Jodhani 07/22/2024

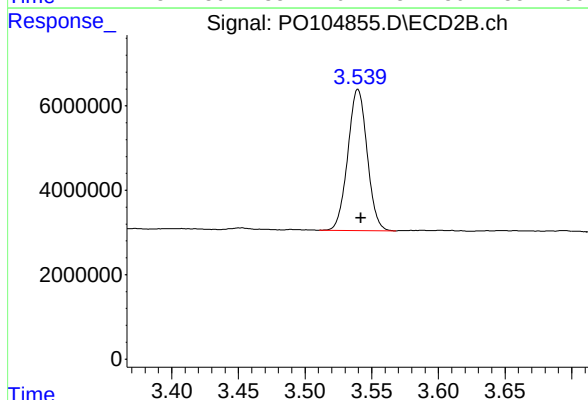


#1 Tetrachloro-m-xylene

R.T.: 3.540 min
Delta R.T.: -0.002 min
Response: 33766322
Conc: 10.35 ng/ml

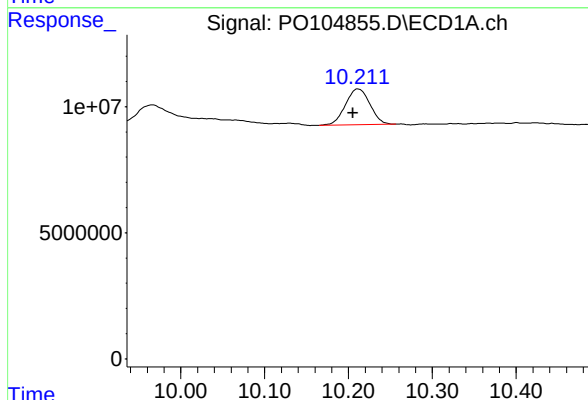

#2 Decachlorobiphenyl

R.T.: 10.211 min
Delta R.T.: 0.005 min
Response: 28888642
Conc: 4.71 ng/ml m

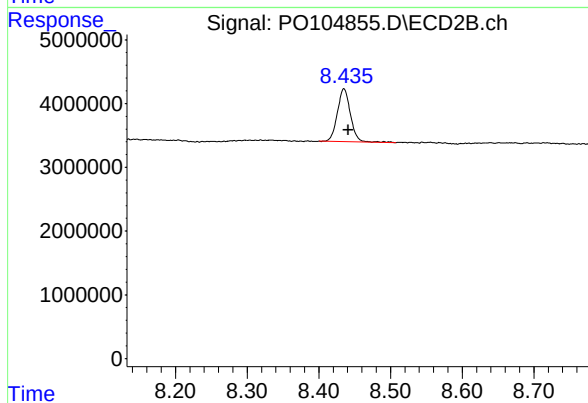

#2 Decachlorobiphenyl

R.T.: 8.435 min
Delta R.T.: -0.006 min
Response: 10475876
Conc: 5.00 ng/ml