

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071924\
 Data File : P0104856.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jul 2024 11:10
 Operator : YP/AJ
 Sample : P3292-01RE
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 703-CRE

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/22/2024
 Supervised By :Ankita Jodhani 07/22/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 19 12:45:01 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070224.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 02 16:29:20 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.426	3.539	53921151	22050329	6.022	6.759
2) SA Decachlor...	10.214	8.437	21195348	6867987	3.456m	3.275

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071924\
Data File : P0104856.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jul 2024 11:10
Operator : YP/AJ
Sample : P3292-01RE
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
703-CRE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/22/2024
Supervised By :Ankita Jodhani 07/22/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 19 12:45:01 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070224.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 02 16:29:20 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

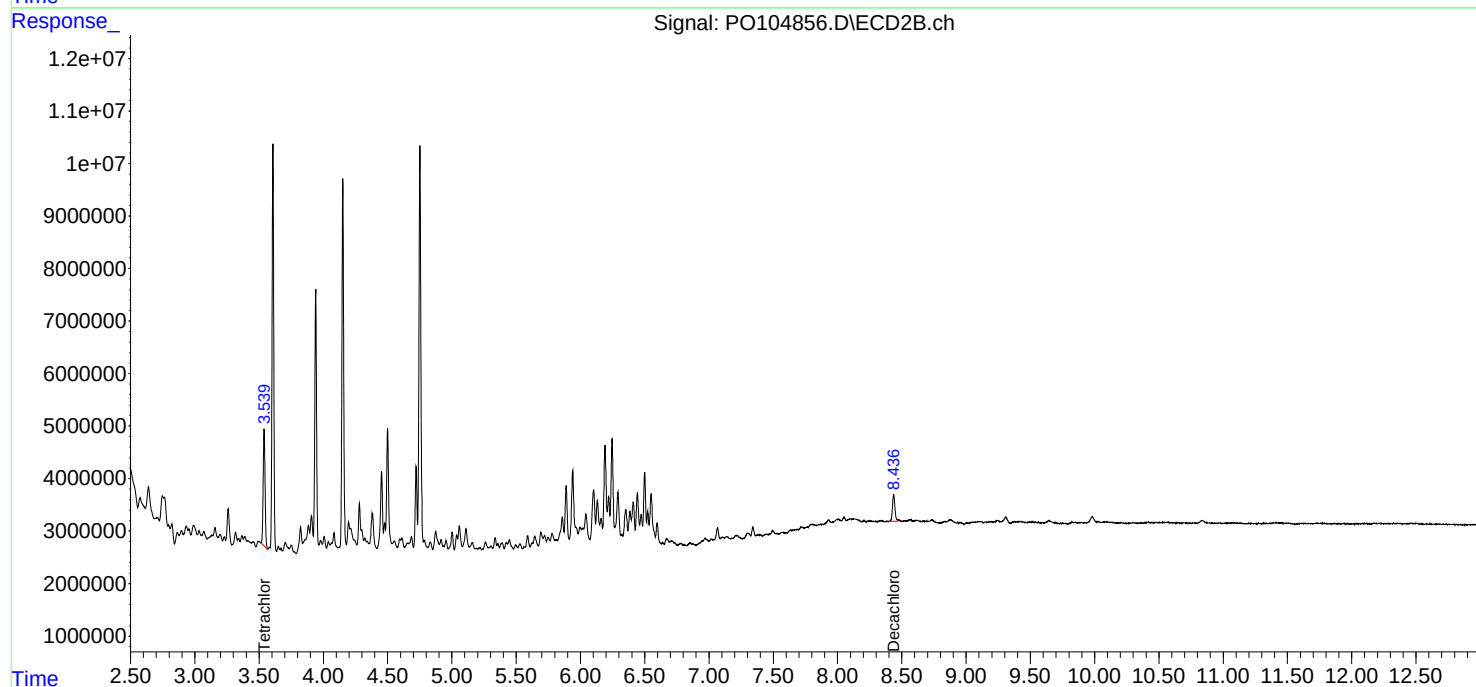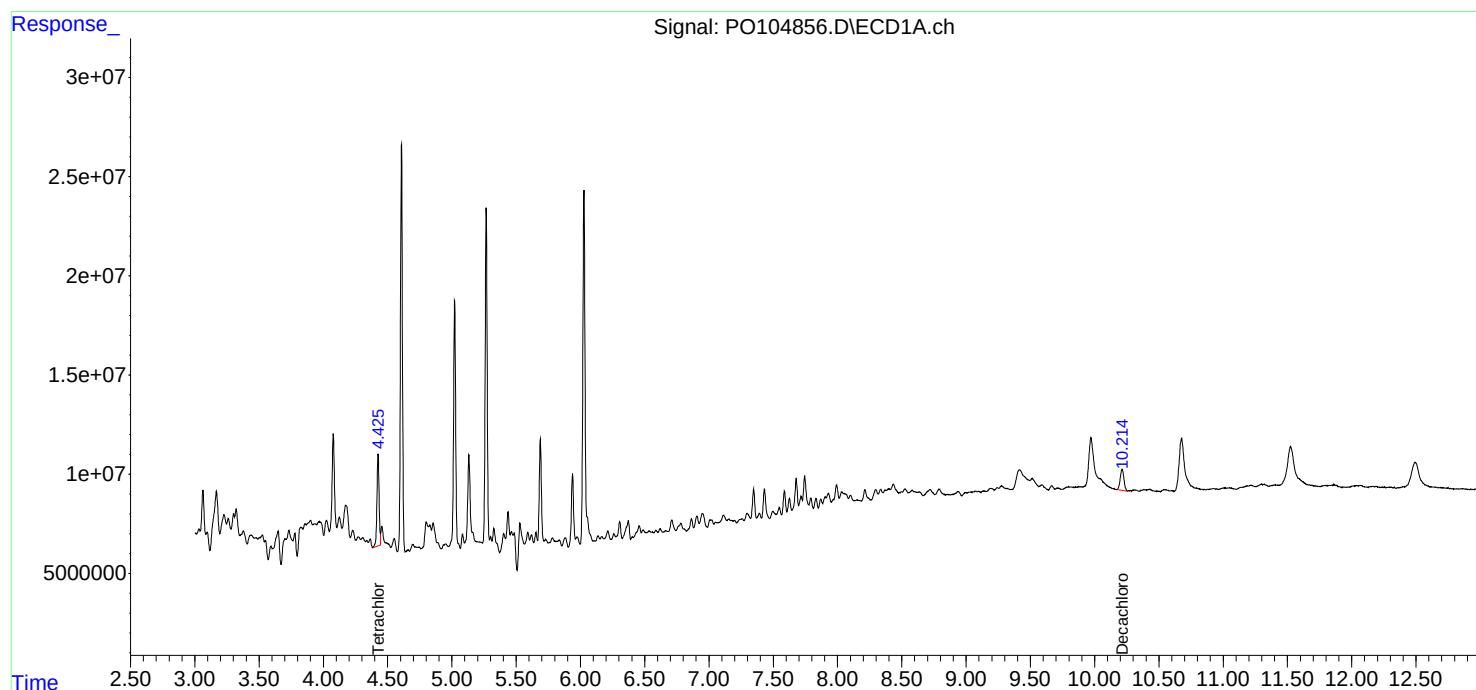

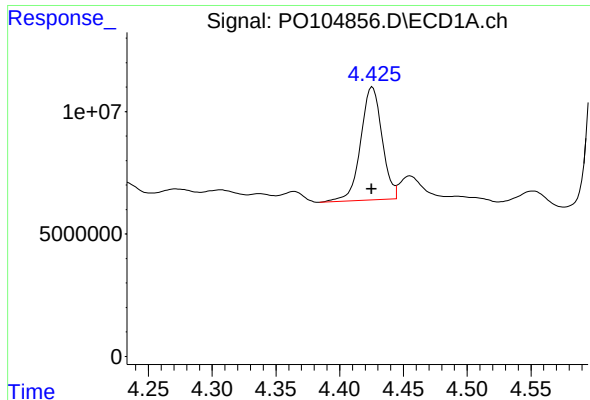


#1 Tetrachloro-m-xylene

R.T.: 4.426 min
Delta R.T.: 0.000 min
Response: 53921151
Conc: 6.02 ng/ml

Instrument :
ECD_O
ClientSampleId :
703-CRE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/22/2024
Supervised By :Ankita Jodhani 07/22/2024

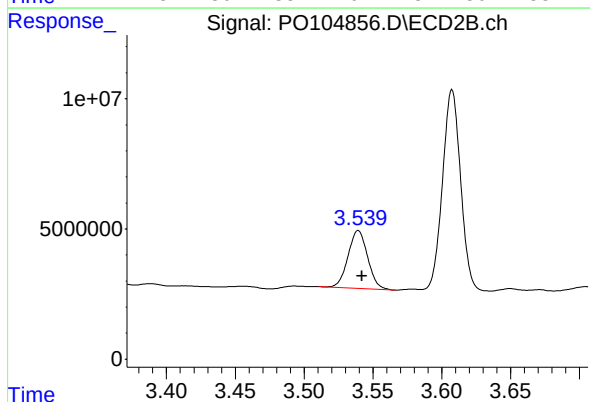


#1 Tetrachloro-m-xylene

R.T.: 3.539 min
Delta R.T.: -0.003 min
Response: 22050329
Conc: 6.76 ng/ml

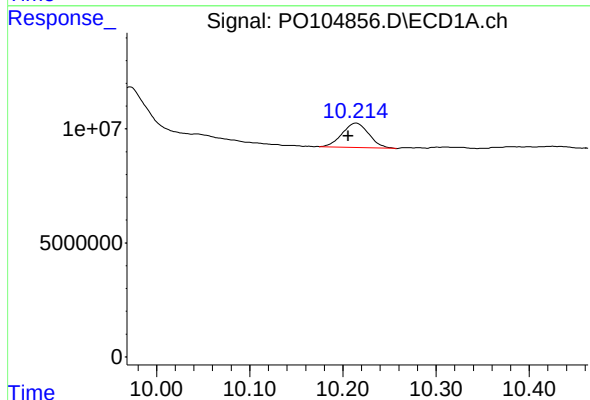

#2 Decachlorobiphenyl

R.T.: 10.214 min
Delta R.T.: 0.008 min
Response: 21195348
Conc: 3.46 ng/ml m

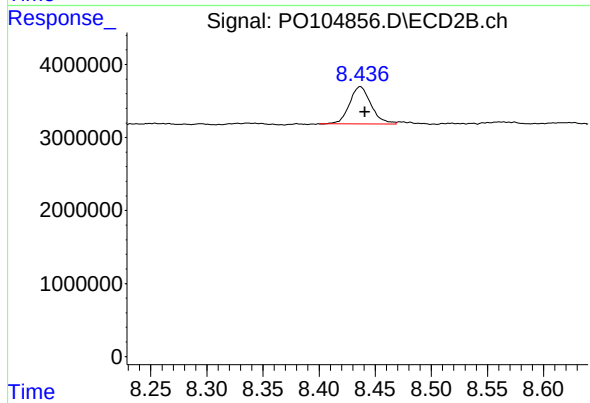

#2 Decachlorobiphenyl

R.T.: 8.437 min
Delta R.T.: -0.004 min
Response: 6867987
Conc: 3.27 ng/ml