

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071924\
 Data File : P0104868.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jul 2024 14:57
 Operator : YP/AJ
 Sample : P3306-02
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 41209

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/22/2024
 Supervised By :Ankita Jodhani 07/22/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 20 00:33:18 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070224.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 02 16:29:20 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.426	3.541	132.0E6	43595144	14.745	13.362
2) SA Decachlor...	10.222	8.448	95523201	23737467	15.576m	11.319m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO071924\
Data File : PO104868.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jul 2024 14:57
Operator : YP/AJ
Sample : P3306-02
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
41209


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/22/2024
Supervised By :Ankita Jodhani 07/22/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 20 00:33:18 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO070224.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 02 16:29:20 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

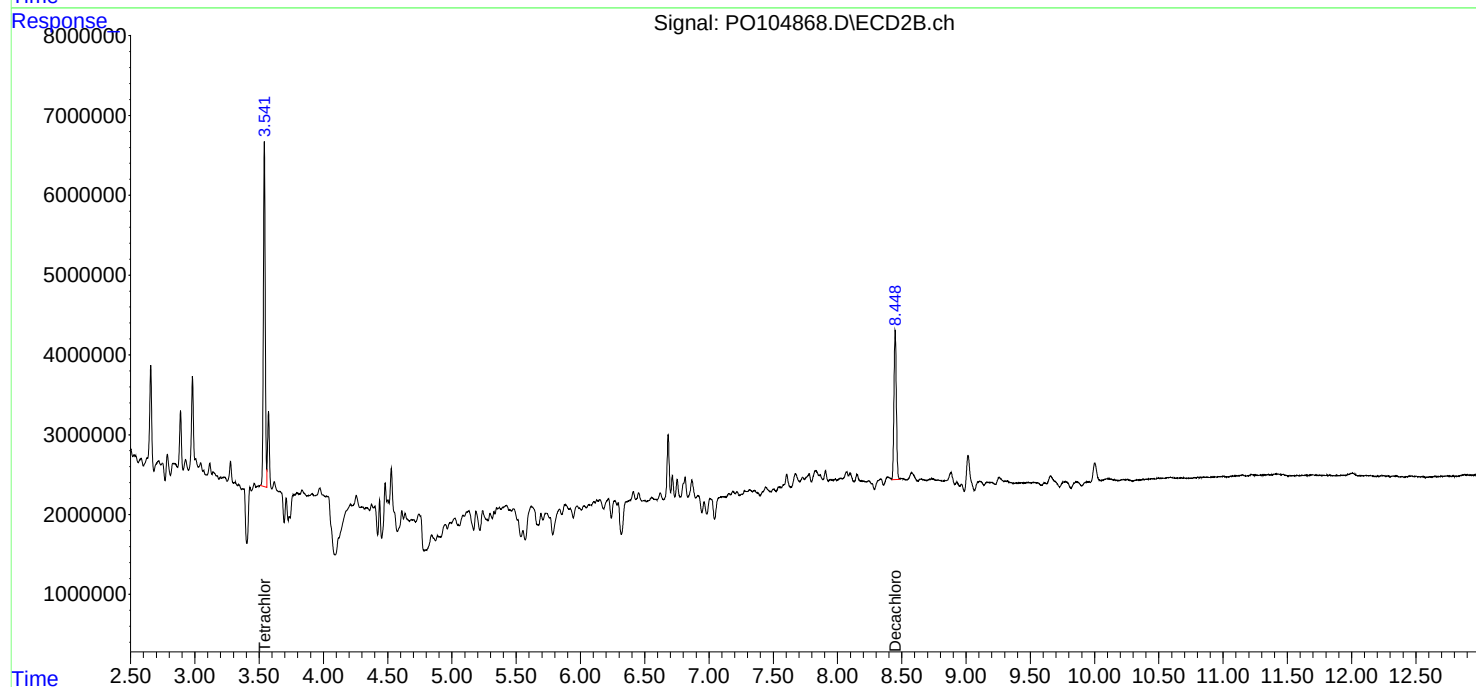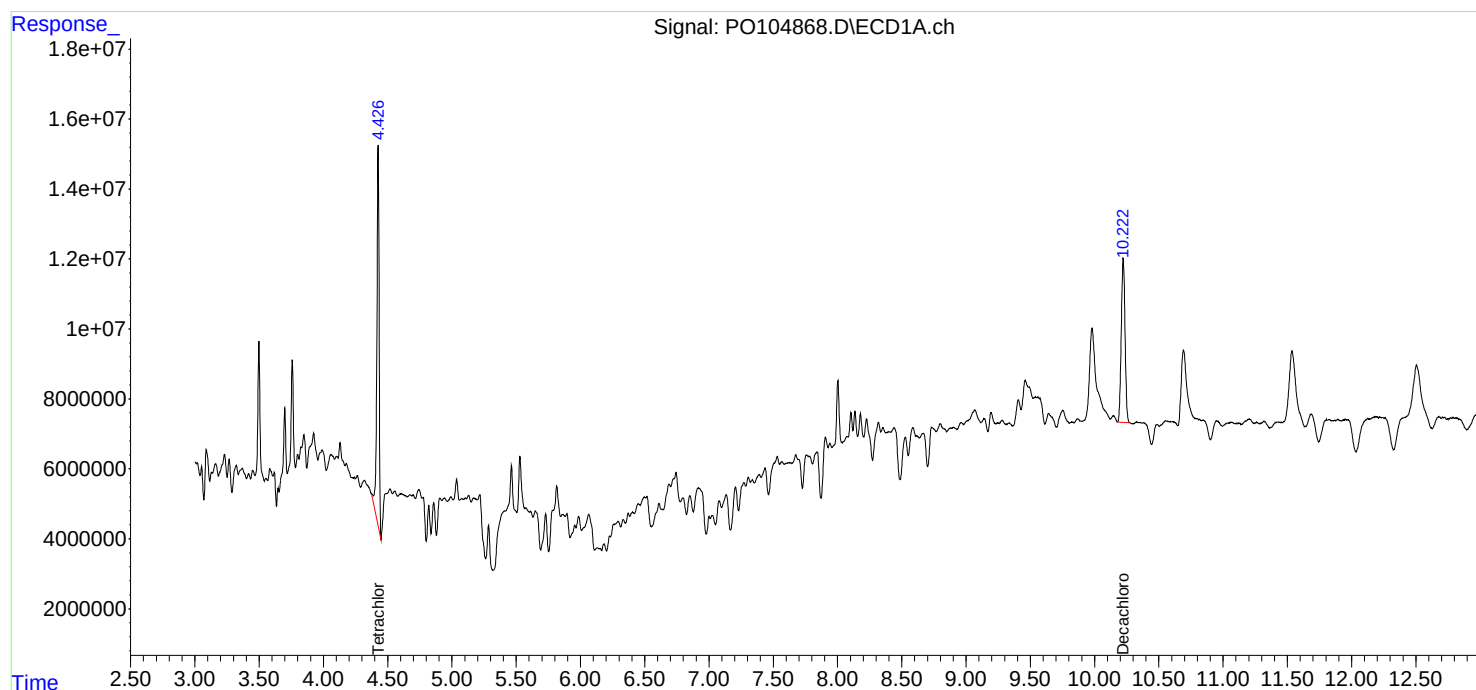

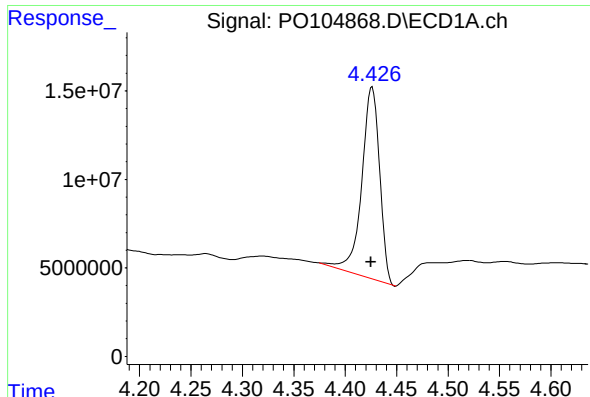

#1 Tetrachloro-m-xylene

R.T.: 4.426 min
Delta R.T.: 0.001 min
Response: 132017555
Conc: 14.74 ng/ml


Instrument :

ECD_O

ClientSampleId :
41209


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/22/2024
Supervised By :Ankita Jodhani 07/22/2024

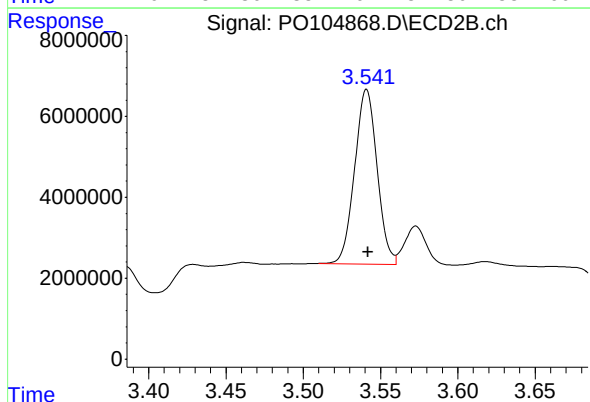


#1 Tetrachloro-m-xylene

R.T.: 3.541 min
Delta R.T.: -0.001 min
Response: 43595144
Conc: 13.36 ng/ml

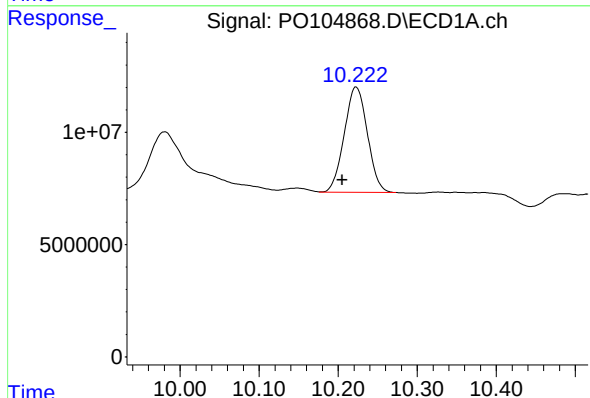

#2 Decachlorobiphenyl

R.T.: 10.222 min
Delta R.T.: 0.016 min
Response: 95523201
Conc: 15.58 ng/ml m

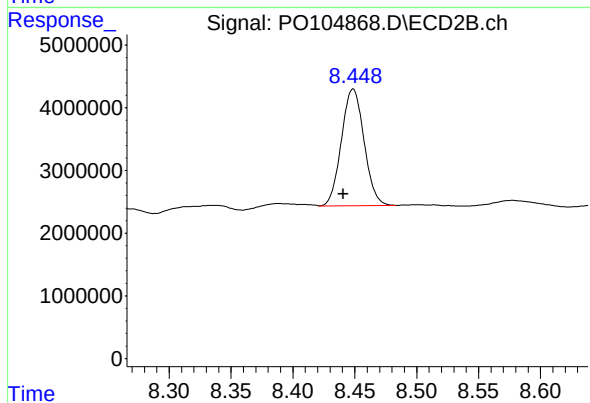

#2 Decachlorobiphenyl

R.T.: 8.448 min
Delta R.T.: 0.008 min
Response: 23737467
Conc: 11.32 ng/ml m