

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082725\
 Data File : P0113267.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Aug 2025 11:02
 Operator : YP/AJ
 Sample : DDT ANALOG
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 DDT ANALOG

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 27 13:34:52 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 19 06:08:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	0.000	3.652	0	43717	N.D.	0.009 #
2)	SA Decachlor...	8.678	8.642	632290	16513	0.091	0.009 #
Target Compounds							
3)	L1 AR-1016-1	4.747	4.733	625368	122629	2.342	0.719 #
4)	L1 AR-1016-2	4.764	4.748	81969	7597	0.204	0.029 #
5)	L1 AR-1016-3	4.837	4.921	602849	285483	2.364	2.045
6)	L1 AR-1016-4	4.946	4.970	4764912	2605060	21.851	22.323
7)	L1 AR-1016-5	5.201	5.175	18785506	1253929	84.761	8.798 #
9)	L2 AR-1221-2	3.967	3.951	415260	191145	6.147	4.095 #
10)	L2 AR-1221-3	4.016	4.023	44416	112023	0.201	0.754 #
11)	L3 AR-1232-1	4.016	4.023	44416	112023	0.255	0.954 #
12)	L3 AR-1232-2	4.497	4.748	281242	7597	2.817	0.062 #
13)	L3 AR-1232-3	4.764	4.921	81969	285483	0.433	4.507 #
14)	L3 AR-1232-4	4.946	5.005	4764912	1206859	50.599	21.466 #
15)	L3 AR-1232-5	5.019	5.175	12963367	1253929	209.279	20.946 #
16)	L4 AR-1242-1	4.747	4.733	625368	122629	2.720	0.849 #
17)	L4 AR-1242-2	4.764	4.748	81969	7597	0.239	0.035 #
18)	L4 AR-1242-3	4.837	4.921	602849	285483	2.717	2.441
19)	L4 AR-1242-4	4.946	5.005	4764912	1206859	27.469	10.259 #
20)	L4 AR-1242-5	5.590	5.518	9700224	3587286	48.462	24.054 #
21)	L5 AR-1248-1	4.747	4.733	625368	122629	3.584	1.100 #
22)	L5 AR-1248-2	5.019	4.970	12963367	2605060	53.597	16.211 #
23)	L5 AR-1248-3	5.201	5.005	18785506	1206859	58.914	7.113 #
24)	L5 AR-1248-4	5.543	5.175	12216434	1253929	24.452	6.294 #
25)	L5 AR-1248-5	5.590	5.572	9700224	2138437	28.405	10.073 #
26)	L6 AR-1254-1	5.543	5.518	12216434	3587286	22.624	11.375 #
27)	L6 AR-1254-2	5.717	5.690	65368652	26583498	132.472	94.826 #
28)	L6 AR-1254-3	6.115	6.086	13121123	22934117	17.758	55.008 #
29)	L6 AR-1254-4	6.329	6.294	2701776	2662252	4.851	9.687 #
30)	L6 AR-1254-5	6.745	6.710	4153.0E6	1830.5E6	5924.551	5120.480
31)	L7 AR-1260-1	6.238	6.199	1447771	6468146	3.246	25.358 #
32)	L7 AR-1260-2	6.423	6.390	14775477	8438964	21.516	24.410
34)	L7 AR-1260-4	7.036	7.003	2528758	336036	5.646	1.621 #
35)	L7 AR-1260-5	7.289	7.248	2843983	826094	2.349	1.764
36)	L8 AR-1262-1	6.829f	6.710f	1112005	1830.5E6	1.214	4415.004 #
37)	L8 AR-1262-2	7.289	7.248	2843983	826094	1.881	1.596
38)	L8 AR-1262-3	7.583	7.541	10348963	3104217	18.677	17.285
39)	L8 AR-1262-4	7.623	7.633	5628704	316306	5.756	1.091 #
40)	L8 AR-1262-5	8.133	8.107	637422	115922	1.529	1.070 #
41)	L9 AR-1268-1	7.583	7.541	10348963	3104217	6.014	6.093
42)	L9 AR-1268-2	7.623	7.633	5628704	316306	3.887	0.761 #
43)	L9 AR-1268-3	7.858	7.814	165936	-41056	0.138	N.D. #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082725\
 Data File : P0113267.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Aug 2025 11:02
 Operator : YP/AJ
 Sample : DDT ANALOG
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 DDT ANALOG

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 27 13:34:52 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 19 06:08:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
44) L9	AR-1268-4	8.133	8.107	637422	115922	1.384	0.963 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO082725\
Data File : PO113267.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Aug 2025 11:02
Operator : YP/AJ
Sample : DDT ANALOG
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 27 13:34:52 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 19 06:08:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

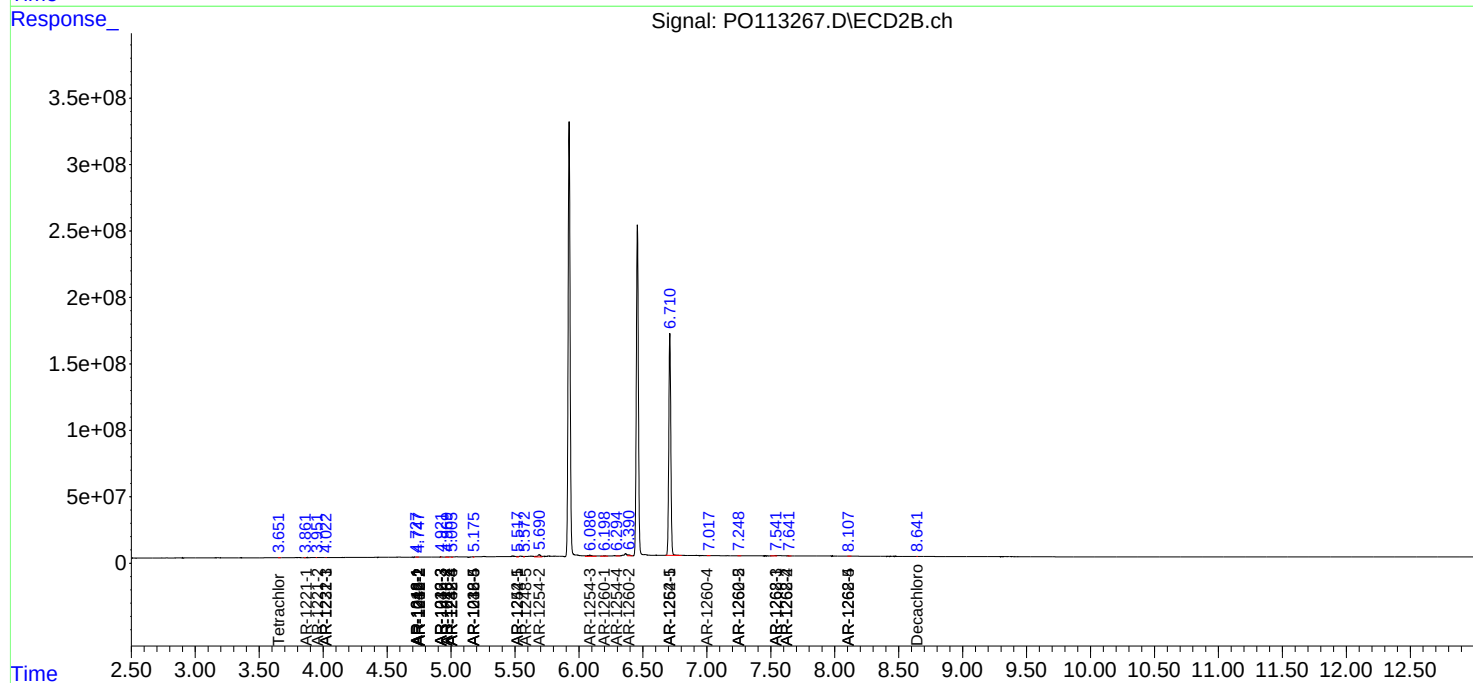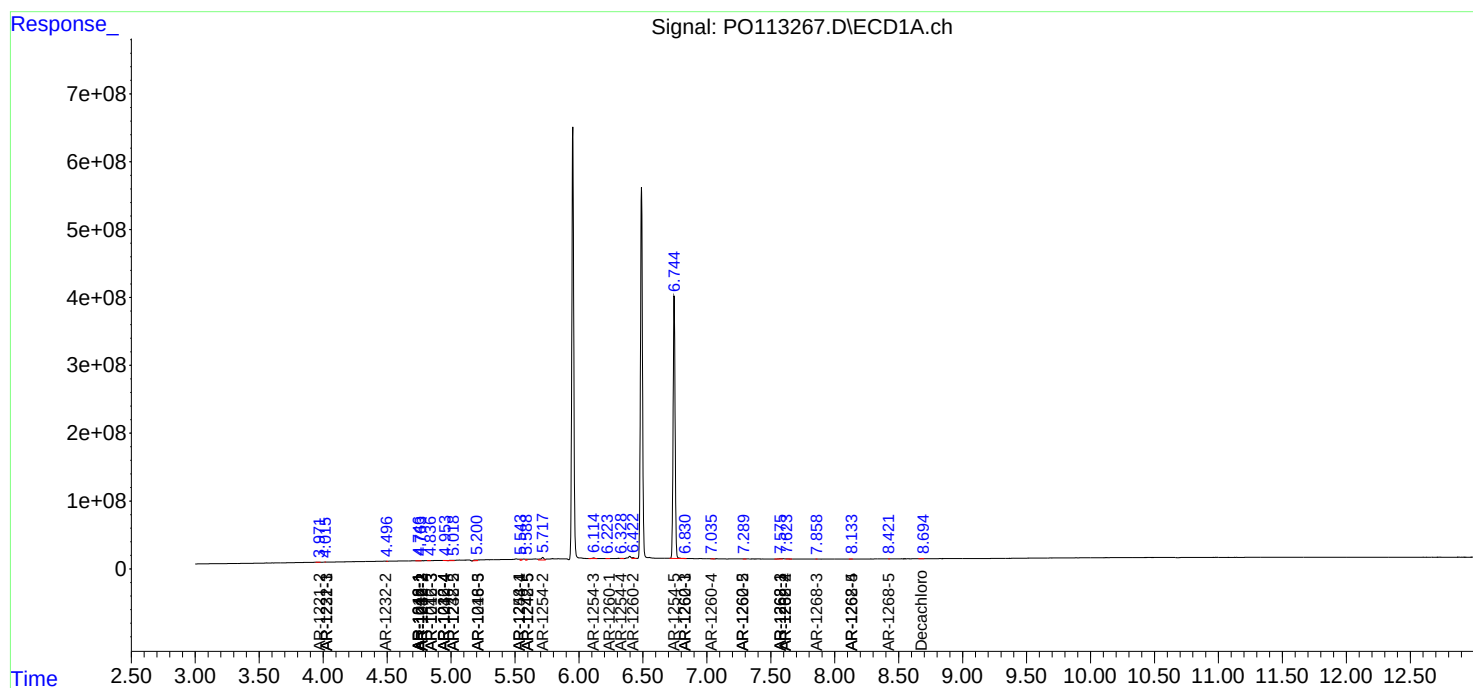


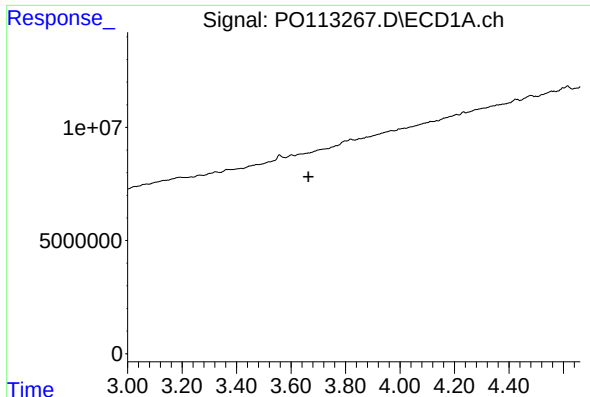

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.663 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

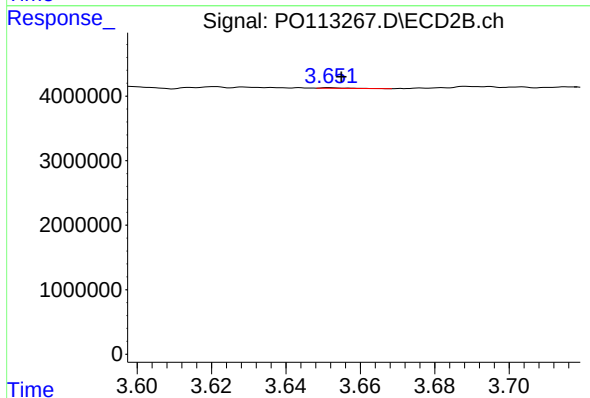


#1 Tetrachloro-m-xylene

R.T.: 3.652 min
Delta R.T.: -0.003 min
Response: 43717
Conc: 0.01 ng/ml

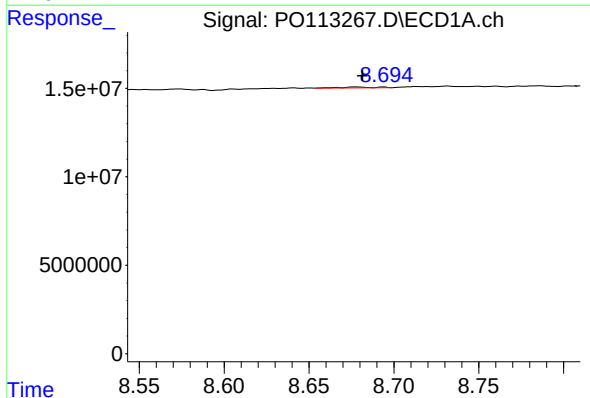


#2 Decachlorobiphenyl

R.T.: 8.678 min
Delta R.T.: -0.004 min
Response: 632290
Conc: 0.09 ng/ml

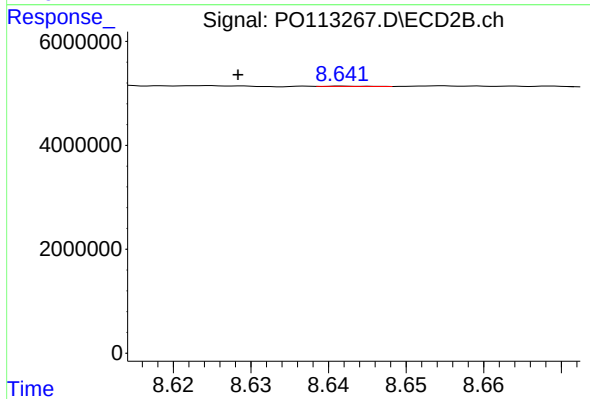

#2 Decachlorobiphenyl


R.T.: 8.642 min
Delta R.T.: 0.014 min
Response: 16513
Conc: 0.01 ng/ml

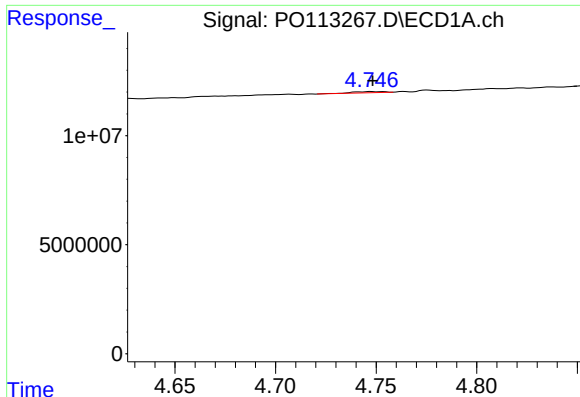

#3 AR-1016-1


R.T.: 4.747 min
Delta R.T.: 0.000 min
Response: 625368
Conc: 2.34 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

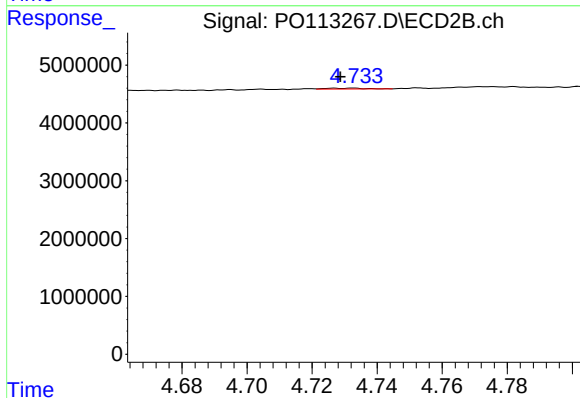


#3 AR-1016-1

R.T.: 4.733 min
Delta R.T.: 0.004 min
Response: 122629
Conc: 0.72 ng/ml

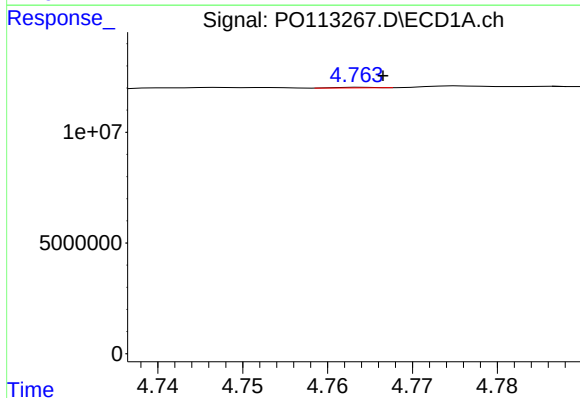


#4 AR-1016-2

R.T.: 4.764 min
Delta R.T.: -0.003 min
Response: 81969
Conc: 0.20 ng/ml

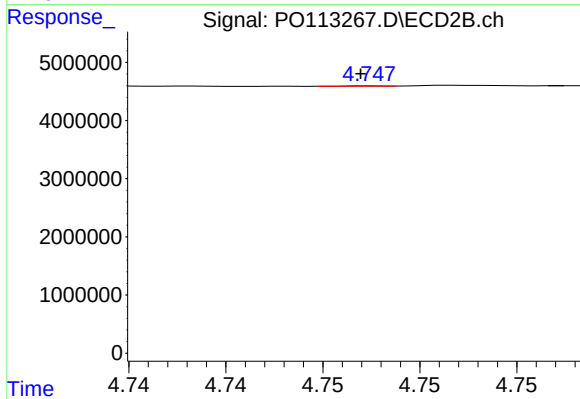

#4 AR-1016-2


R.T.: 4.748 min
Delta R.T.: 0.000 min
Response: 7597
Conc: 0.03 ng/ml

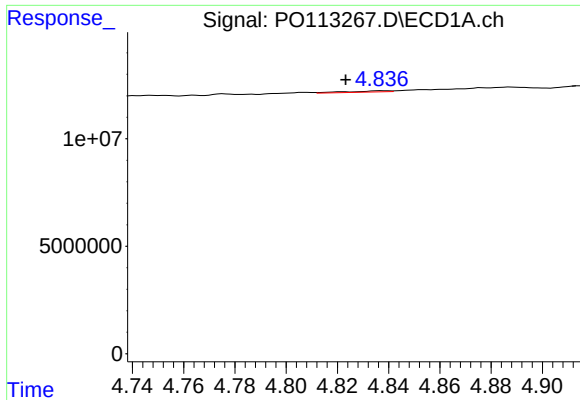

#5 AR-1016-3


R.T.: 4.837 min
Delta R.T.: 0.014 min
Response: 602849
Conc: 2.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

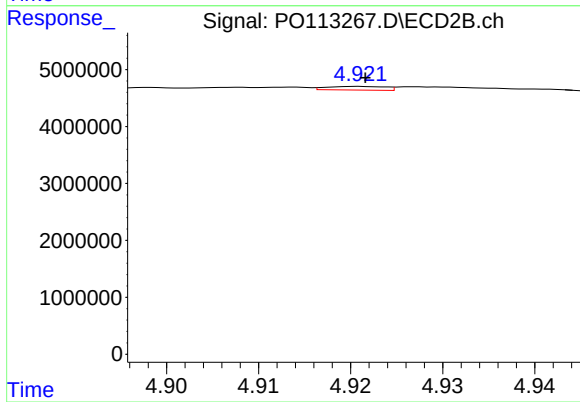


#5 AR-1016-3

R.T.: 4.921 min
Delta R.T.: 0.000 min
Response: 285483
Conc: 2.04 ng/ml

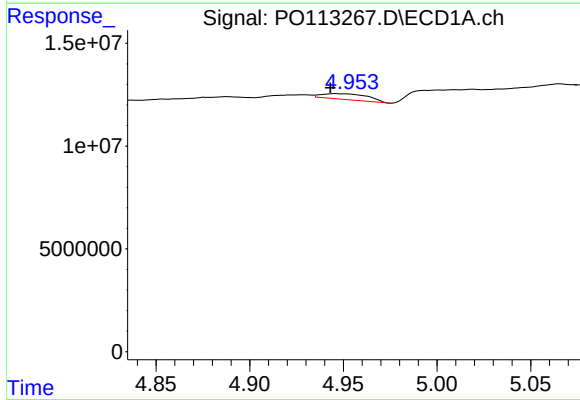


#6 AR-1016-4

R.T.: 4.946 min
Delta R.T.: 0.003 min
Response: 4764912
Conc: 21.85 ng/ml

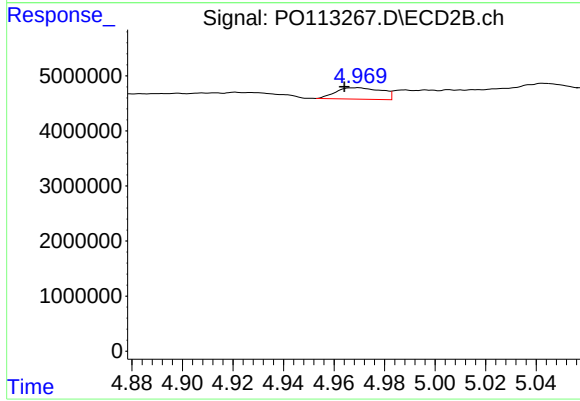

#6 AR-1016-4


R.T.: 4.970 min
Delta R.T.: 0.006 min
Response: 2605060
Conc: 22.32 ng/ml

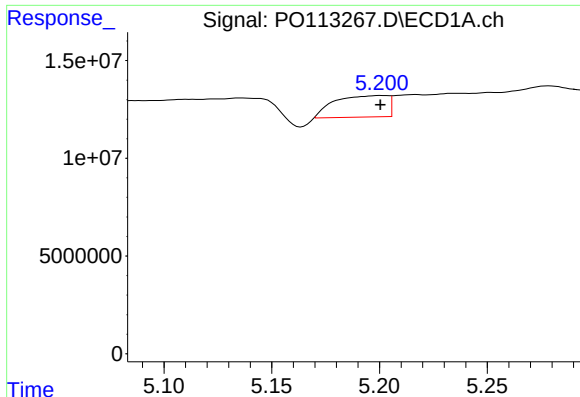

#7 AR-1016-5


R.T.: 5.201 min
Delta R.T.: 0.000 min
Response: 18785506
Conc: 84.76 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

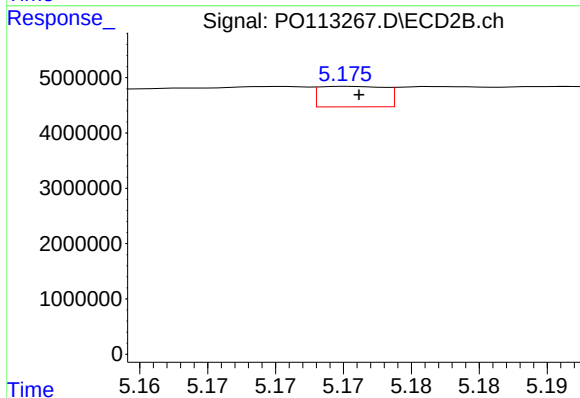


#7 AR-1016-5

R.T.: 5.175 min
Delta R.T.: 0.000 min
Response: 1253929
Conc: 8.80 ng/ml

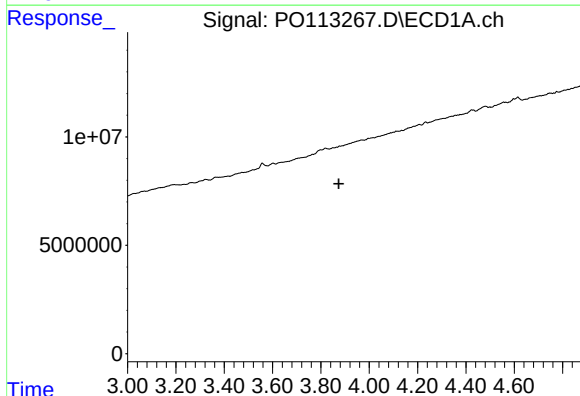


#8 AR-1221-1

R.T.: 3.877 min
Delta R.T.: 0.003 min
Response: -108913
Conc: N.D.

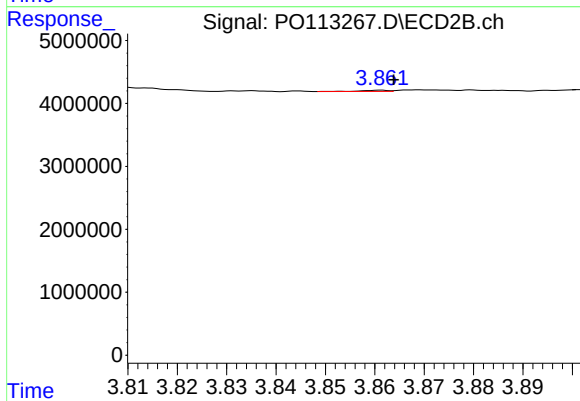

#8 AR-1221-1


R.T.: 3.861 min
Delta R.T.: -0.003 min
Response: 73401
Conc: 1.16 ng/ml

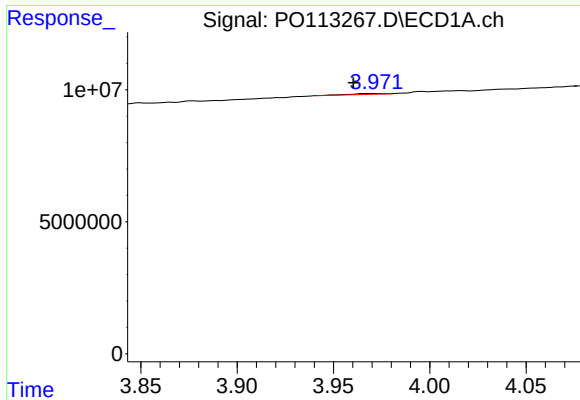

#9 AR-1221-2


R.T.: 3.967 min
Delta R.T.: 0.007 min
Response: 415260
Conc: 6.15 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

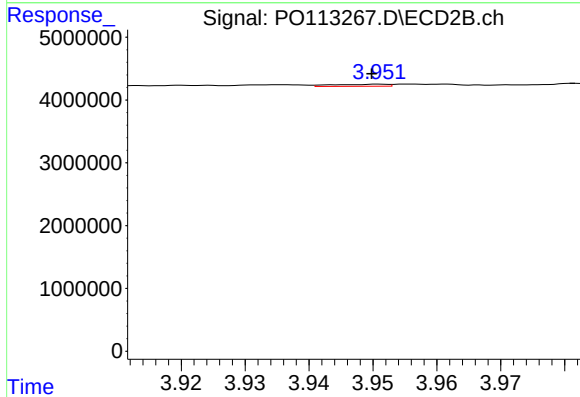


#9 AR-1221-2

R.T.: 3.951 min
Delta R.T.: 0.001 min
Response: 191145
Conc: 4.10 ng/ml

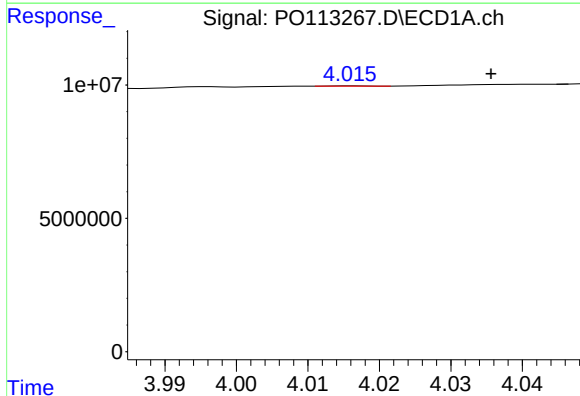


#10 AR-1221-3

R.T.: 4.016 min
Delta R.T.: -0.019 min
Response: 44416
Conc: 0.20 ng/ml

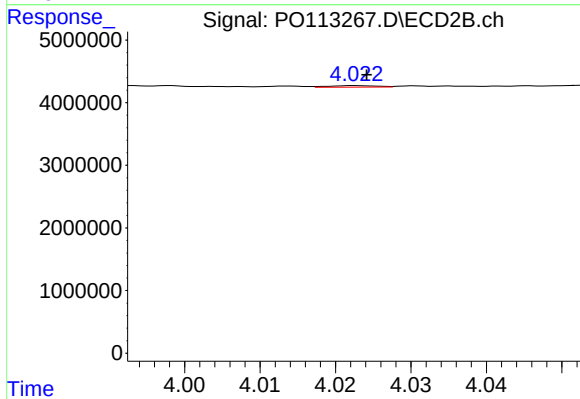

#10 AR-1221-3


R.T.: 4.023 min
Delta R.T.: -0.001 min
Response: 112023
Conc: 0.75 ng/ml

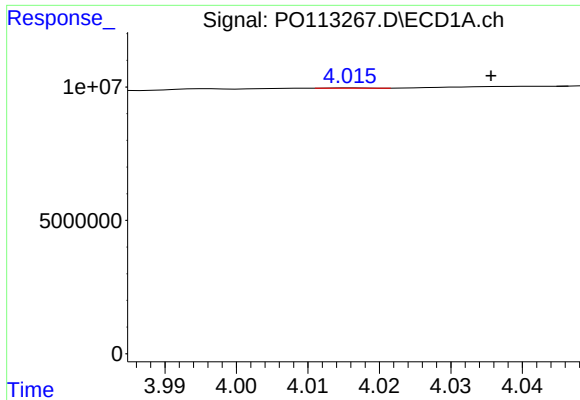

#11 AR-1232-1


R.T.: 4.016 min
Delta R.T.: -0.019 min
Response: 44416
Conc: 0.26 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

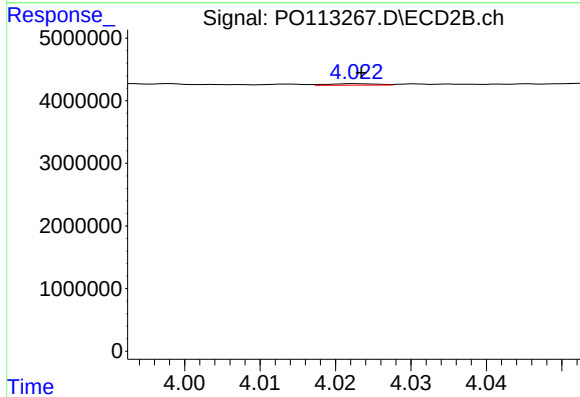


#11 AR-1232-1

R.T.: 4.023 min
Delta R.T.: 0.000 min
Response: 112023
Conc: 0.95 ng/ml

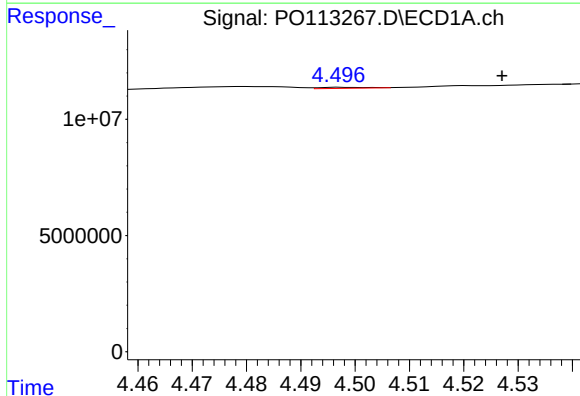


#12 AR-1232-2

R.T.: 4.497 min
Delta R.T.: -0.030 min
Response: 281242
Conc: 2.82 ng/ml

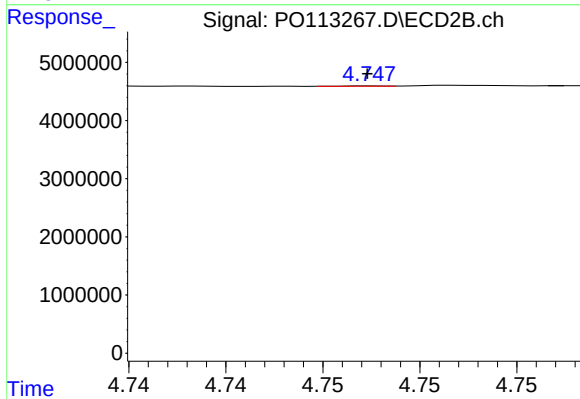

#12 AR-1232-2


R.T.: 4.748 min
Delta R.T.: 0.000 min
Response: 7597
Conc: 0.06 ng/ml

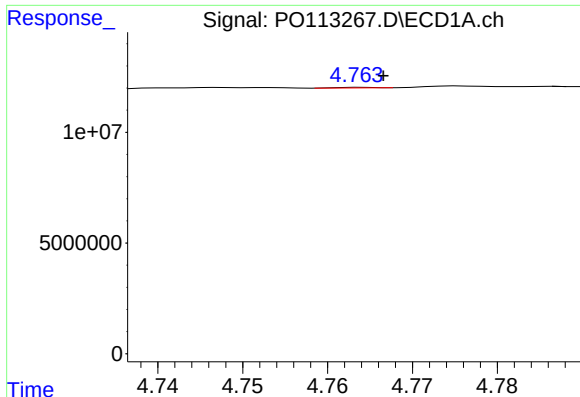

#13 AR-1232-3


R.T.: 4.764 min
Delta R.T.: -0.003 min
Response: 81969
Conc: 0.43 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

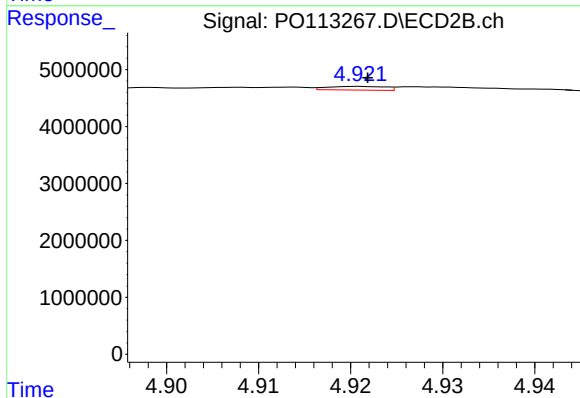


#13 AR-1232-3

R.T.: 4.921 min
Delta R.T.: 0.000 min
Response: 285483
Conc: 4.51 ng/ml

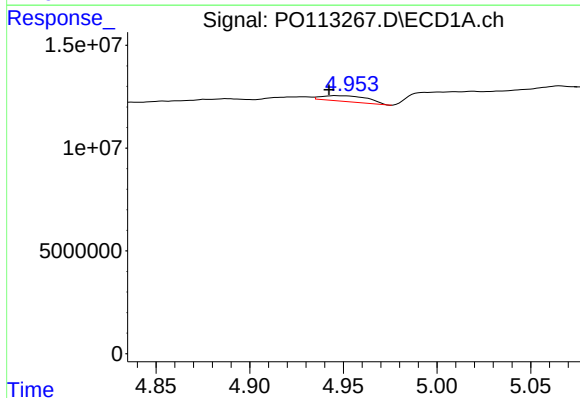


#14 AR-1232-4

R.T.: 4.946 min
Delta R.T.: 0.003 min
Response: 4764912
Conc: 50.60 ng/ml

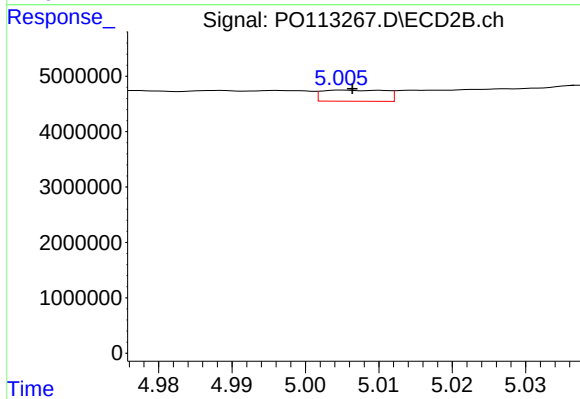

#14 AR-1232-4


R.T.: 5.005 min
Delta R.T.: -0.001 min
Response: 1206859
Conc: 21.47 ng/ml

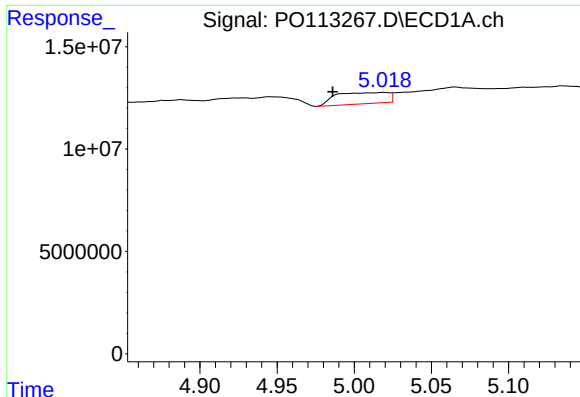

#15 AR-1232-5


R.T.: 5.019 min
Delta R.T.: 0.033 min
Response: 12963367
Conc: 209.28 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

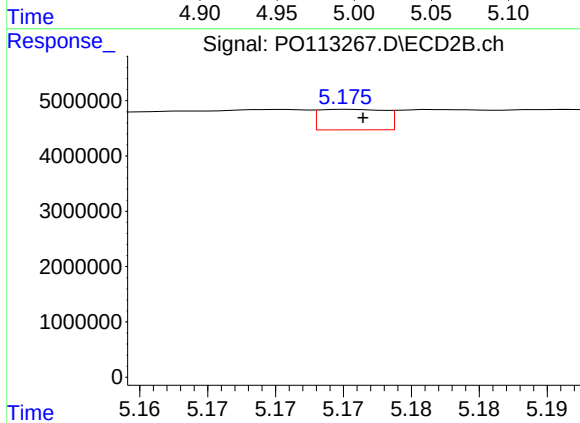


#15 AR-1232-5

R.T.: 5.175 min
Delta R.T.: -0.001 min
Response: 1253929
Conc: 20.95 ng/ml

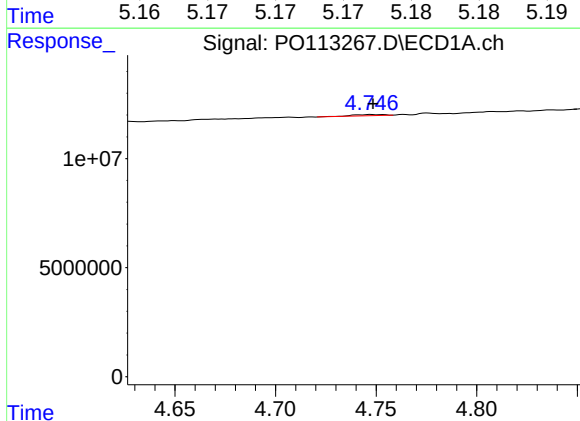


#16 AR-1242-1

R.T.: 4.747 min
Delta R.T.: -0.001 min
Response: 625368
Conc: 2.72 ng/ml

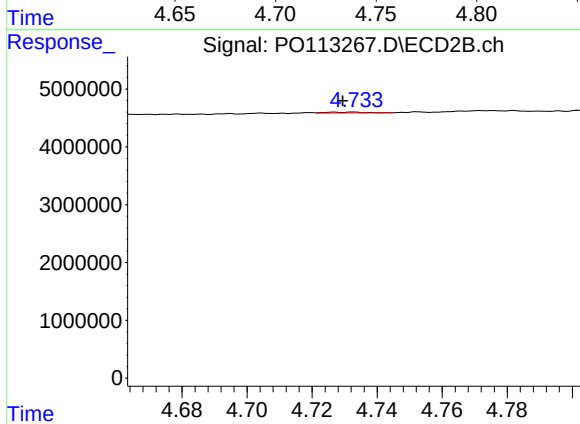

#16 AR-1242-1


R.T.: 4.733 min
Delta R.T.: 0.003 min
Response: 122629
Conc: 0.85 ng/ml

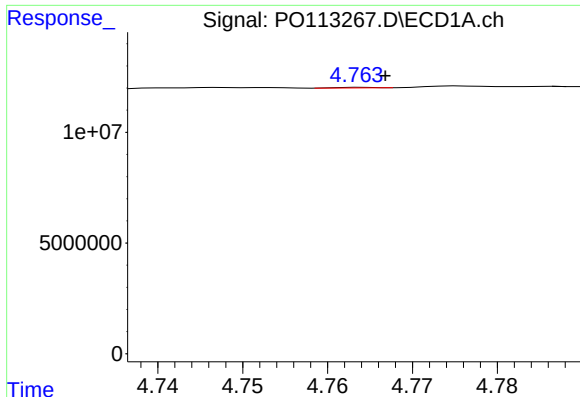

#17 AR-1242-2


R.T.: 4.764 min
Delta R.T.: -0.003 min
Response: 81969
Conc: 0.24 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

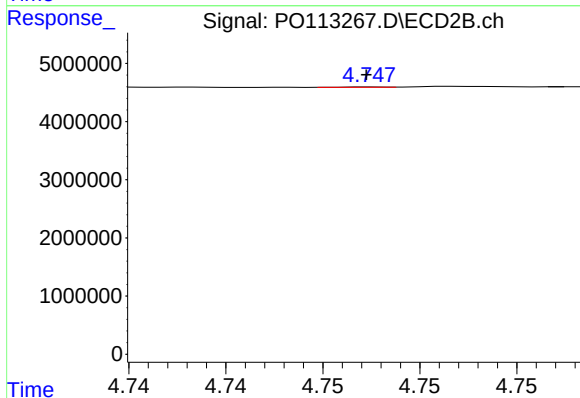


#17 AR-1242-2

R.T.: 4.748 min
Delta R.T.: 0.000 min
Response: 7597
Conc: 0.04 ng/ml

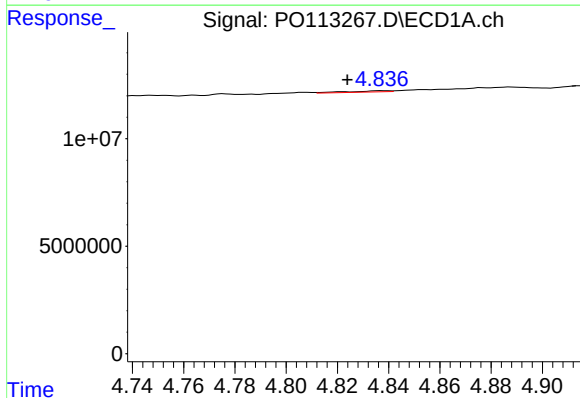


#18 AR-1242-3

R.T.: 4.837 min
Delta R.T.: 0.013 min
Response: 602849
Conc: 2.72 ng/ml

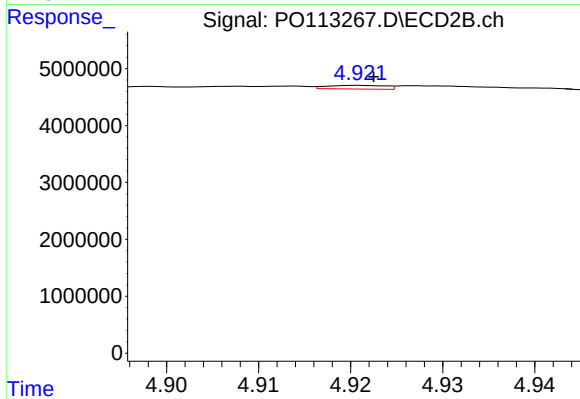

#18 AR-1242-3


R.T.: 4.921 min
Delta R.T.: -0.002 min
Response: 285483
Conc: 2.44 ng/ml

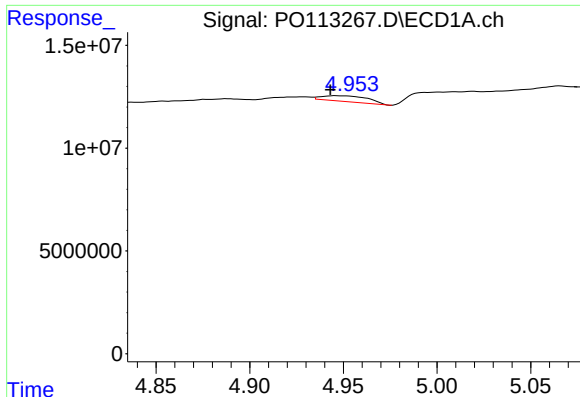

#19 AR-1242-4


R.T.: 4.946 min
Delta R.T.: 0.003 min
Response: 4764912
Conc: 27.47 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

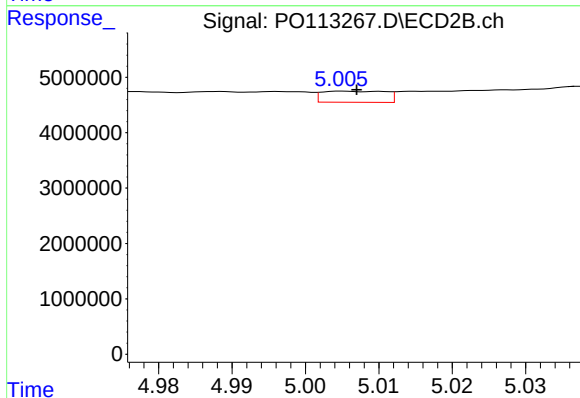


#19 AR-1242-4

R.T.: 5.005 min
Delta R.T.: -0.002 min
Response: 1206859
Conc: 10.26 ng/ml

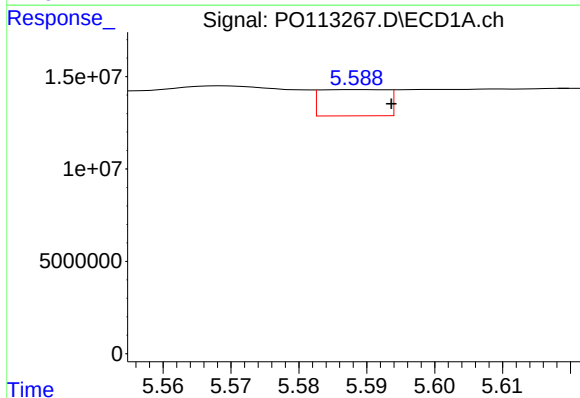


#20 AR-1242-5

R.T.: 5.590 min
Delta R.T.: -0.004 min
Response: 9700224
Conc: 48.46 ng/ml

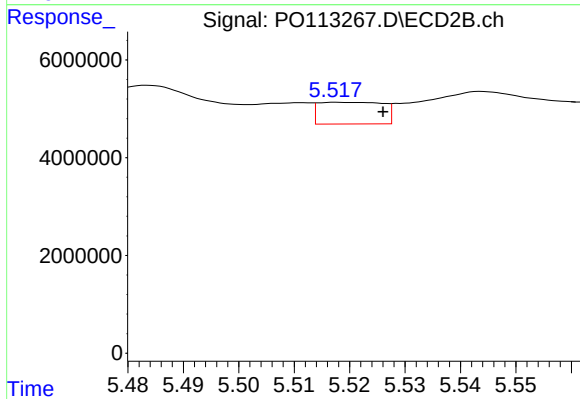

#20 AR-1242-5


R.T.: 5.518 min
Delta R.T.: -0.009 min
Response: 3587286
Conc: 24.05 ng/ml

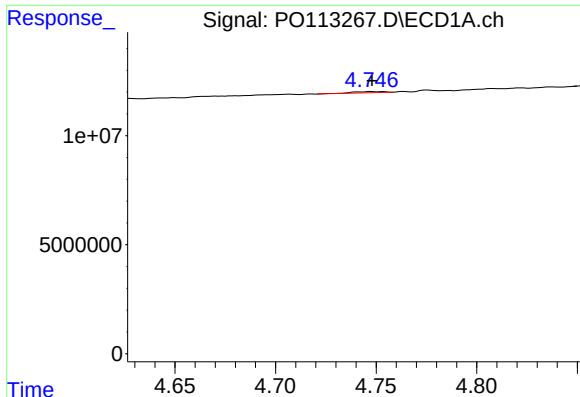

#21 AR-1248-1


R.T.: 4.747 min
Delta R.T.: 0.000 min
Response: 625368
Conc: 3.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

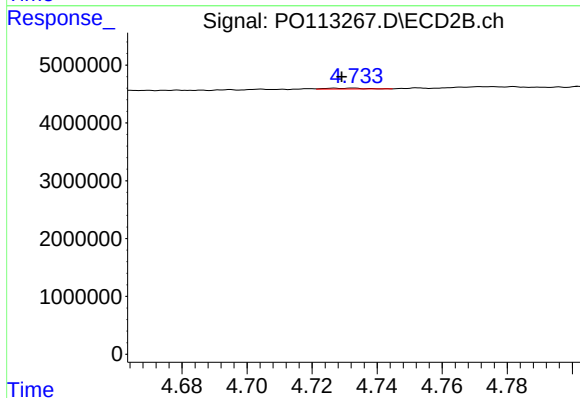


#21 AR-1248-1

R.T.: 4.733 min
Delta R.T.: 0.004 min
Response: 122629
Conc: 1.10 ng/ml

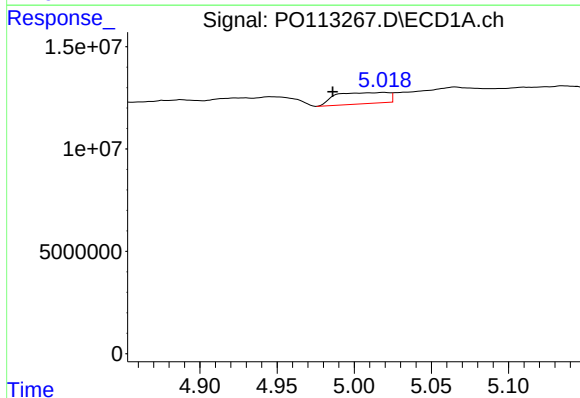


#22 AR-1248-2

R.T.: 5.019 min
Delta R.T.: 0.033 min
Response: 12963367
Conc: 53.60 ng/ml

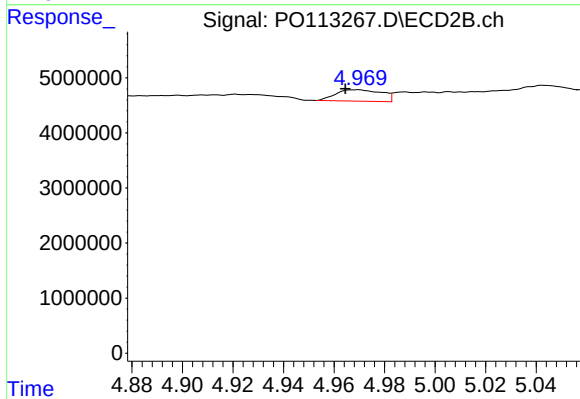

#22 AR-1248-2


R.T.: 4.970 min
Delta R.T.: 0.005 min
Response: 2605060
Conc: 16.21 ng/ml

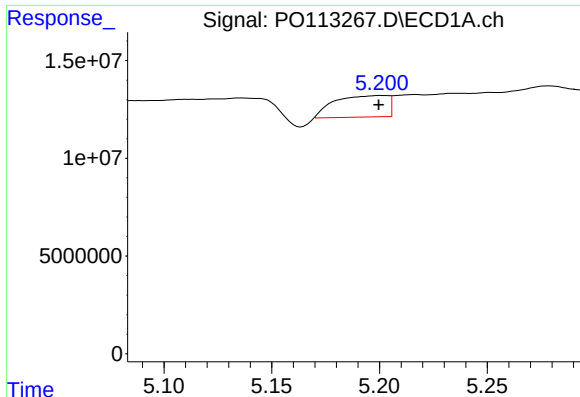

#23 AR-1248-3


R.T.: 5.201 min
Delta R.T.: 0.001 min
Response: 18785506
Conc: 58.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

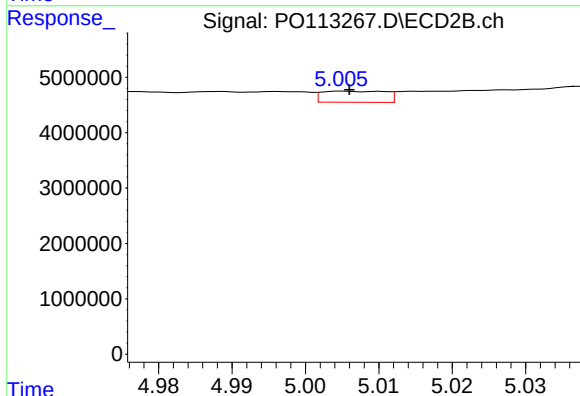


#23 AR-1248-3

R.T.: 5.005 min
Delta R.T.: 0.000 min
Response: 1206859
Conc: 7.11 ng/ml

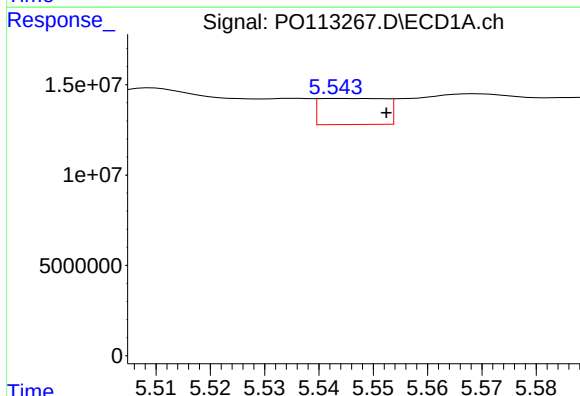


#24 AR-1248-4

R.T.: 5.543 min
Delta R.T.: -0.009 min
Response: 12216434
Conc: 24.45 ng/ml

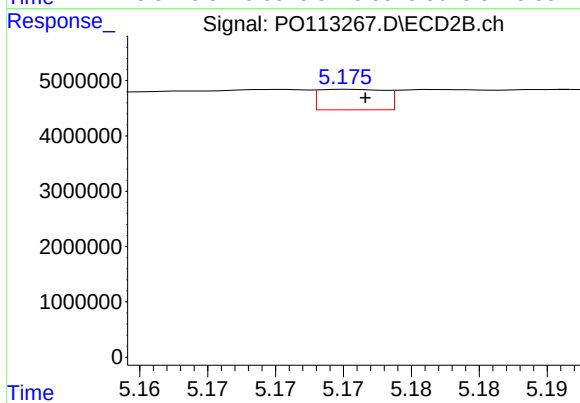

#24 AR-1248-4


R.T.: 5.175 min
Delta R.T.: -0.001 min
Response: 1253929
Conc: 6.29 ng/ml

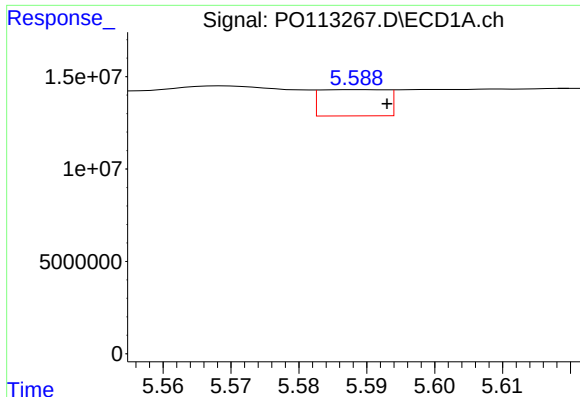

#25 AR-1248-5


R.T.: 5.590 min
Delta R.T.: -0.003 min
Response: 9700224
Conc: 28.41 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

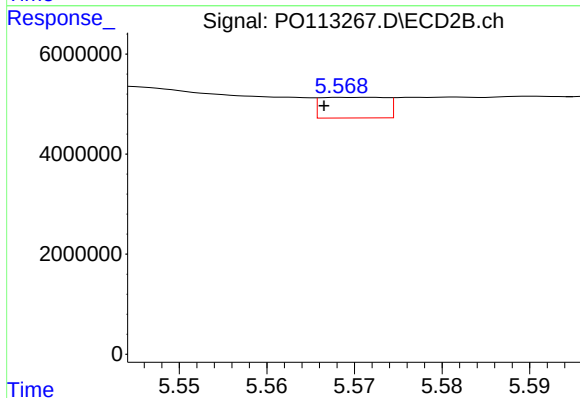


#25 AR-1248-5

R.T.: 5.572 min
Delta R.T.: 0.005 min
Response: 2138437
Conc: 10.07 ng/ml

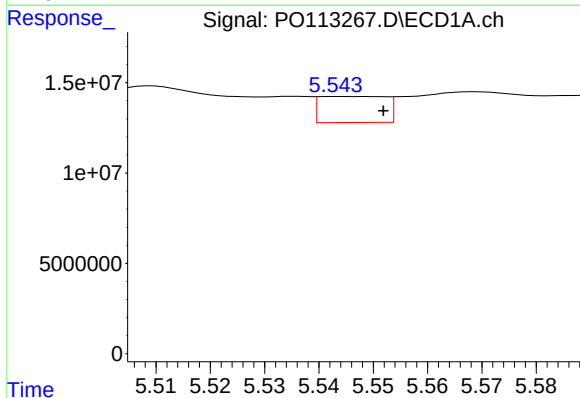


#26 AR-1254-1

R.T.: 5.543 min
Delta R.T.: -0.009 min
Response: 12216434
Conc: 22.62 ng/ml

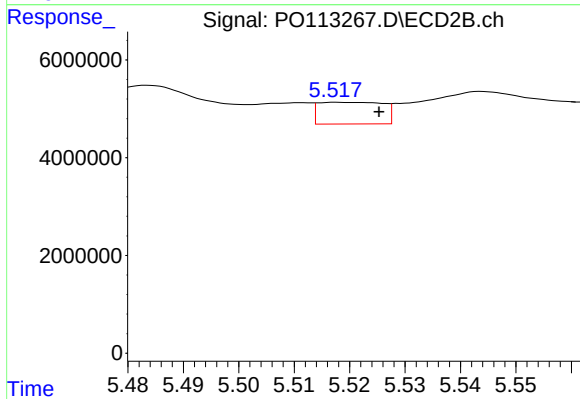

#26 AR-1254-1


R.T.: 5.518 min
Delta R.T.: -0.008 min
Response: 3587286
Conc: 11.38 ng/ml

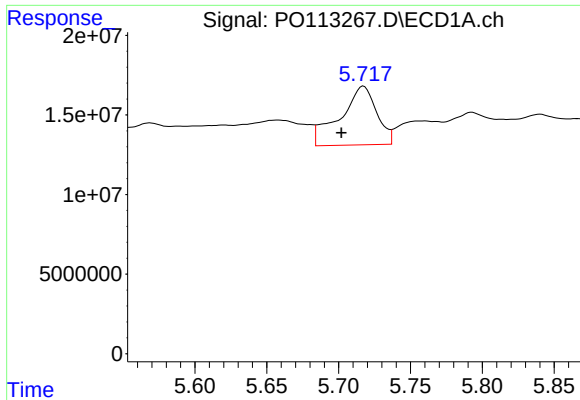

#27 AR-1254-2


R.T.: 5.717 min
Delta R.T.: 0.016 min
Response: 65368652
Conc: 132.47 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

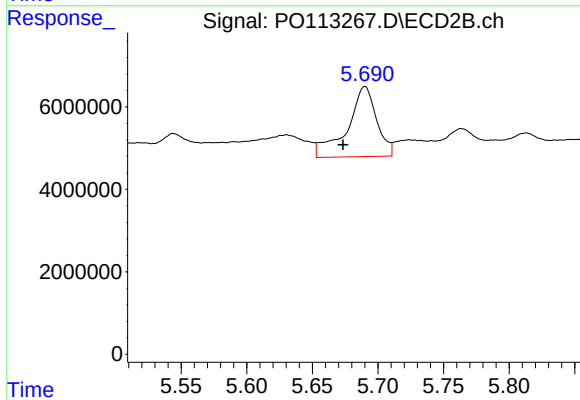


#27 AR-1254-2

R.T.: 5.690 min
Delta R.T.: 0.017 min
Response: 26583498
Conc: 94.83 ng/ml

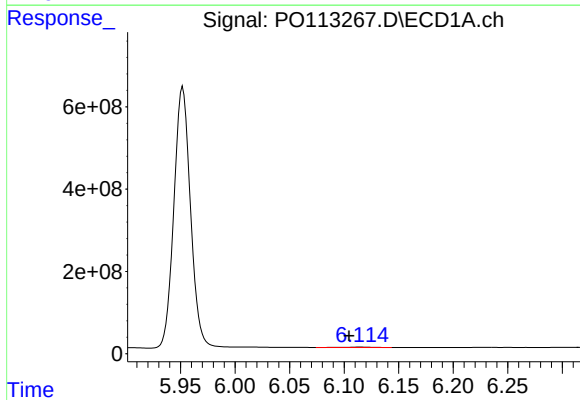


#28 AR-1254-3

R.T.: 6.115 min
Delta R.T.: 0.010 min
Response: 13121123
Conc: 17.76 ng/ml

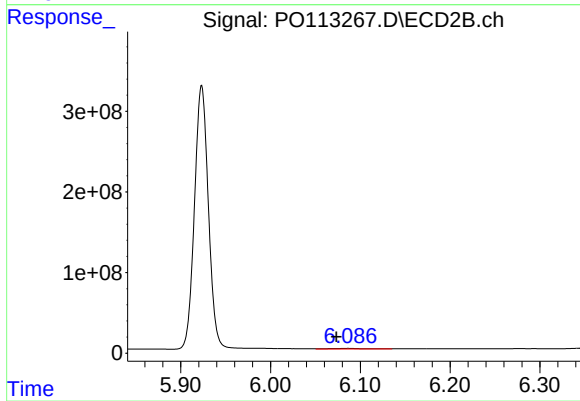

#28 AR-1254-3


R.T.: 6.086 min
Delta R.T.: 0.013 min
Response: 22934117
Conc: 55.01 ng/ml

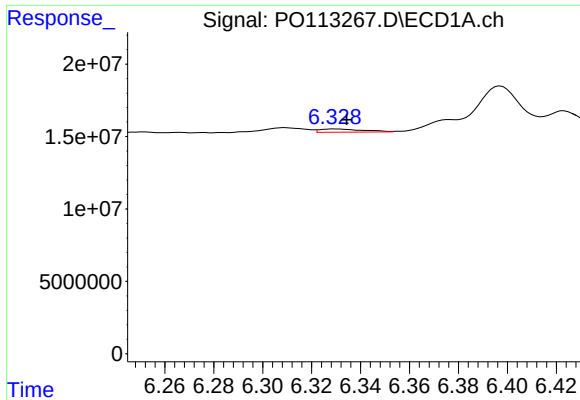

#29 AR-1254-4


R.T.: 6.329 min
Delta R.T.: -0.005 min
Response: 2701776
Conc: 4.85 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

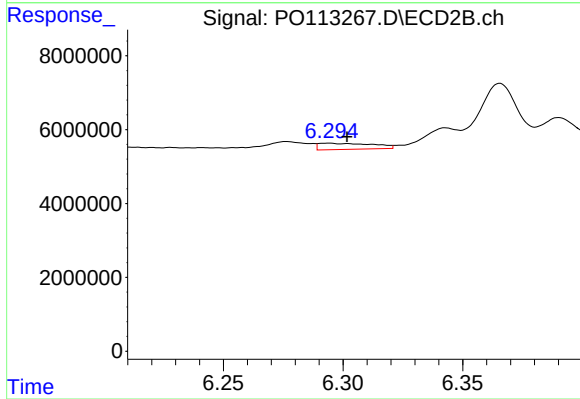


#29 AR-1254-4

R.T.: 6.294 min
Delta R.T.: -0.008 min
Response: 2662252
Conc: 9.69 ng/ml

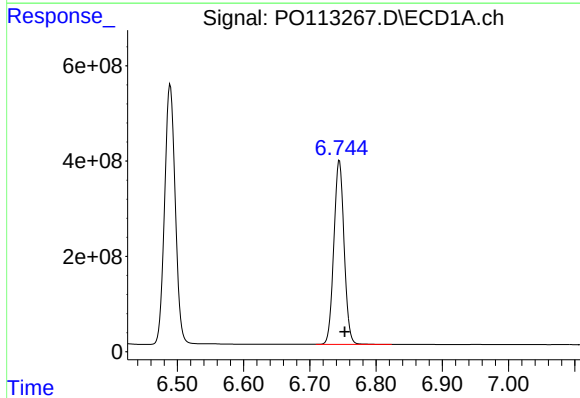


#30 AR-1254-5

R.T.: 6.745 min
Delta R.T.: -0.008 min
Response: 4152954335
Conc: 5924.55 ng/ml

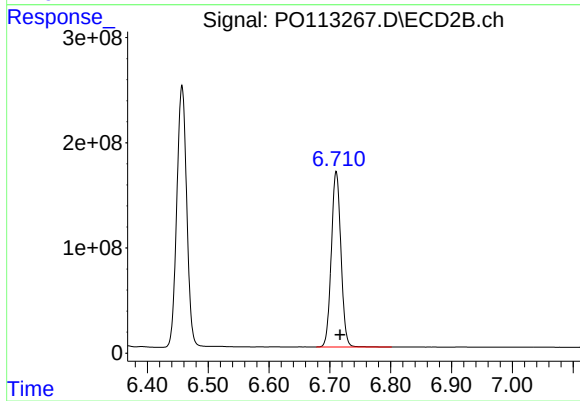

#30 AR-1254-5


R.T.: 6.710 min
Delta R.T.: -0.006 min
Response: 1830523403
Conc: 5120.48 ng/ml

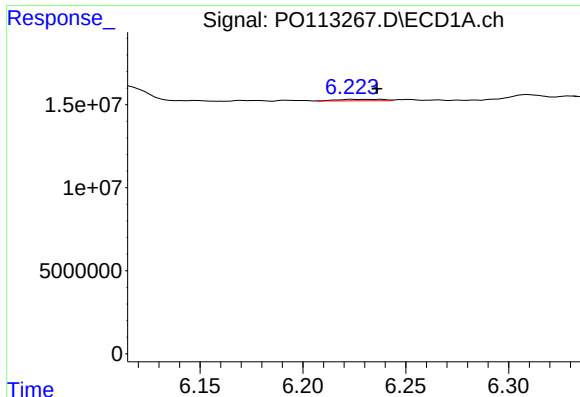

#31 AR-1260-1


R.T.: 6.238 min
Delta R.T.: 0.002 min
Response: 1447771
Conc: 3.25 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

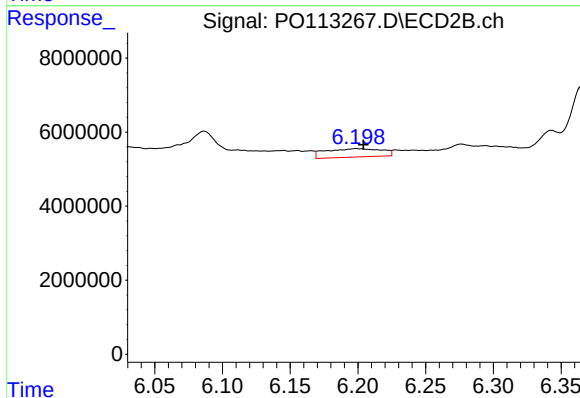


#31 AR-1260-1

R.T.: 6.199 min
Delta R.T.: -0.005 min
Response: 6468146
Conc: 25.36 ng/ml

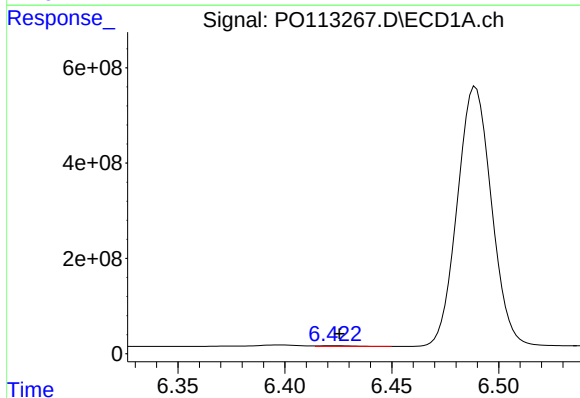


#32 AR-1260-2

R.T.: 6.423 min
Delta R.T.: -0.002 min
Response: 14775477
Conc: 21.52 ng/ml

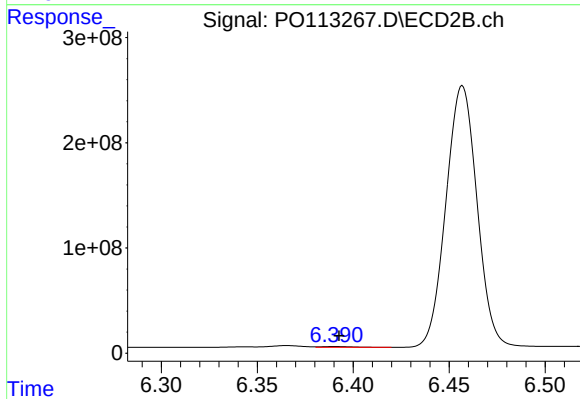

#32 AR-1260-2


R.T.: 6.390 min
Delta R.T.: -0.002 min
Response: 8438964
Conc: 24.41 ng/ml

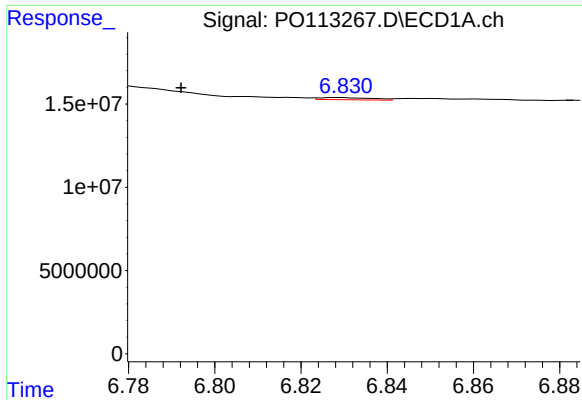

#33 AR-1260-3


R.T.: 6.829 min
Delta R.T.: 0.037 min
Response: 1112005
Conc: 1.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

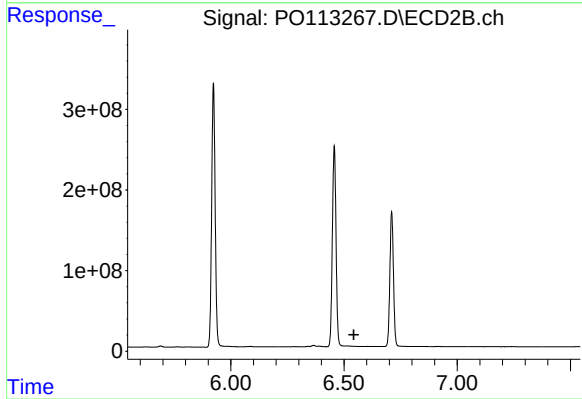


#33 AR-1260-3

R.T.: 6.517 min
Delta R.T.: -0.026 min
Response: -1721025
Conc: N.D.

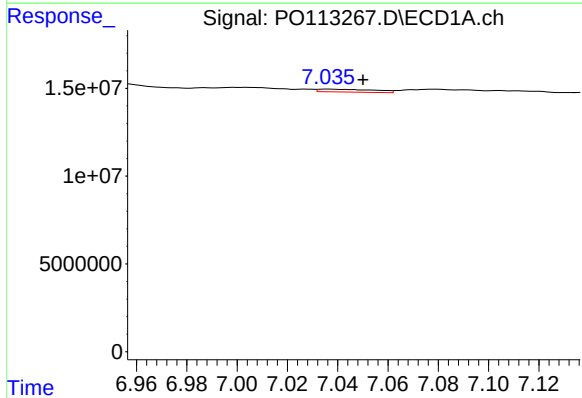


#34 AR-1260-4

R.T.: 7.036 min
Delta R.T.: -0.014 min
Response: 2528758
Conc: 5.65 ng/ml

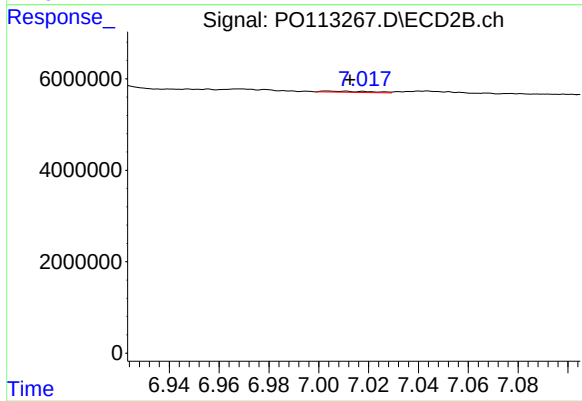

#34 AR-1260-4


R.T.: 7.003 min
Delta R.T.: -0.009 min
Response: 336036
Conc: 1.62 ng/ml

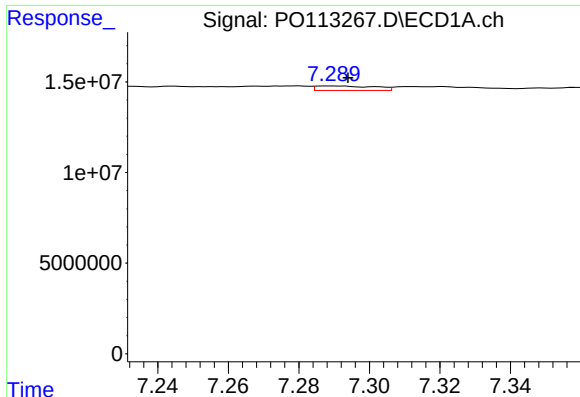

#35 AR-1260-5


R.T.: 7.289 min
Delta R.T.: -0.005 min
Response: 2843983
Conc: 2.35 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

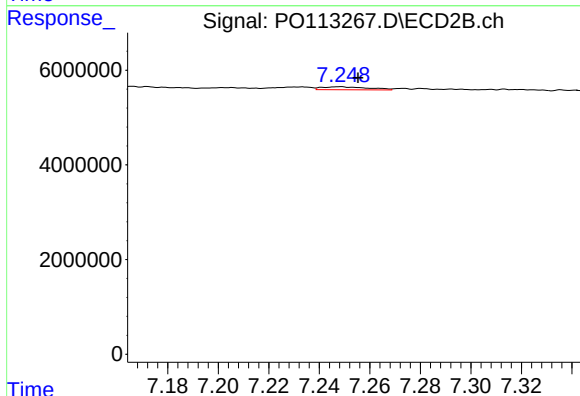


#35 AR-1260-5

R.T.: 7.248 min
Delta R.T.: -0.007 min
Response: 826094
Conc: 1.76 ng/ml

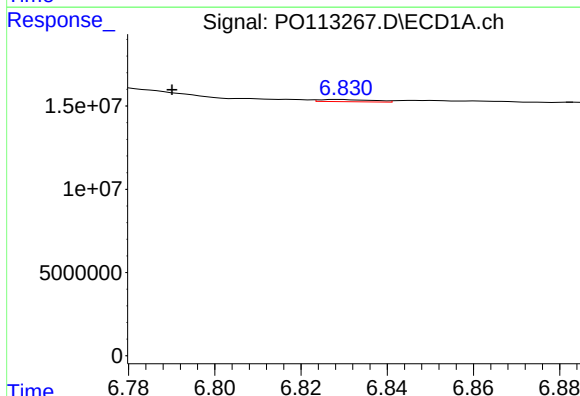


#36 AR-1262-1

R.T.: 6.829 min
Delta R.T.: 0.039 min
Response: 1112005
Conc: 1.21 ng/ml

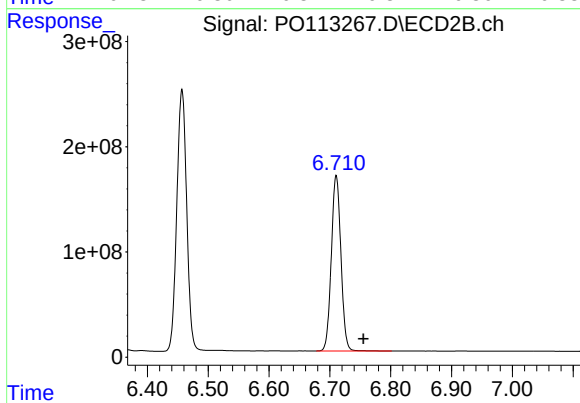

#36 AR-1262-1


R.T.: 6.710 min
Delta R.T.: -0.045 min
Response: 1830523403
Conc: 4415.00 ng/ml

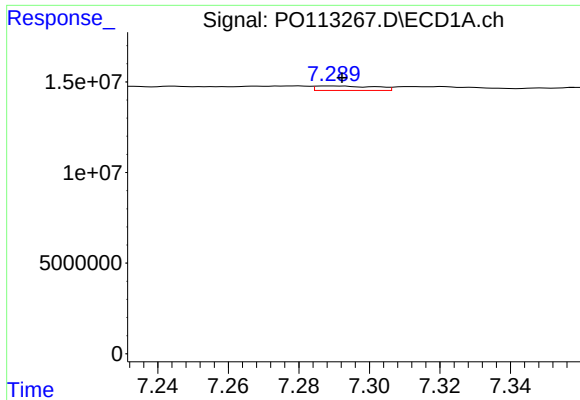

#37 AR-1262-2


R.T.: 7.289 min
Delta R.T.: -0.003 min
Response: 2843983
Conc: 1.88 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

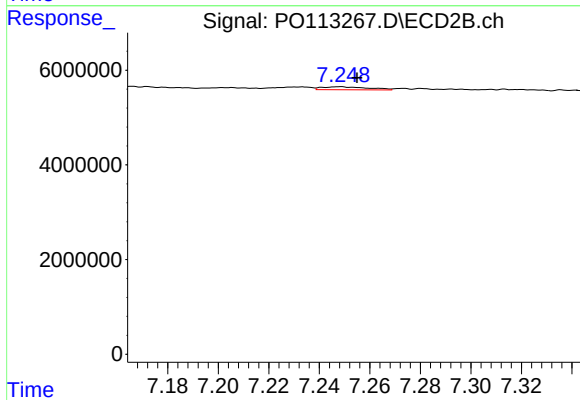


#37 AR-1262-2

R.T.: 7.248 min
Delta R.T.: -0.007 min
Response: 826094
Conc: 1.60 ng/ml

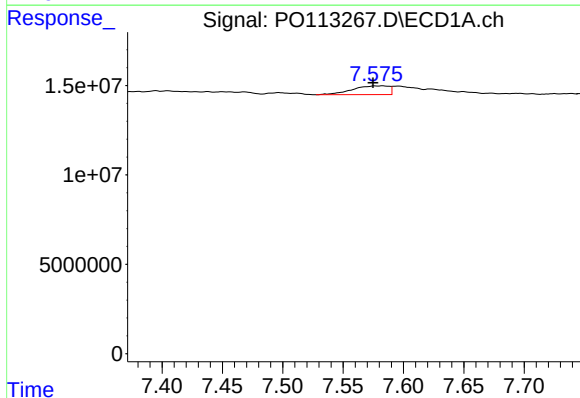


#38 AR-1262-3

R.T.: 7.583 min
Delta R.T.: 0.008 min
Response: 10348963
Conc: 18.68 ng/ml

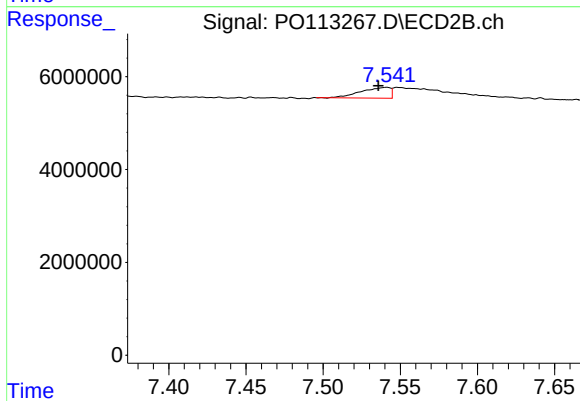

#38 AR-1262-3


R.T.: 7.541 min
Delta R.T.: 0.005 min
Response: 3104217
Conc: 17.28 ng/ml

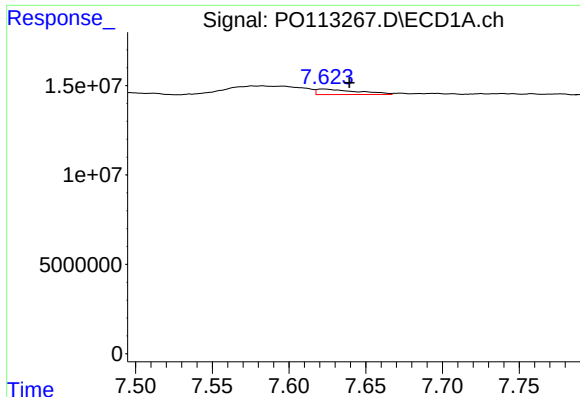

#39 AR-1262-4


R.T.: 7.623 min
Delta R.T.: -0.016 min
Response: 5628704
Conc: 5.76 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

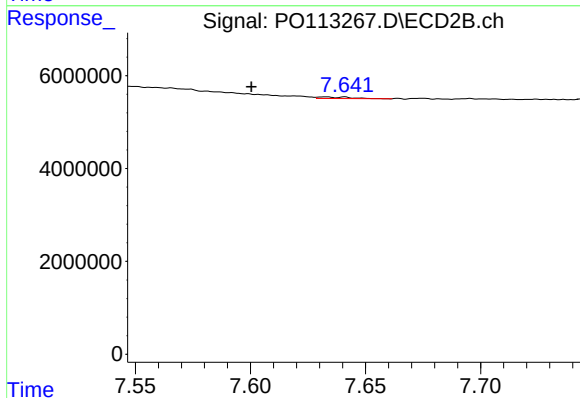


#39 AR-1262-4

R.T.: 7.633 min
Delta R.T.: 0.032 min
Response: 316306
Conc: 1.09 ng/ml

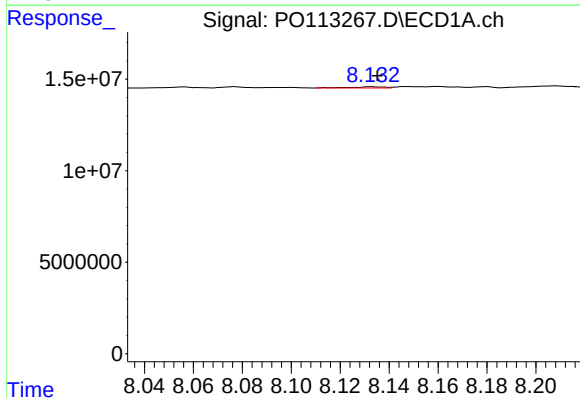


#40 AR-1262-5

R.T.: 8.133 min
Delta R.T.: -0.002 min
Response: 637422
Conc: 1.53 ng/ml

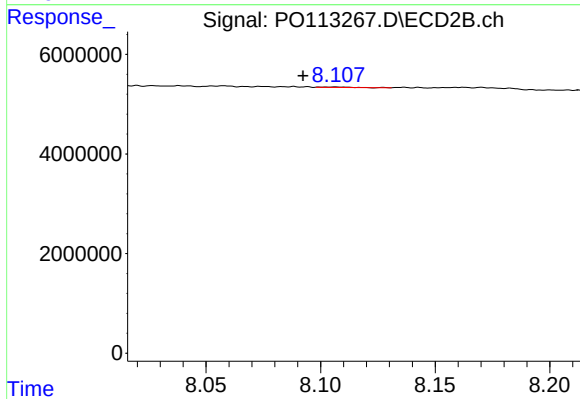

#40 AR-1262-5


R.T.: 8.107 min
Delta R.T.: 0.014 min
Response: 115922
Conc: 1.07 ng/ml

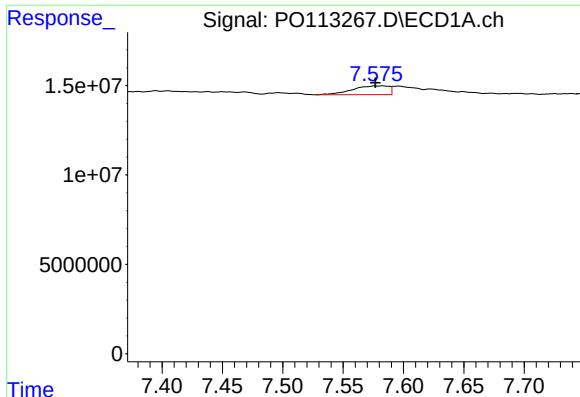

#41 AR-1268-1


R.T.: 7.583 min
Delta R.T.: 0.006 min
Response: 10348963
Conc: 6.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

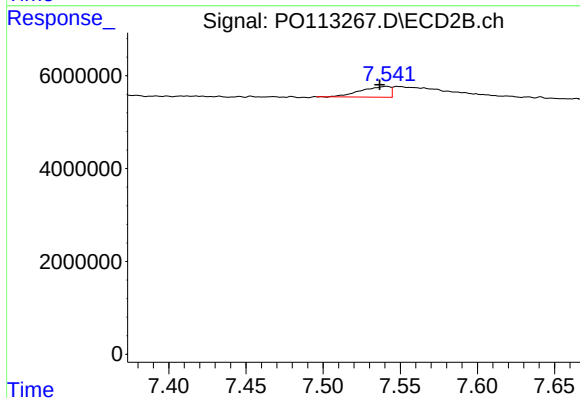


#41 AR-1268-1

R.T.: 7.541 min
Delta R.T.: 0.004 min
Response: 3104217
Conc: 6.09 ng/ml

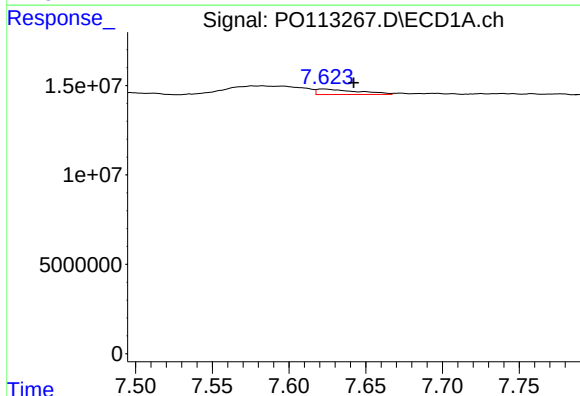


#42 AR-1268-2

R.T.: 7.623 min
Delta R.T.: -0.019 min
Response: 5628704
Conc: 3.89 ng/ml

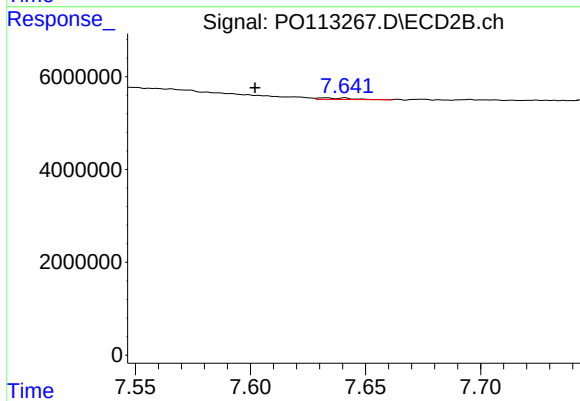

#42 AR-1268-2


R.T.: 7.633 min
Delta R.T.: 0.031 min
Response: 316306
Conc: 0.76 ng/ml

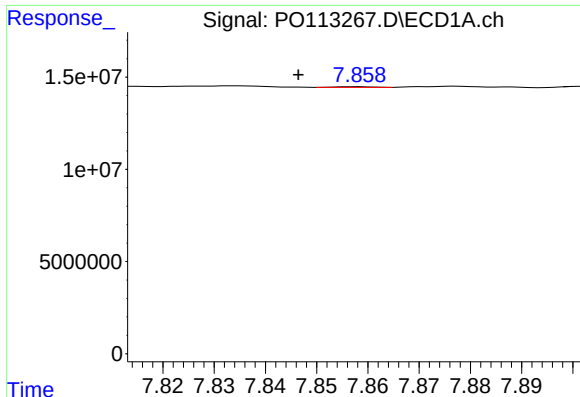

#43 AR-1268-3


R.T.: 7.858 min
Delta R.T.: 0.011 min
Response: 165936
Conc: 0.14 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

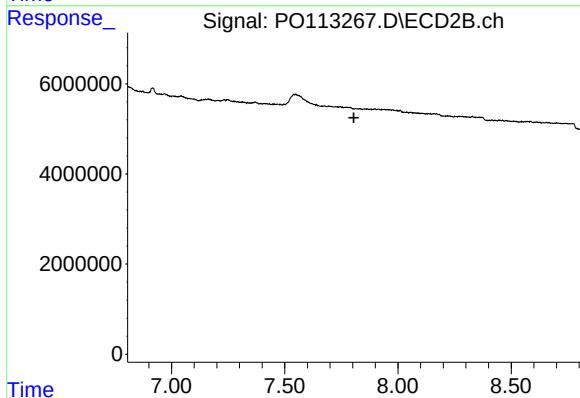


#43 AR-1268-3

R.T.: 7.814 min
Delta R.T.: 0.009 min
Response: -41056
Conc: N.D.

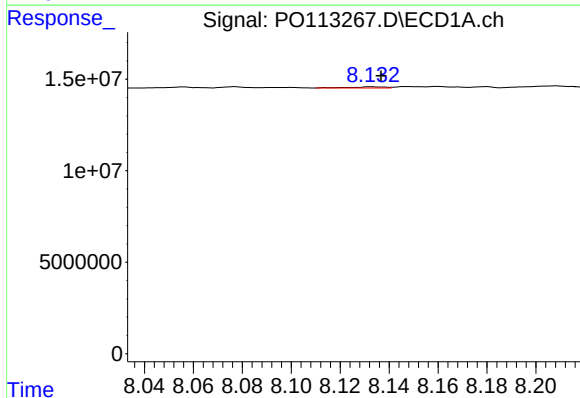


#44 AR-1268-4

R.T.: 8.133 min
Delta R.T.: -0.004 min
Response: 637422
Conc: 1.38 ng/ml

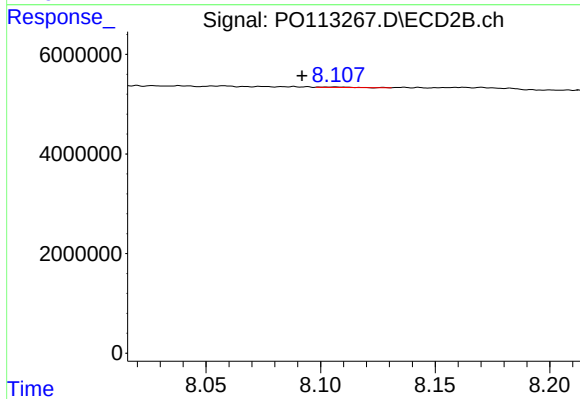

#44 AR-1268-4


R.T.: 8.107 min
Delta R.T.: 0.015 min
Response: 115922
Conc: 0.96 ng/ml

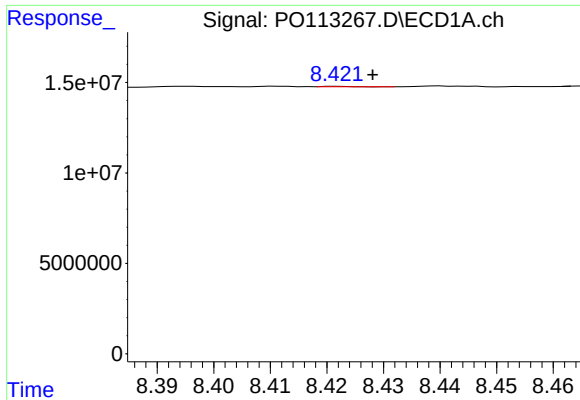

#45 AR-1268-5

R.T.: 8.422 min
Delta R.T.: -0.006 min
Response: 69525
Conc: 0.02 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

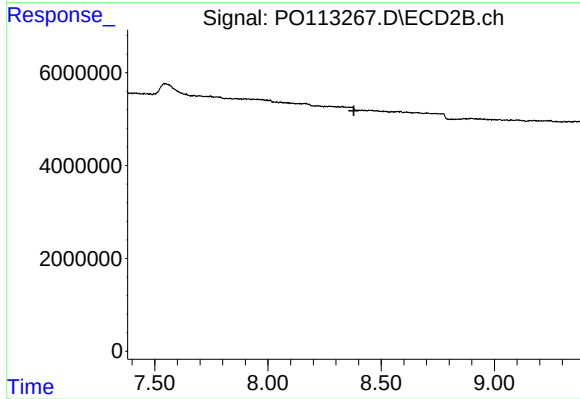

#45 AR-1268-5

R.T.: 8.393 min
Delta R.T.: 0.014 min
Response: -143191
Conc: N.D.