

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0122923\
 Data File : P0100860.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Dec 2023 12:14
 Operator : YP/AJ
 Sample : 06025-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 50200

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 01/02/2024
 Supervised By :Ankita Jodhani 01/02/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 29 23:33:29 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0122023.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Dec 21 04:28:19 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.348	3.644	67641134	42614455	21.678m	20.854m
2) SA Decachlor...	10.096	8.706	37360715	29137253	17.884	19.304

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122923\
Data File : PO100860.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Dec 2023 12:14
Operator : YP/AJ
Sample : 06025-01
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
50200


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/02/2024
Supervised By :Ankita Jodhani 01/02/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 29 23:33:29 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO122023.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Dec 21 04:28:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

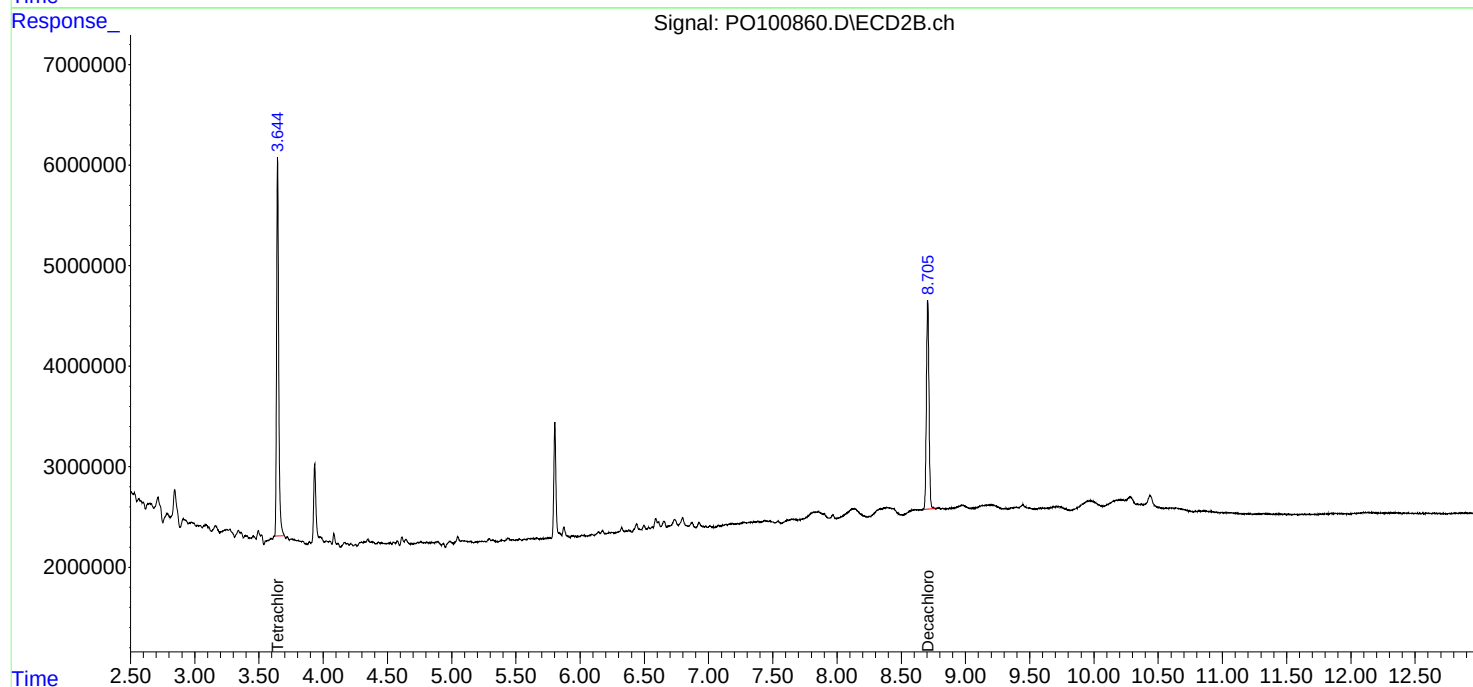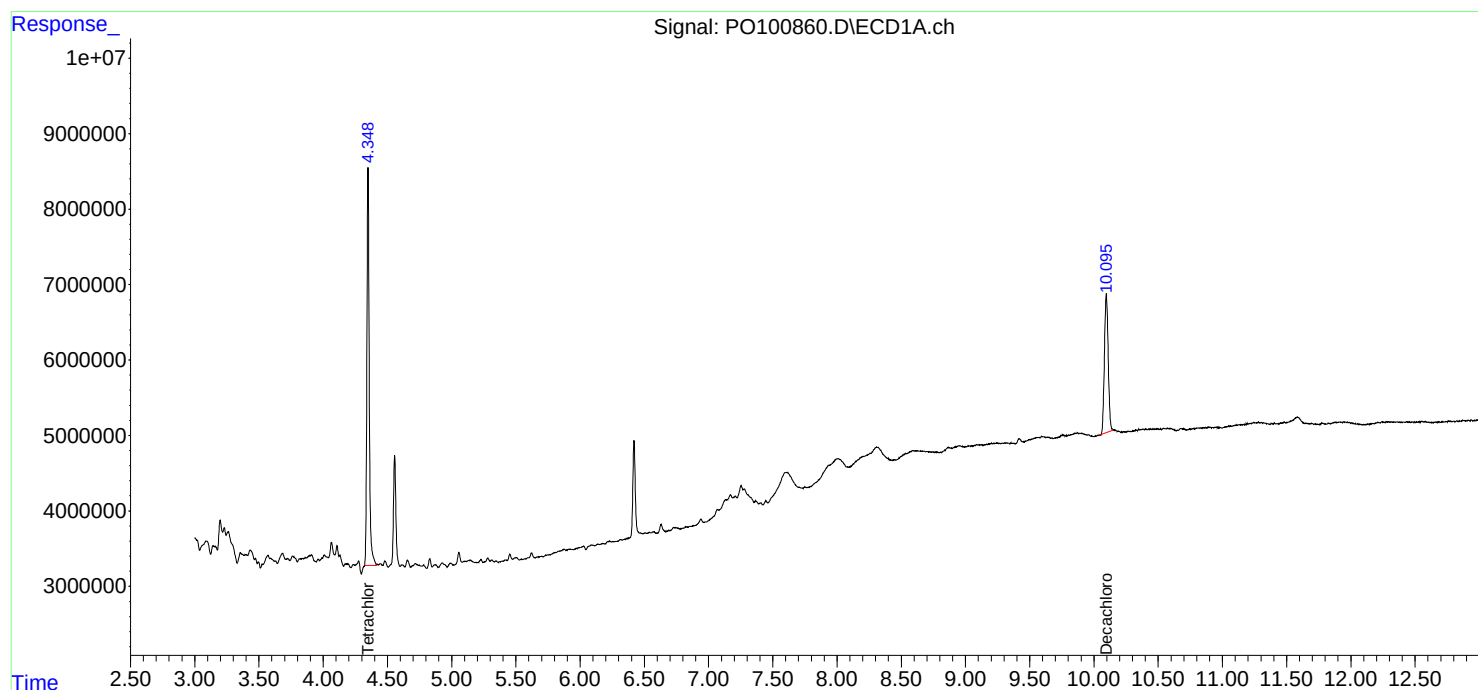

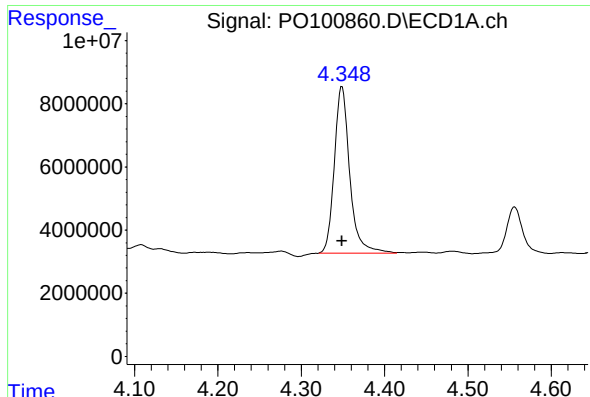


#1 Tetrachloro-m-xylene

R.T.: 4.348 min
Delta R.T.: 0.000 min
Response: 67641134
Conc: 21.68 ng/ml

Instrument :
ECD_O
ClientSampleId :
50200


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/02/2024
Supervised By :Ankita Jodhani 01/02/2024

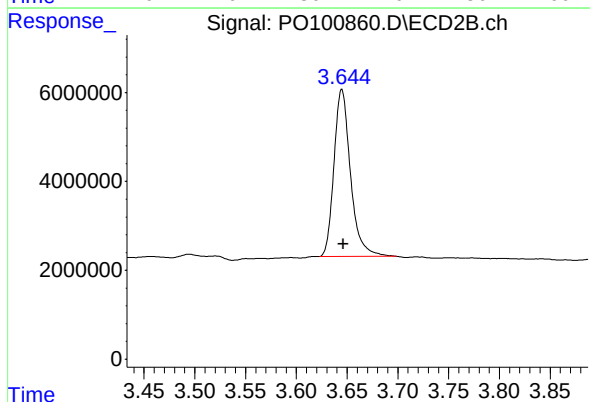


#1 Tetrachloro-m-xylene

R.T.: 3.644 min
Delta R.T.: -0.002 min
Response: 42614455
Conc: 20.85 ng/ml

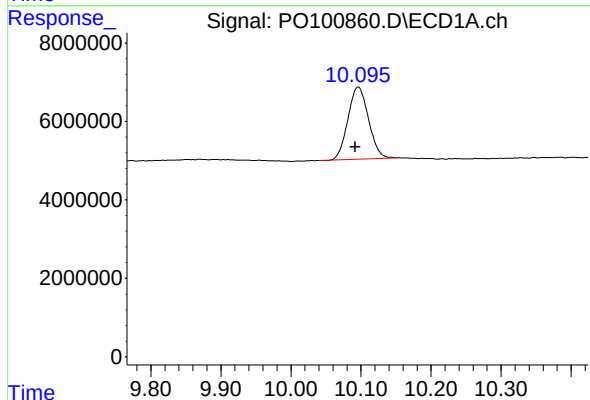

#2 Decachlorobiphenyl

R.T.: 10.096 min
Delta R.T.: 0.004 min
Response: 37360715
Conc: 17.88 ng/ml

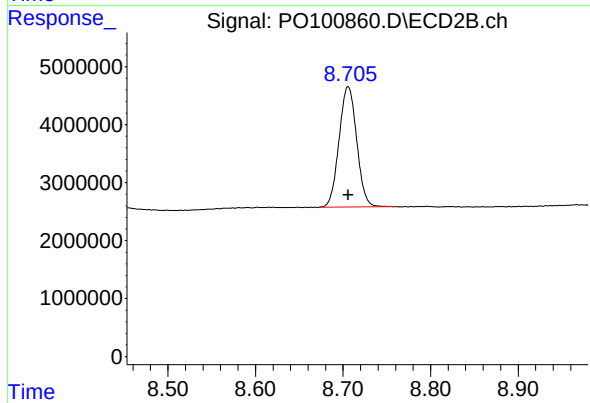

#2 Decachlorobiphenyl

R.T.: 8.706 min
Delta R.T.: 0.000 min
Response: 29137253
Conc: 19.30 ng/ml