

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042419\
Data File : P0055634.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Apr 2019 23:08
Operator : SM/SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: 24 Apr 2019 02:09:48
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042419.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Apr 25 01:58:33 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.285	3.598	405725	404508	16.013	16.610
2)	SA Decachlor...	9.895	8.557	730993	526746	17.034	17.136

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042419\
Data File : P0055634.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Apr 2019 23:08
Operator : SM/SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 25 02:09:48 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042419.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Apr 25 01:58:33 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

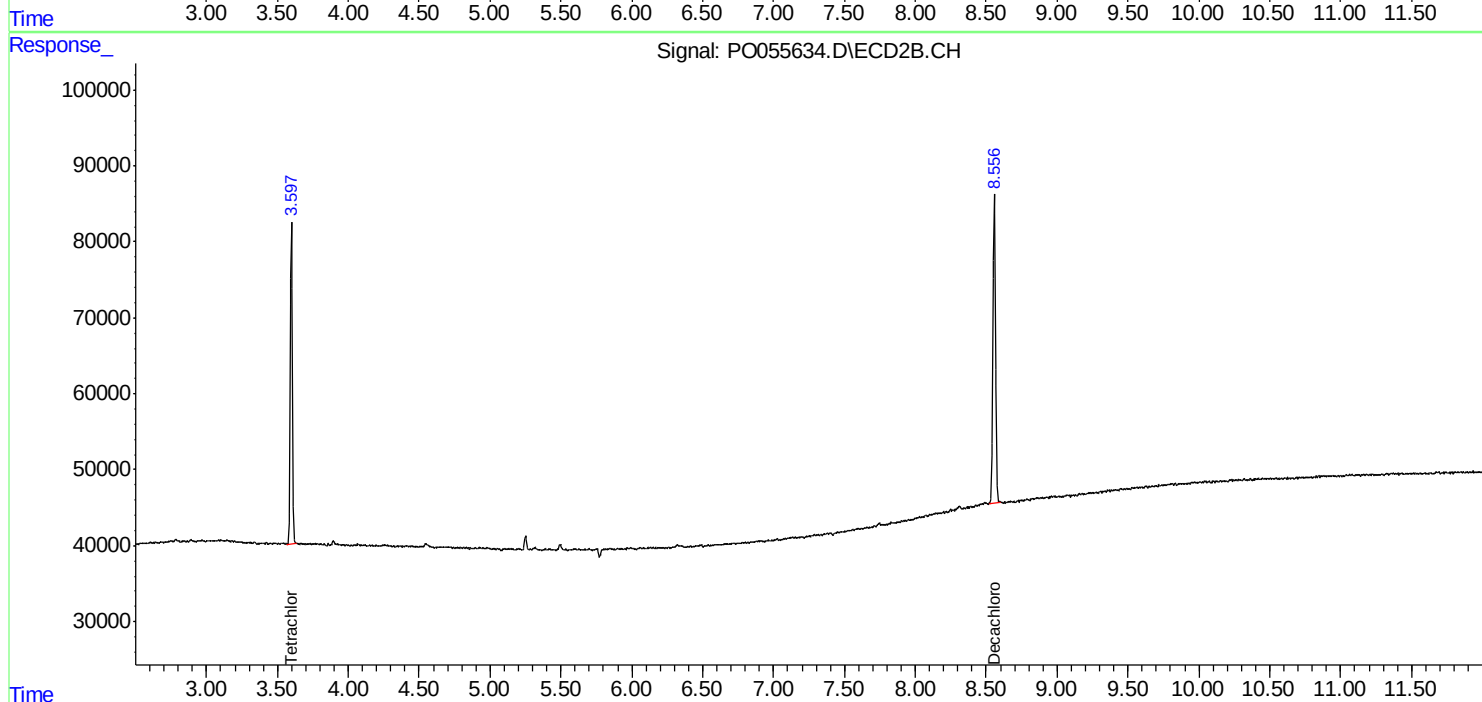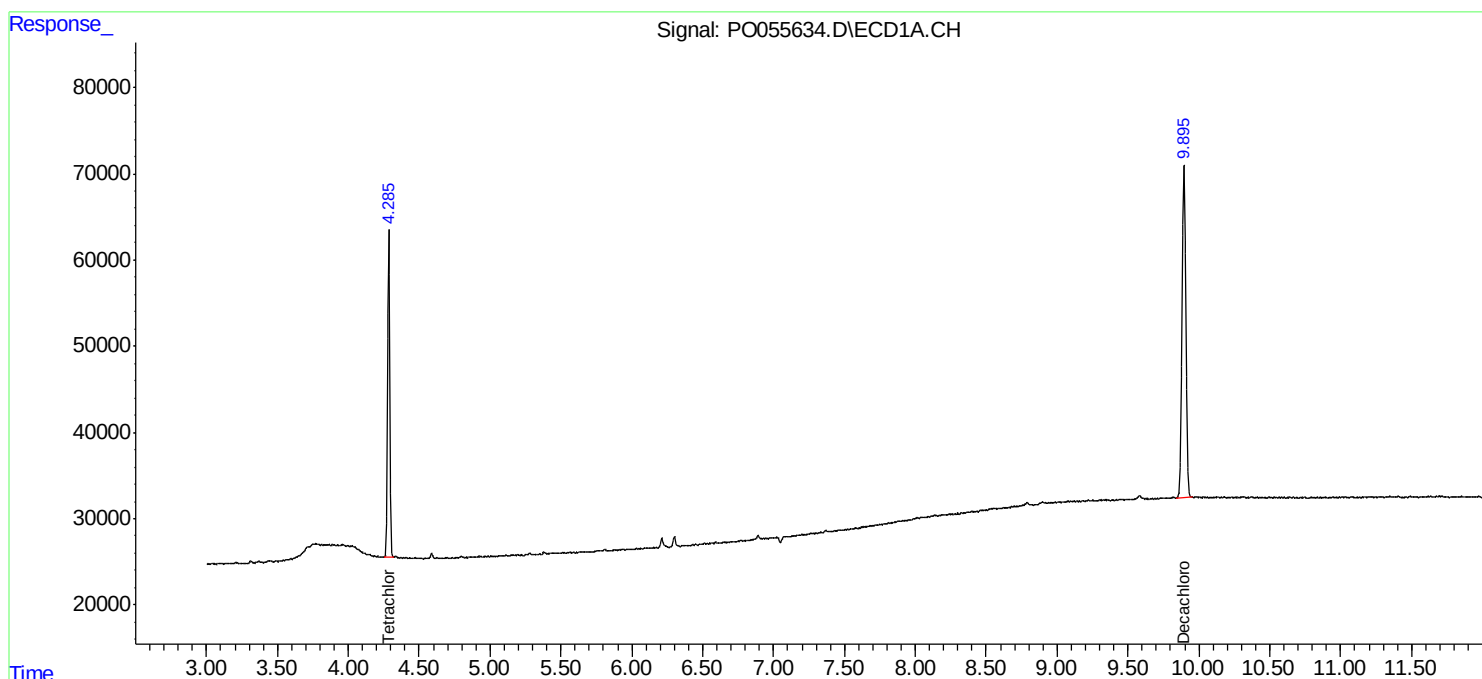


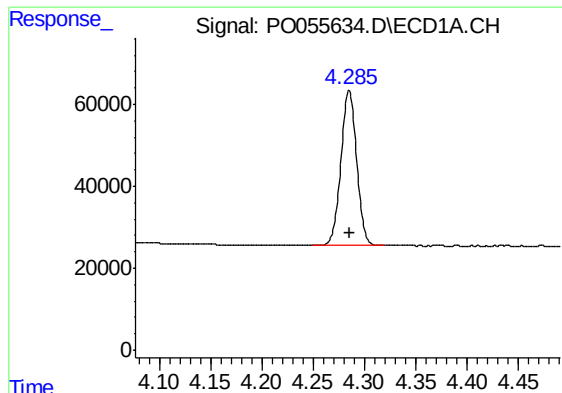

#1 Tetrachloro-m-xylene


R.T.: 4.285 min
Delta R.T.: -0.001 min
Response: 405725
Conc: 16.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

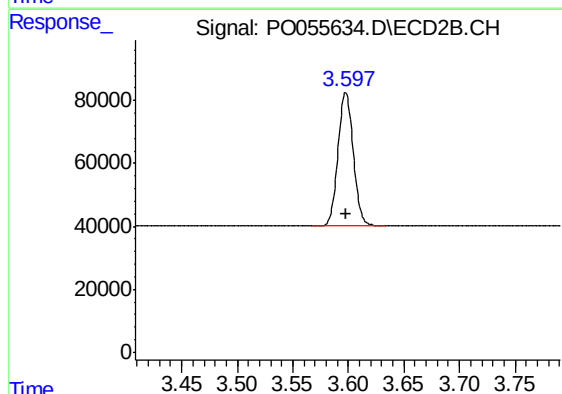


#1 Tetrachloro-m-xylene

R.T.: 3.598 min
Delta R.T.: 0.000 min
Response: 404508
Conc: 16.61 ng/ml

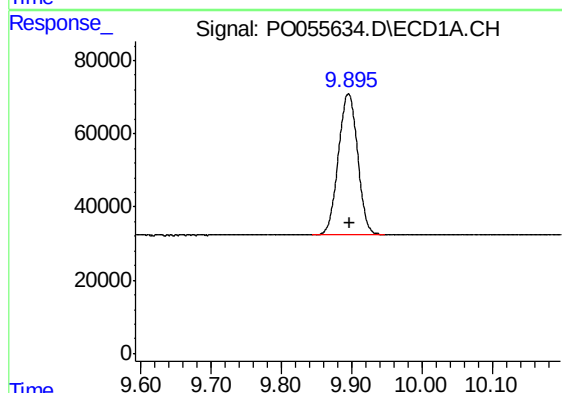

#2 Decachlorobiphenyl

R.T.: 9.895 min
Delta R.T.: -0.002 min
Response: 730993
Conc: 17.03 ng/ml

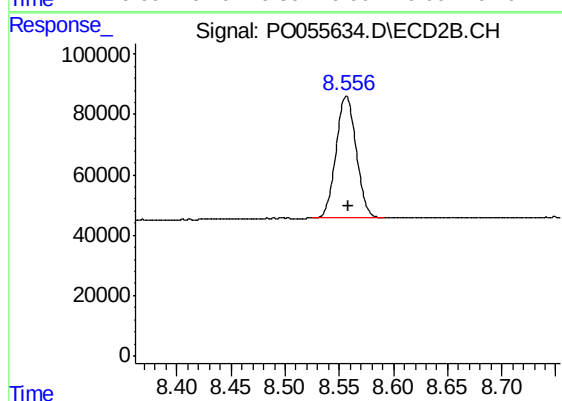

#2 Decachlorobiphenyl

R.T.: 8.557 min
Delta R.T.: -0.002 min
Response: 526746
Conc: 17.14 ng/ml