

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091818\
 Data File : P0049091.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Sep 2018 16:54
 Operator : SM/SJ
 Sample : J4773-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CL-01-091418-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 19 00:59:43 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091118.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 12 08:13:07 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.407	3.527	4072340	4780603	24.857m	26.205
2) SA Decachlor...	10.133	8.469	3368655	2560702	15.120m	13.799

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091818\
Data File : PO049091.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Sep 2018 16:54
Operator : SM/SJ
Sample : J4773-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CL-01-091418-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 19 00:59:43 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091118.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 12 08:13:07 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

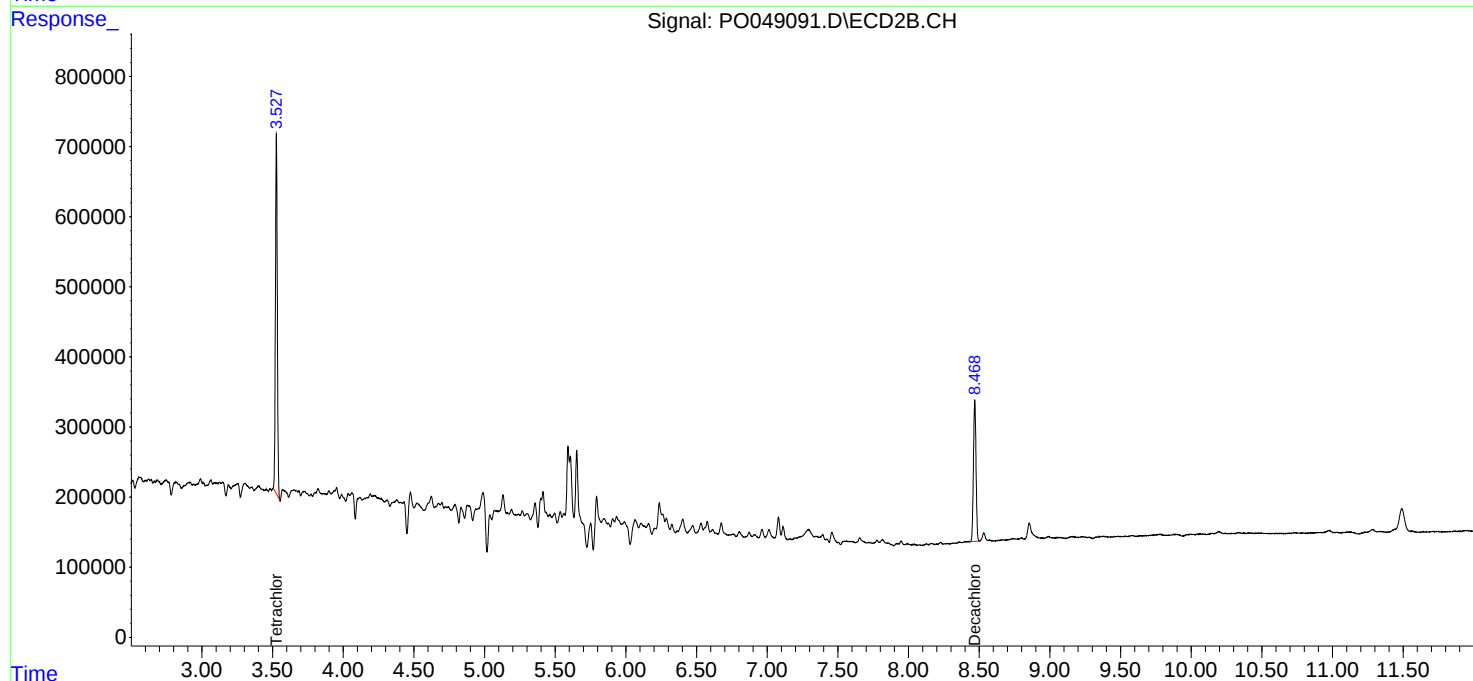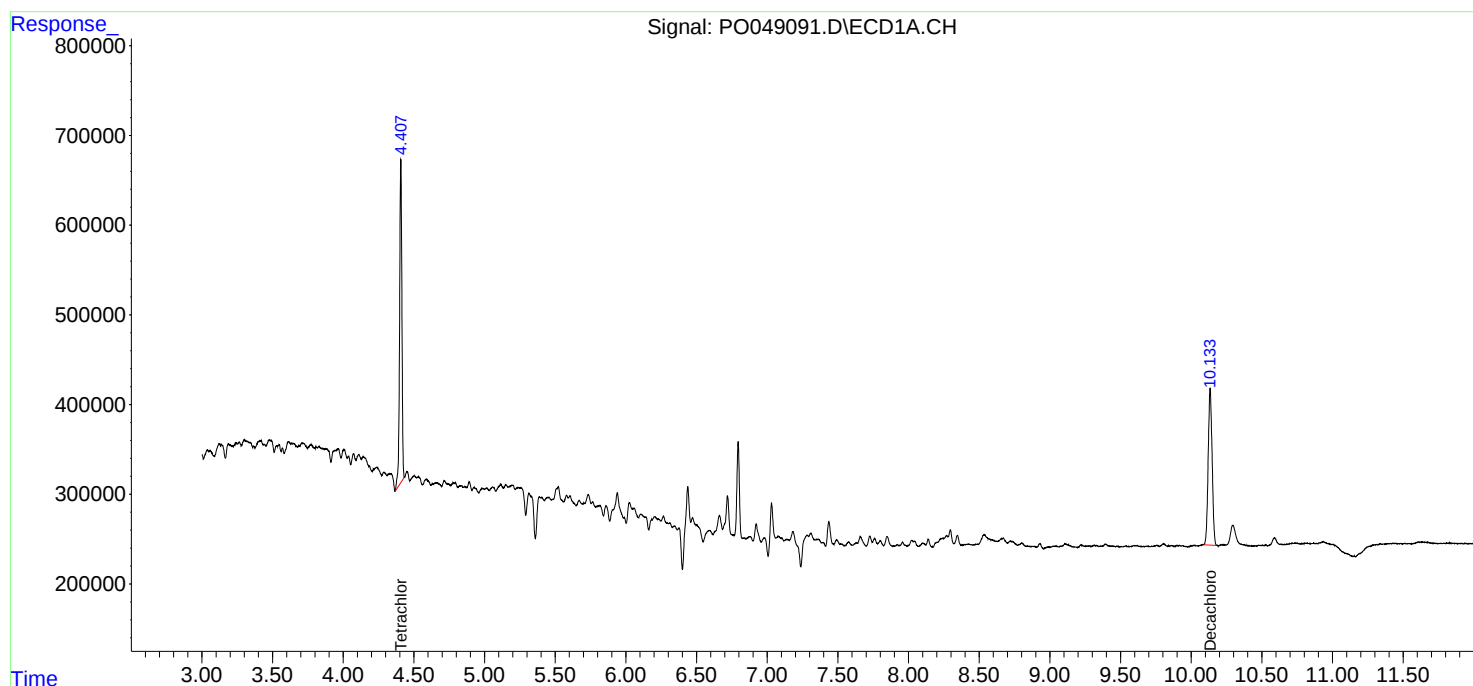


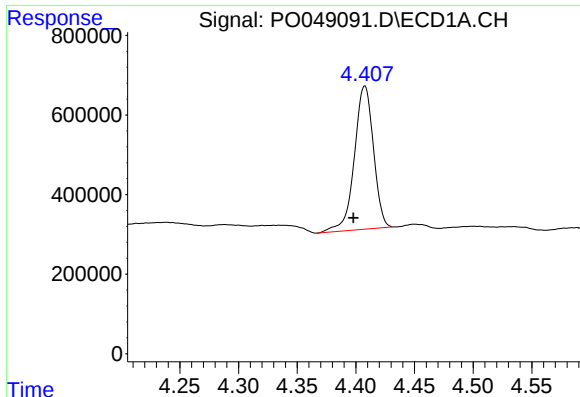

#1 Tetrachloro-m-xylene


R.T.: 4.407 min
Delta R.T.: 0.009 min
Response: 4072340
Conc: 24.86 ng/ml m

Instrument :
ECD_O
ClientSampleId :
CL-01-091418-A

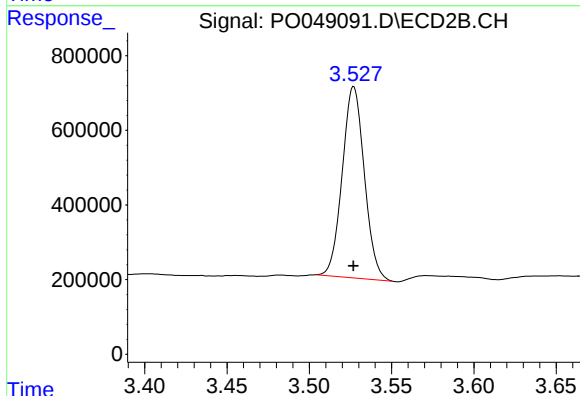


#1 Tetrachloro-m-xylene

R.T.: 3.527 min
Delta R.T.: 0.000 min
Response: 4780603
Conc: 26.21 ng/ml

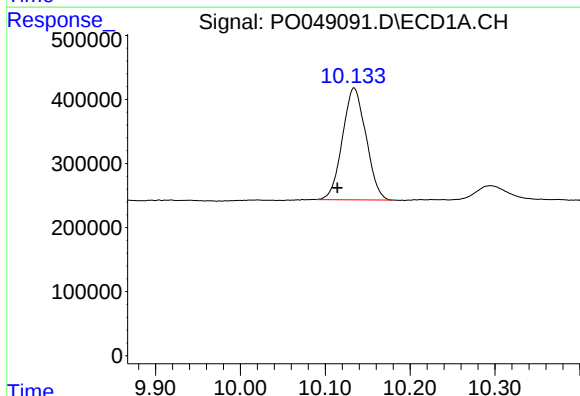

#2 Decachlorobiphenyl

R.T.: 10.133 min
Delta R.T.: 0.019 min
Response: 3368655
Conc: 15.12 ng/ml m

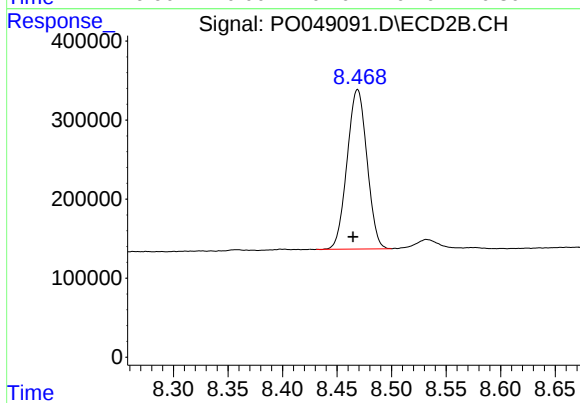

#2 Decachlorobiphenyl

R.T.: 8.469 min
Delta R.T.: 0.004 min
Response: 2560702
Conc: 13.80 ng/ml