

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091818\
Data File : P0049100.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Sep 2018 19:18
Operator : SM/SJ
Sample : J4929-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SP-PIT-6

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 19 01:06:24 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091118.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 12 08:13:07 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.397	3.526	4248057	5044313	25.930	27.651
2) SA Decachlor...	10.118	8.463	2988987	2271726	13.416	12.242

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091818\
Data File : P0049100.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Sep 2018 19:18
Operator : SM/SJ
Sample : J4929-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SP-PIT-6

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 19 01:06:24 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091118.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 12 08:13:07 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

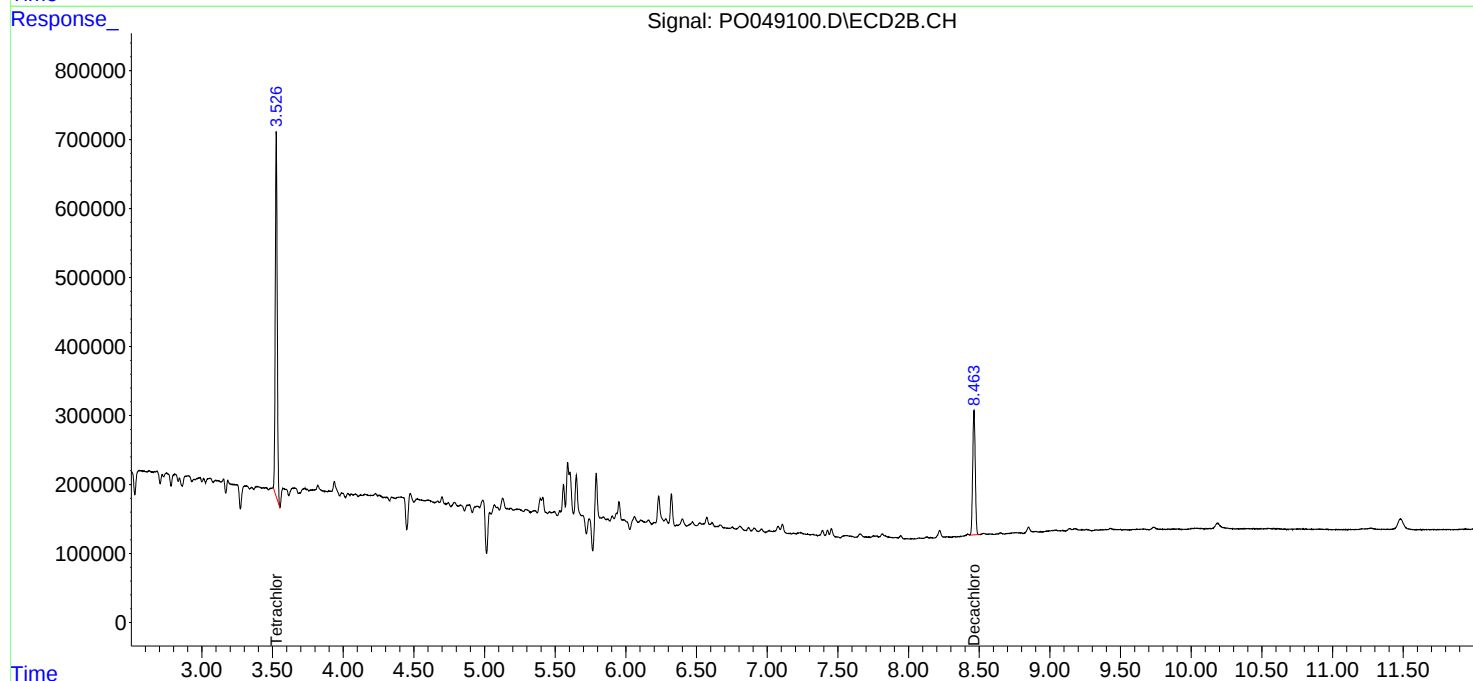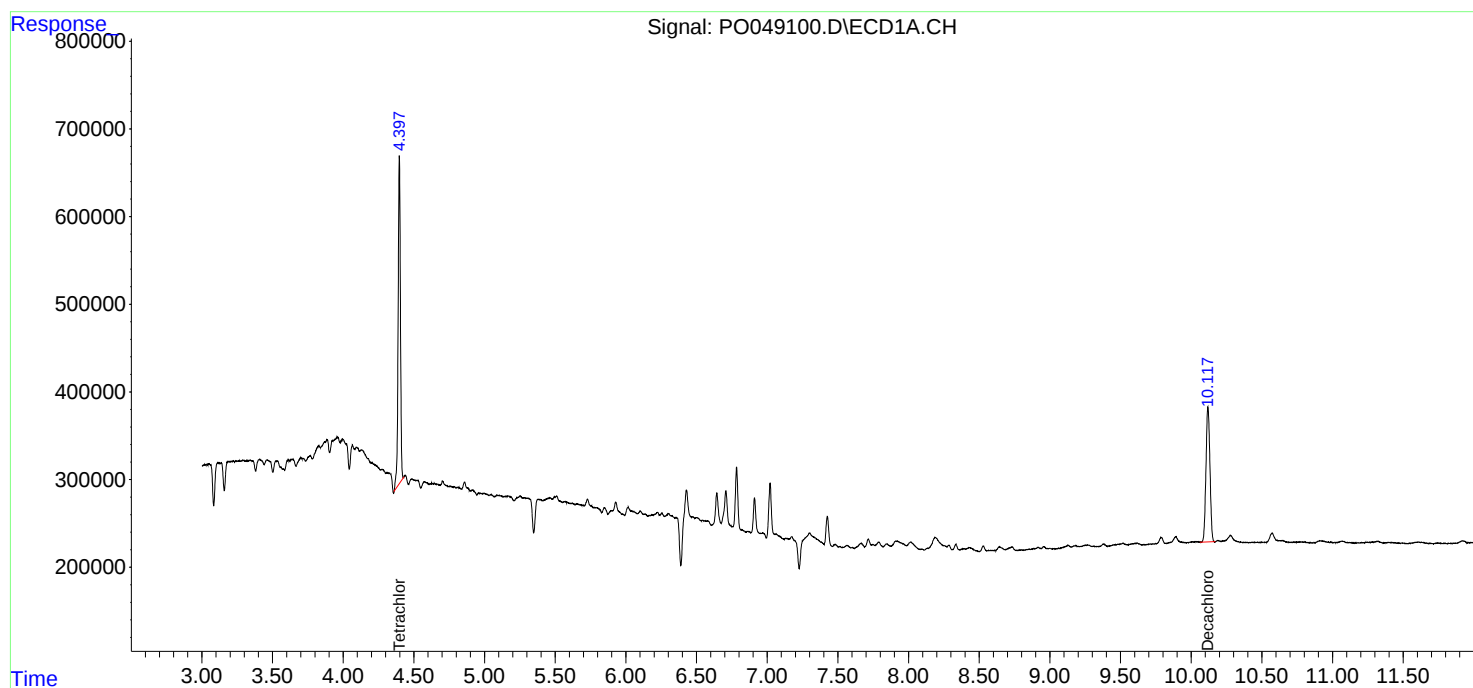


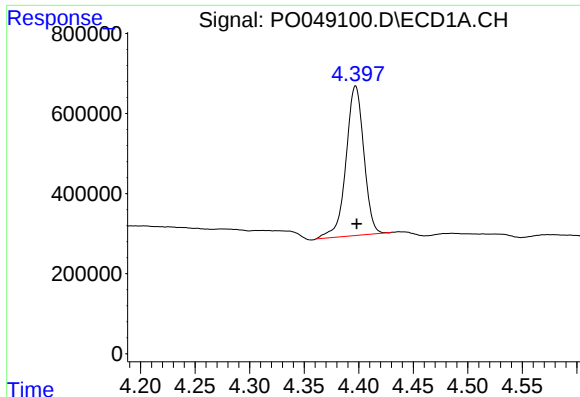

#1 Tetrachloro-m-xylene


R.T.: 4.397 min
Delta R.T.: 0.000 min
Response: 4248057
Conc: 25.93 ng/ml

Instrument :
ECD_O
ClientSampleId :
SP-PIT-6

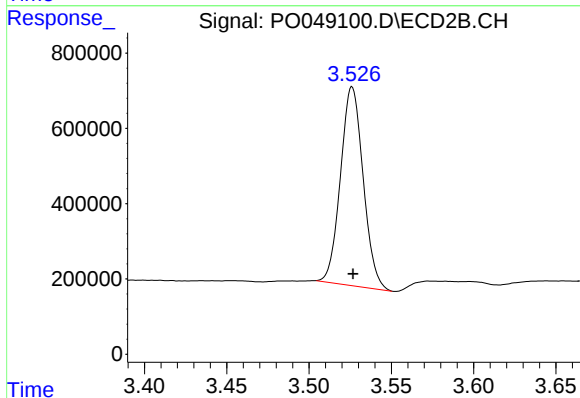


#1 Tetrachloro-m-xylene

R.T.: 3.526 min
Delta R.T.: 0.000 min
Response: 5044313
Conc: 27.65 ng/ml

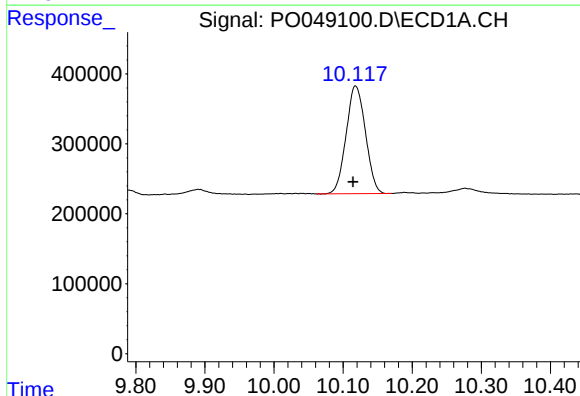

#2 Decachlorobiphenyl

R.T.: 10.118 min
Delta R.T.: 0.003 min
Response: 2988987
Conc: 13.42 ng/ml

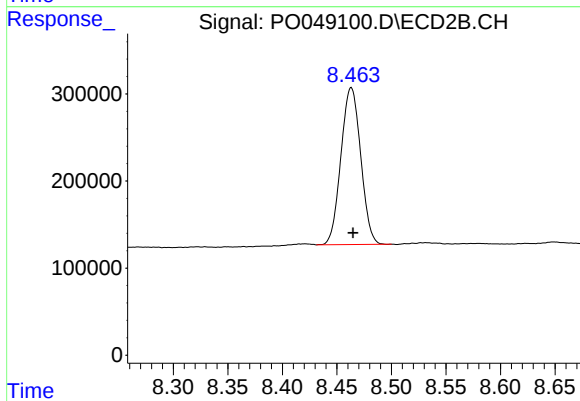

#2 Decachlorobiphenyl

R.T.: 8.463 min
Delta R.T.: -0.002 min
Response: 2271726
Conc: 12.24 ng/ml