

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091818\
 Data File : P0049119.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Sep 2018 1:41
 Operator : SM/SJ
 Sample : J4931-02
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 091418-SIDI-E-D-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 19 04:35:24 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091118.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 12 08:13:07 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.397	3.527	6038783	6152216	36.860m	33.724m
2) SA Decachlor...	10.120	8.464	5120685	3948509	22.984	21.278

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091818\
Data File : PO049119.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Sep 2018 1:41
Operator : SM/SJ
Sample : J4931-02
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
091418-SIDI-E-D-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 19 04:35:24 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091118.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 12 08:13:07 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

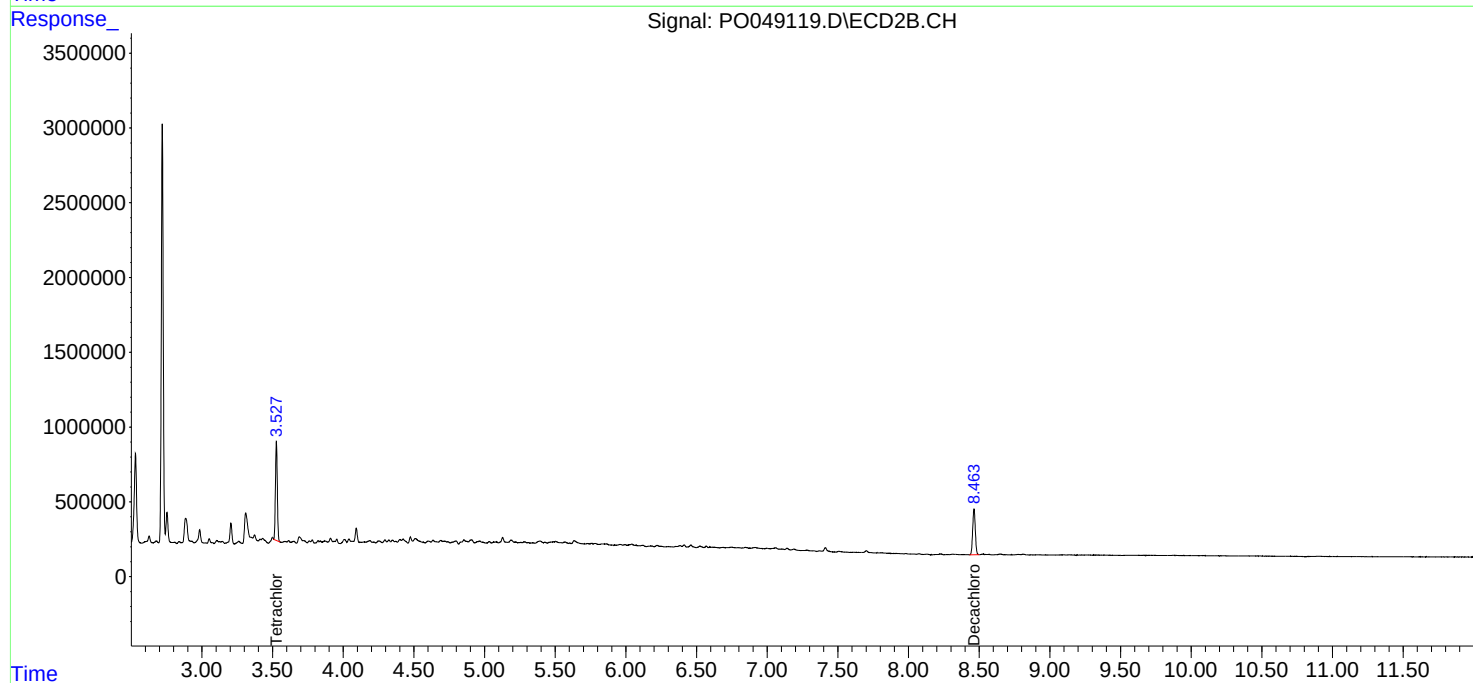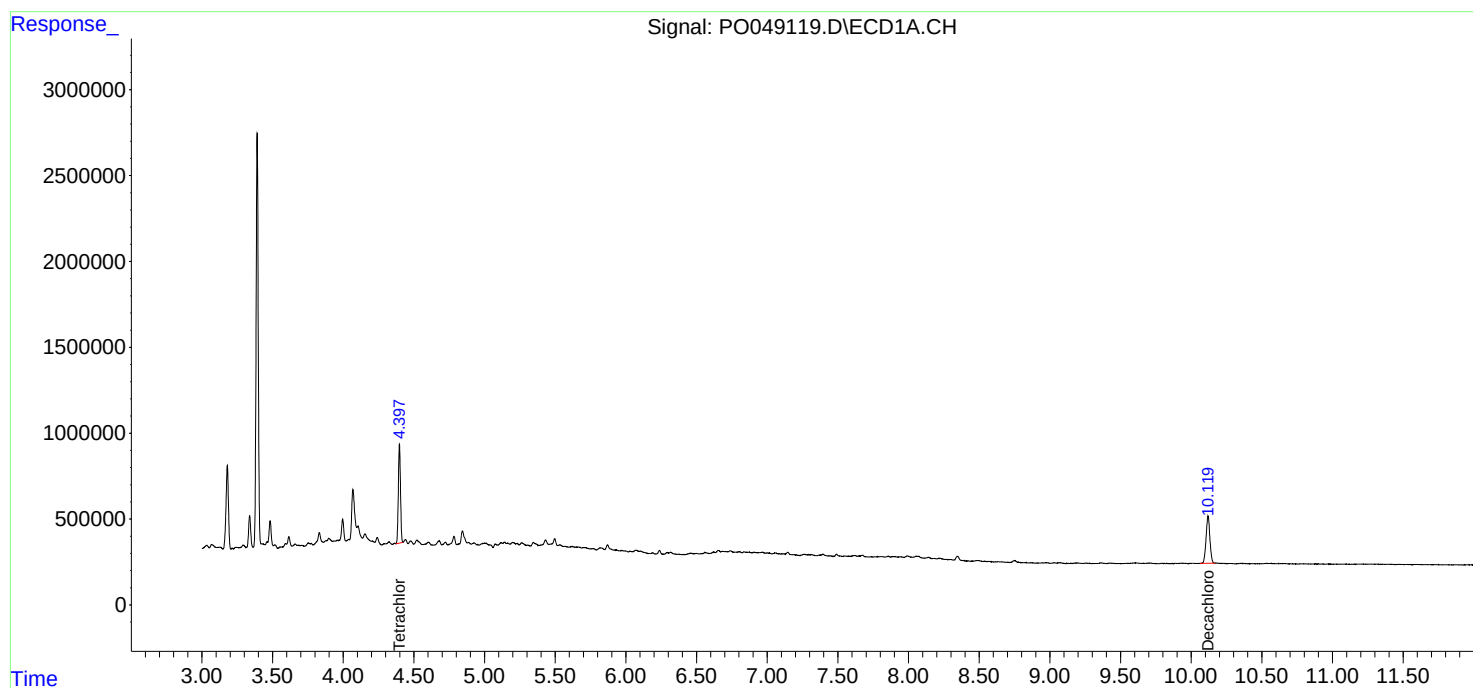


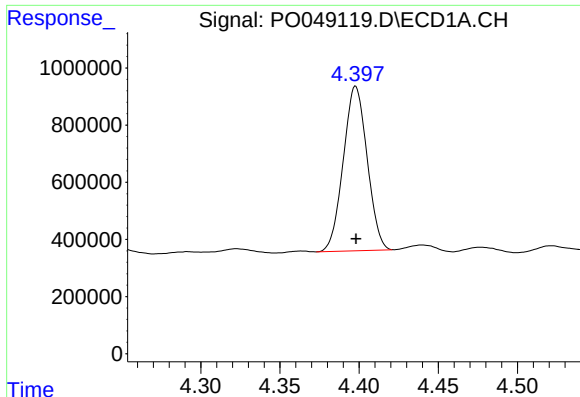

#1 Tetrachloro-m-xylene


R.T.: 4.397 min
Delta R.T.: 0.000 min
Response: 6038783
Conc: 36.86 ng/ml m

Instrument :
ECD_O
ClientSampleId :
091418-SIDI-E-D-S

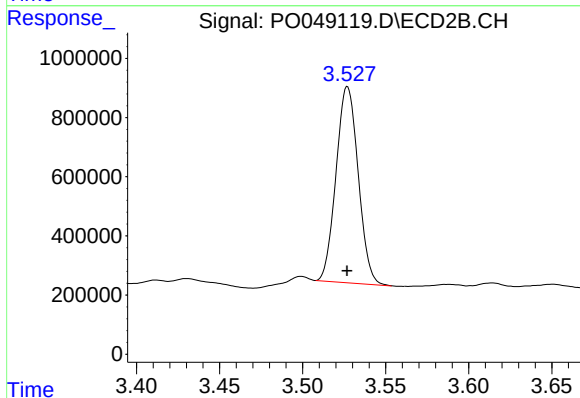


#1 Tetrachloro-m-xylene

R.T.: 3.527 min
Delta R.T.: 0.000 min
Response: 6152216
Conc: 33.72 ng/ml m

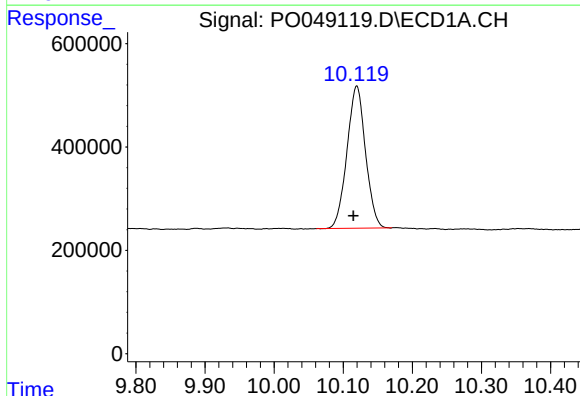

#2 Decachlorobiphenyl

R.T.: 10.120 min
Delta R.T.: 0.005 min
Response: 5120685
Conc: 22.98 ng/ml

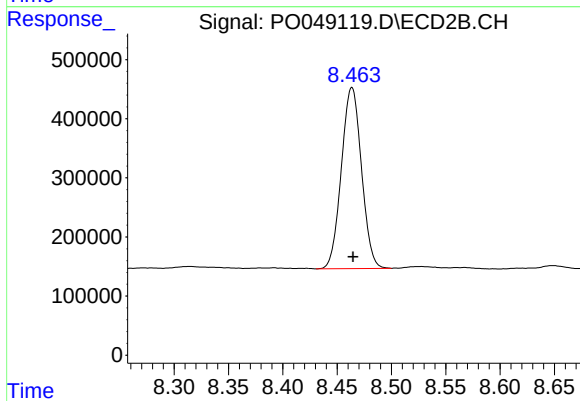

#2 Decachlorobiphenyl

R.T.: 8.464 min
Delta R.T.: -0.001 min
Response: 3948509
Conc: 21.28 ng/ml