

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091818\
 Data File : P0049121.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Sep 2018 2:13
 Operator : SM/SJ
 Sample : J4931-04
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 091418-SIDI-E-U-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 19 04:37:03 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091118.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 12 08:13:07 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.397	3.526	5698115	5588591	34.781m	30.634m
2) SA Decachlor...	10.116	8.464	5360351	3956910	24.060	21.323

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091818\
Data File : P0049121.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Sep 2018 2:13
Operator : SM/SJ
Sample : J4931-04
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
091418-SIDI-E-U-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 19 04:37:03 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091118.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 12 08:13:07 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

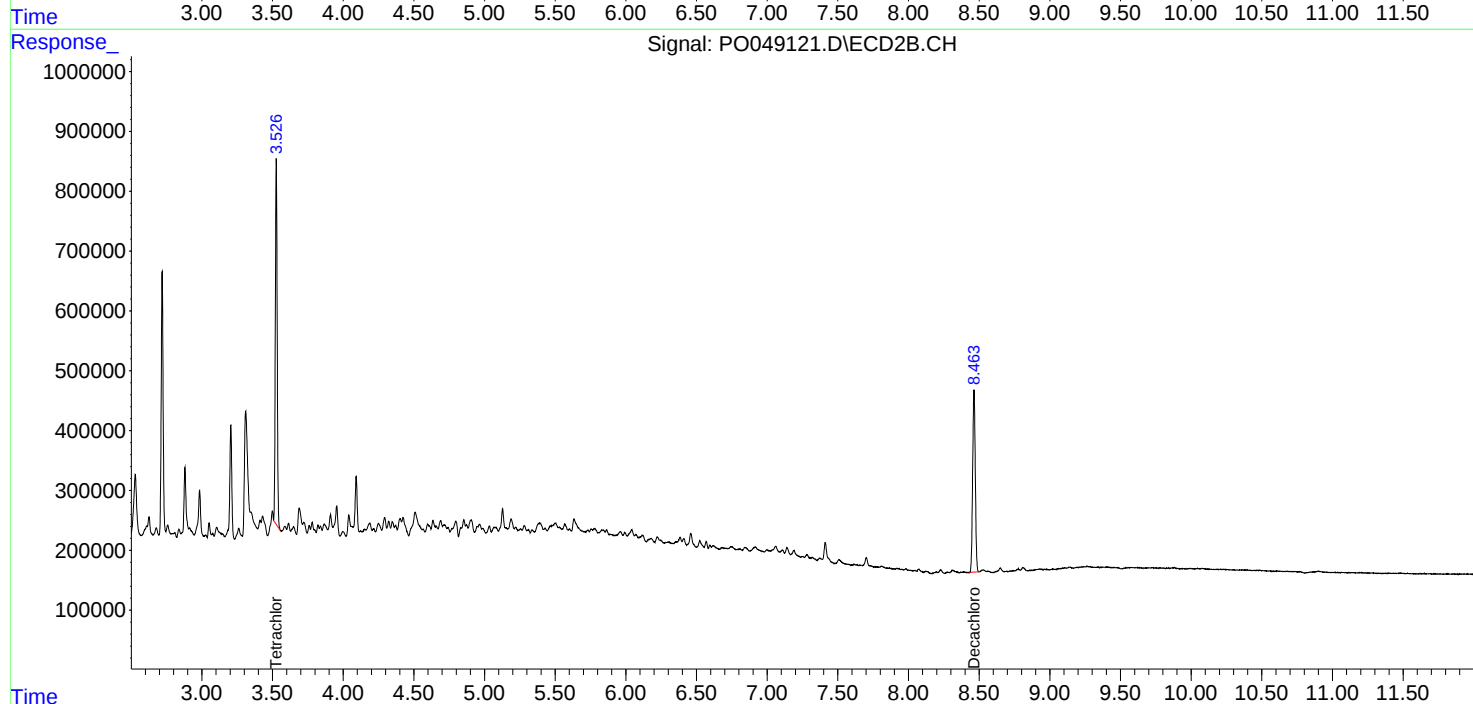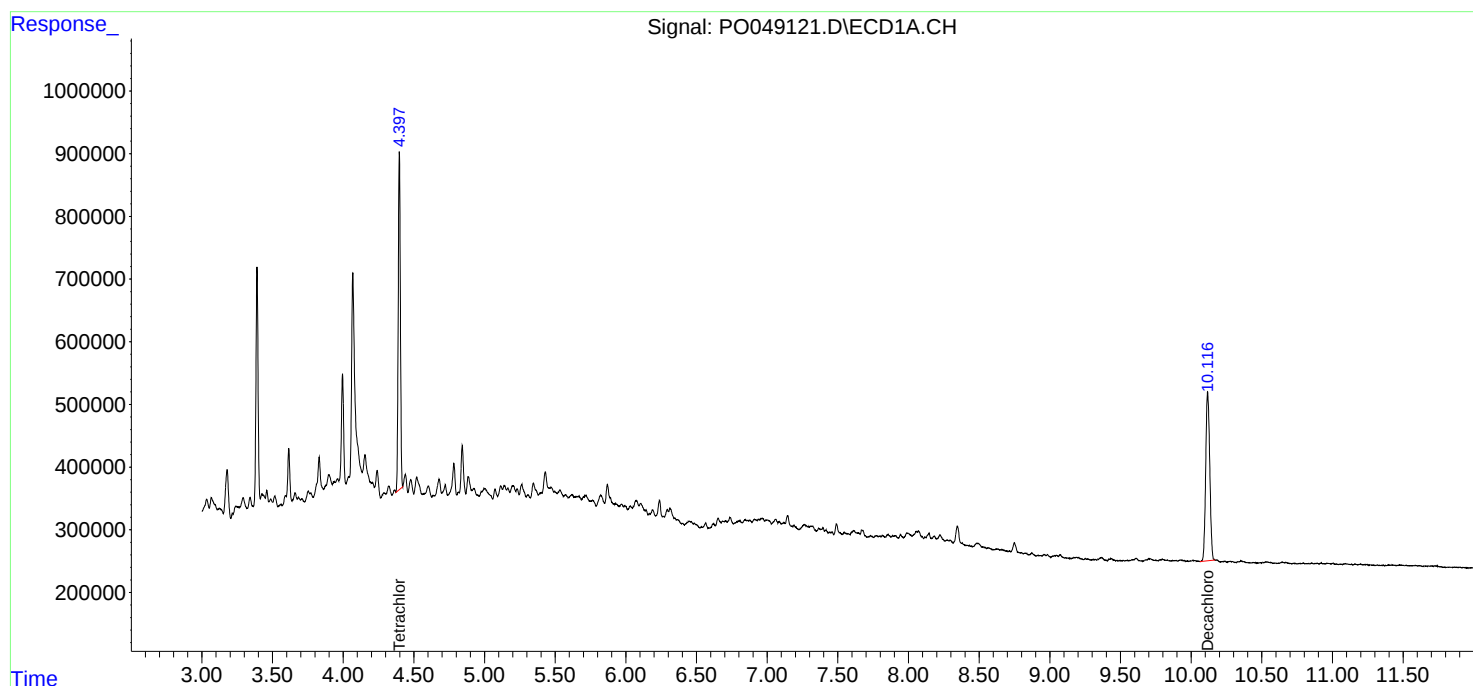


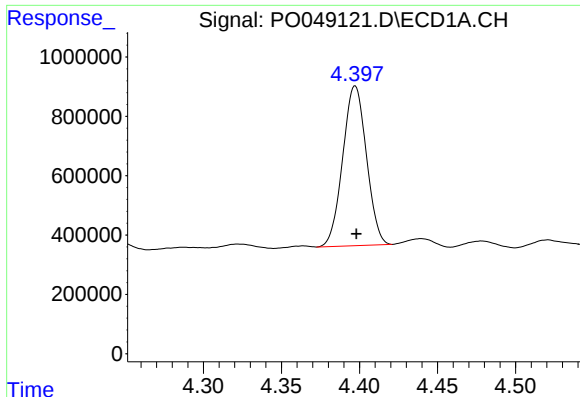

#1 Tetrachloro-m-xylene


R.T.: 4.397 min
Delta R.T.: -0.001 min
Response: 5698115
Conc: 34.78 ng/ml m

Instrument :
ECD_O
ClientSampleId :
091418-SIDI-E-U-S

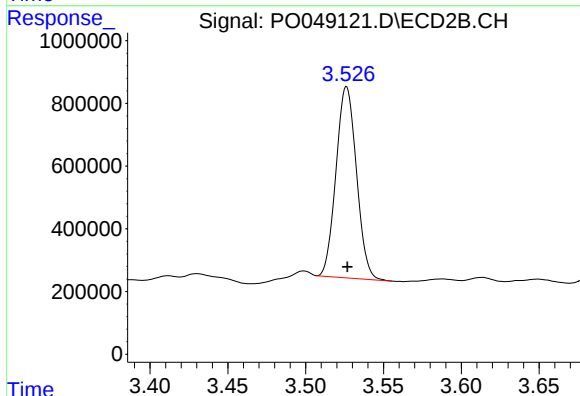


#1 Tetrachloro-m-xylene

R.T.: 3.526 min
Delta R.T.: 0.000 min
Response: 5588591
Conc: 30.63 ng/ml m

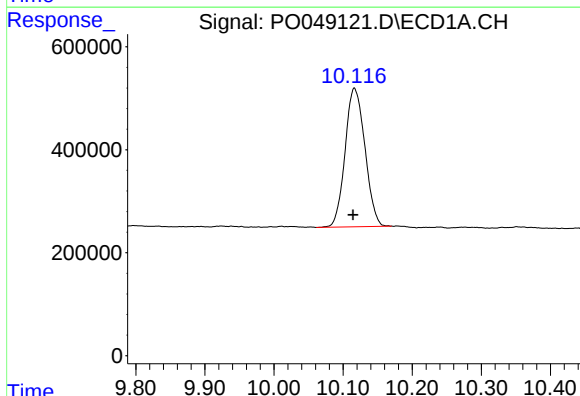

#2 Decachlorobiphenyl

R.T.: 10.116 min
Delta R.T.: 0.002 min
Response: 5360351
Conc: 24.06 ng/ml

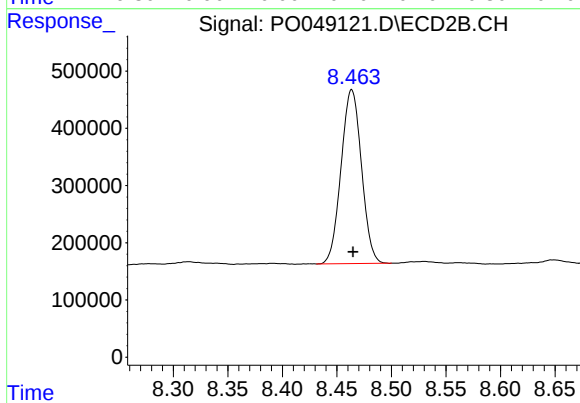

#2 Decachlorobiphenyl

R.T.: 8.464 min
Delta R.T.: -0.001 min
Response: 3956910
Conc: 21.32 ng/ml