

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0100318\
 Data File : P0049568.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Oct 2018 8:38
 Operator : SM/SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 03 08:51:29 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0100118.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 02 05:32:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.385	3.515	6675963	6477417	18.905	19.044
2)	SA Decachlor...	10.092	8.444	8184087	5893655	17.271	19.290

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100318\
Data File : PO049568.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Oct 2018 8:38
Operator : SM/SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 08:51:29 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100118.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 02 05:32:25 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

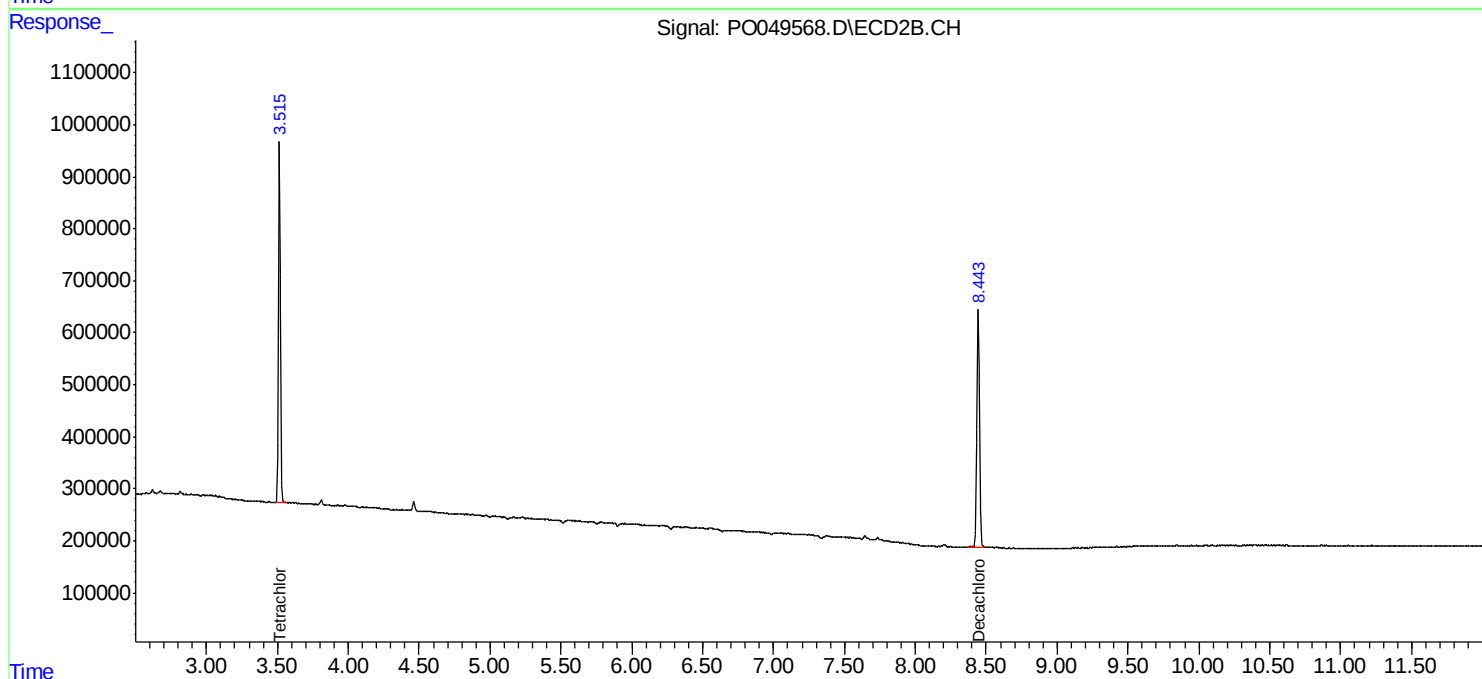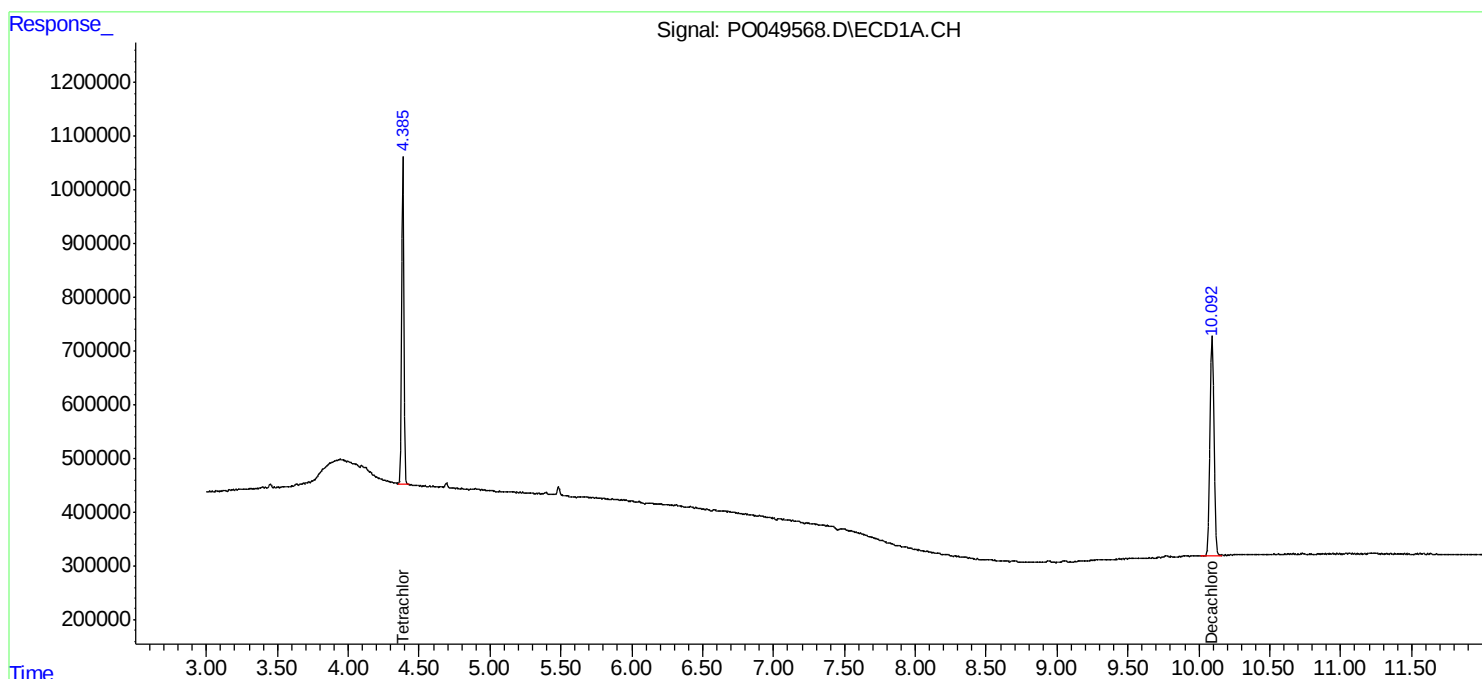


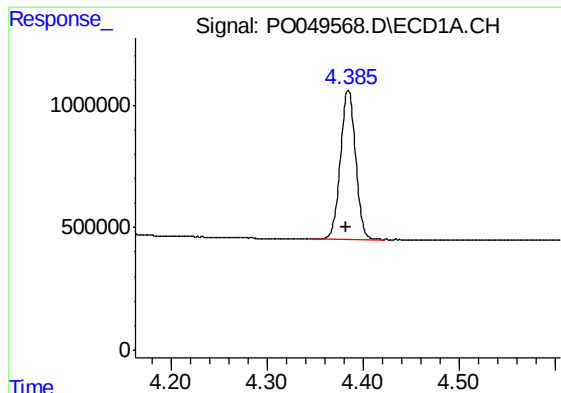

#1 Tetrachloro-m-xylene


R.T.: 4.385 min
Delta R.T.: 0.002 min
Response: 6675963
Conc: 18.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

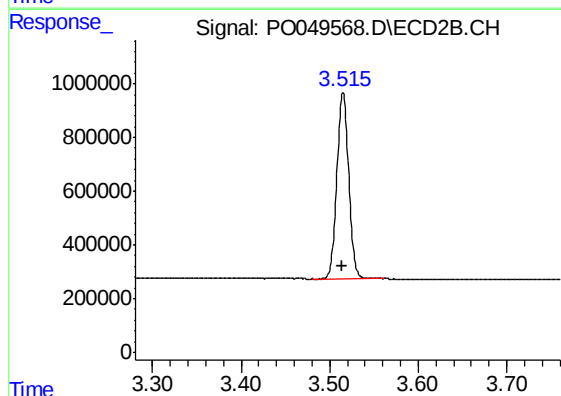


#1 Tetrachloro-m-xylene

R.T.: 3.515 min
Delta R.T.: 0.001 min
Response: 6477417
Conc: 19.04 ng/ml

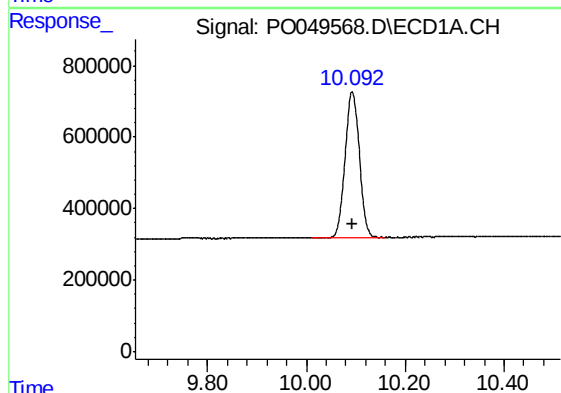

#2 Decachlorobiphenyl

R.T.: 10.092 min
Delta R.T.: -0.002 min
Response: 8184087
Conc: 17.27 ng/ml

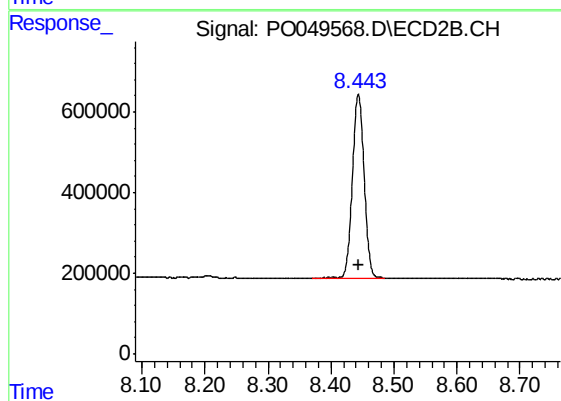

#2 Decachlorobiphenyl

R.T.: 8.444 min
Delta R.T.: 0.000 min
Response: 5893655
Conc: 19.29 ng/ml