

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102418\
 Data File : P0050464.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Oct 2018 10:40
 Operator : SM/SJ
 Sample : J5604-03RE
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MS-VB-25868-BOX-1RE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 24 11:02:27 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101818.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 19 02:02:26 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.358	3.353	2380371	1938036	7.977	9.858
2)	SA Decachlor...	10.021	8.106	1209729	1095620	5.575m	5.732

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102418\
Data File : PO050464.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Oct 2018 10:40
Operator : SM/SJ
Sample : J5604-03RE
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MS-VB-25868-BOX-1RE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 24 11:02:27 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101818.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 19 02:02:26 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

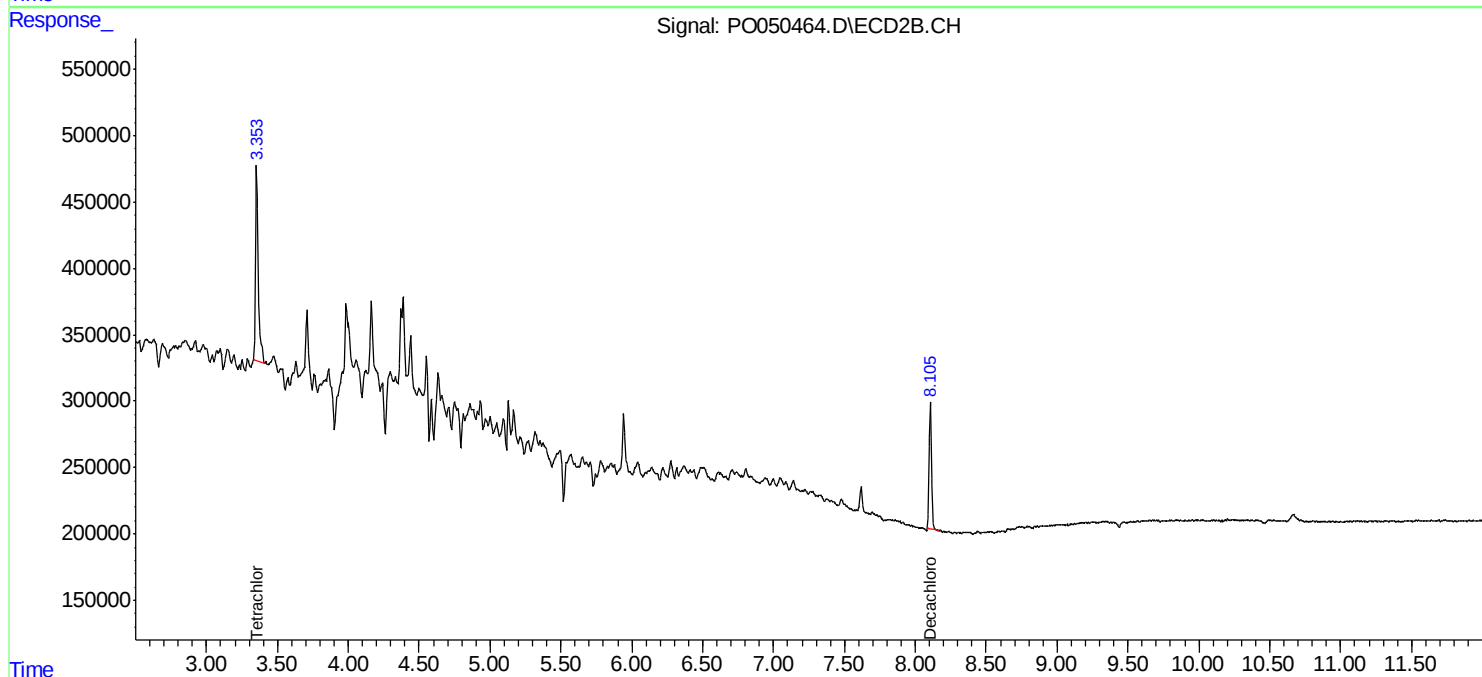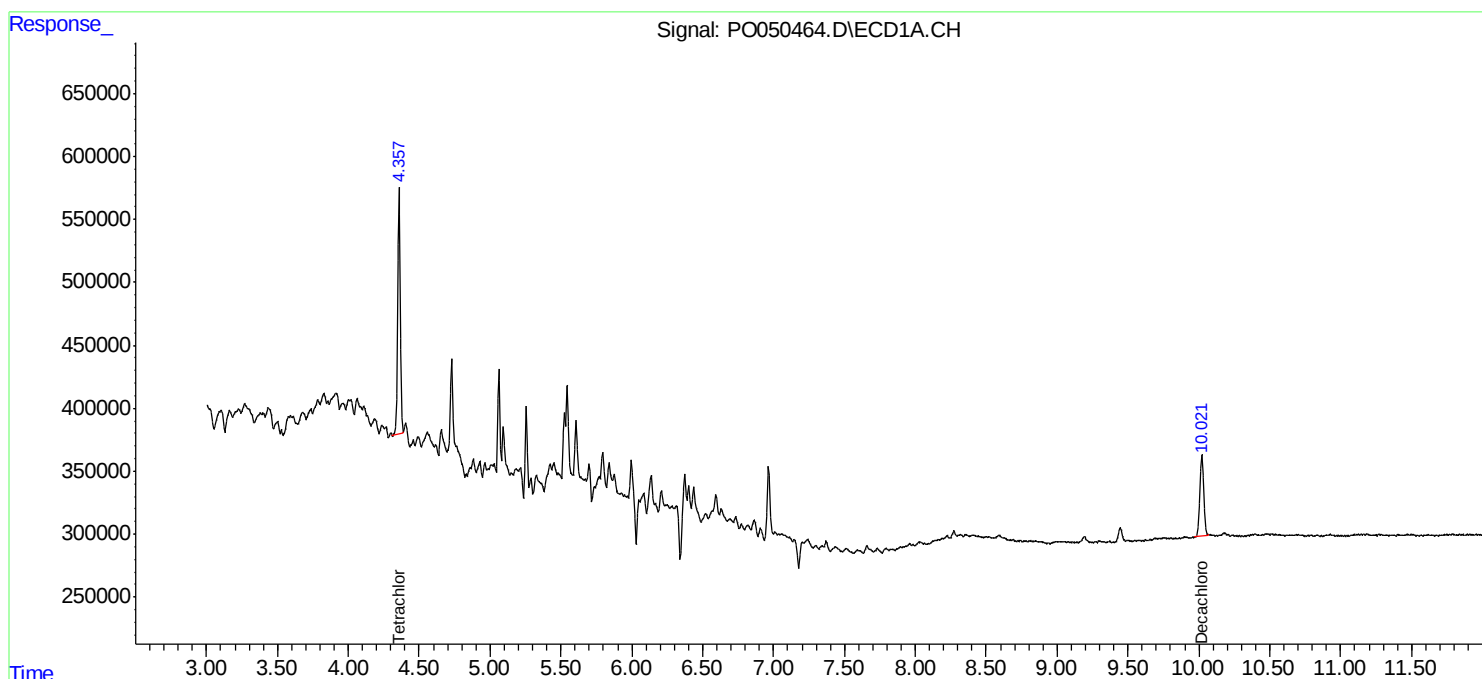


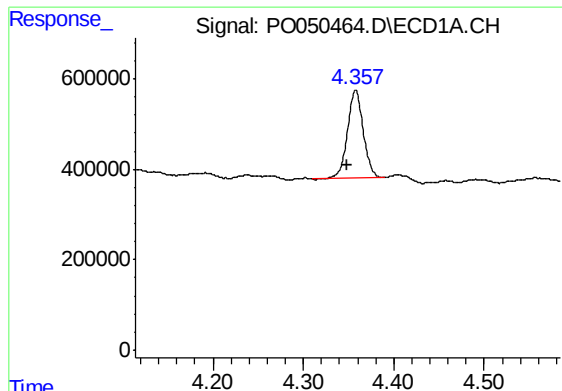

#1 Tetrachloro-m-xylene


R.T.: 4.358 min
Delta R.T.: 0.009 min
Response: 2380371
Conc: 7.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
MS-VB-25868-BOX-1RE

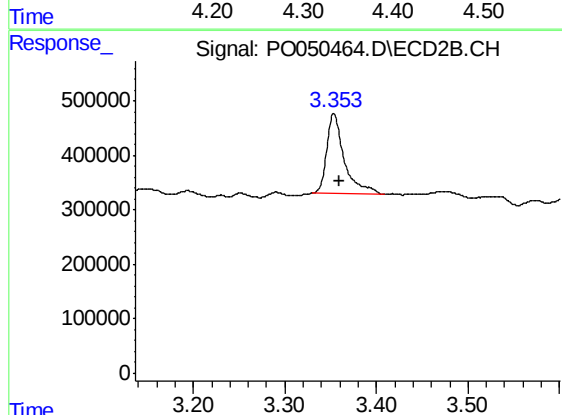


#1 Tetrachloro-m-xylene

R.T.: 3.353 min
Delta R.T.: -0.006 min
Response: 1938036
Conc: 9.86 ng/ml

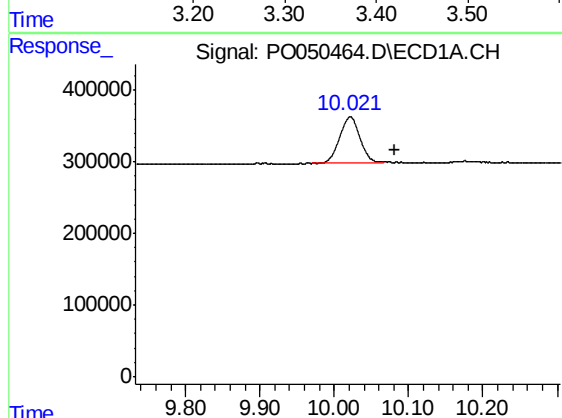

#2 Decachlorobiphenyl

R.T.: 10.021 min
Delta R.T.: -0.060 min
Response: 1209729
Conc: 5.58 ng/ml m

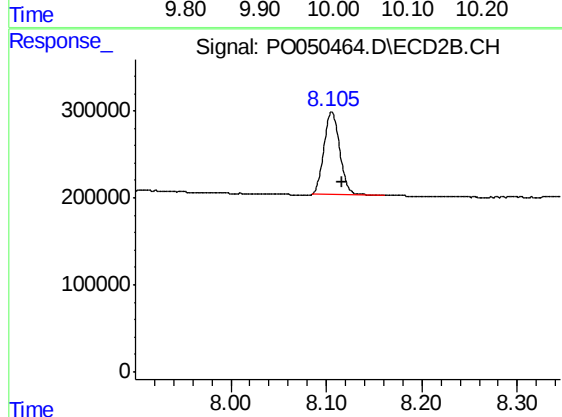

#2 Decachlorobiphenyl

R.T.: 8.106 min
Delta R.T.: -0.010 min
Response: 1095620
Conc: 5.73 ng/ml