

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0102418\
 Data File : P0050482.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Oct 2018 17:19
 Operator : SM/SJ
 Sample : J4767-01 10X
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SPRINGDALE-SV33366L

Manual Integrations
 APPROVED

Sohil
 10/25/2018 1:58:47 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 25 11:05:52 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101818.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 19 02:02:26 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.370	3.355	719723	362857	2.412	1.846m
2)	SA Decachlor...	10.043	8.113	485203	303754	2.236m	1.589 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102418\
Data File : PO050482.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Oct 2018 17:19
Operator : SM/SJ
Sample : J4767-01 10X
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SPRINGDALE-SV33366L


Manual Integrations
APPROVED

Sohil
10/25/2018 1:58:47 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 25 11:05:52 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101818.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 19 02:02:26 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

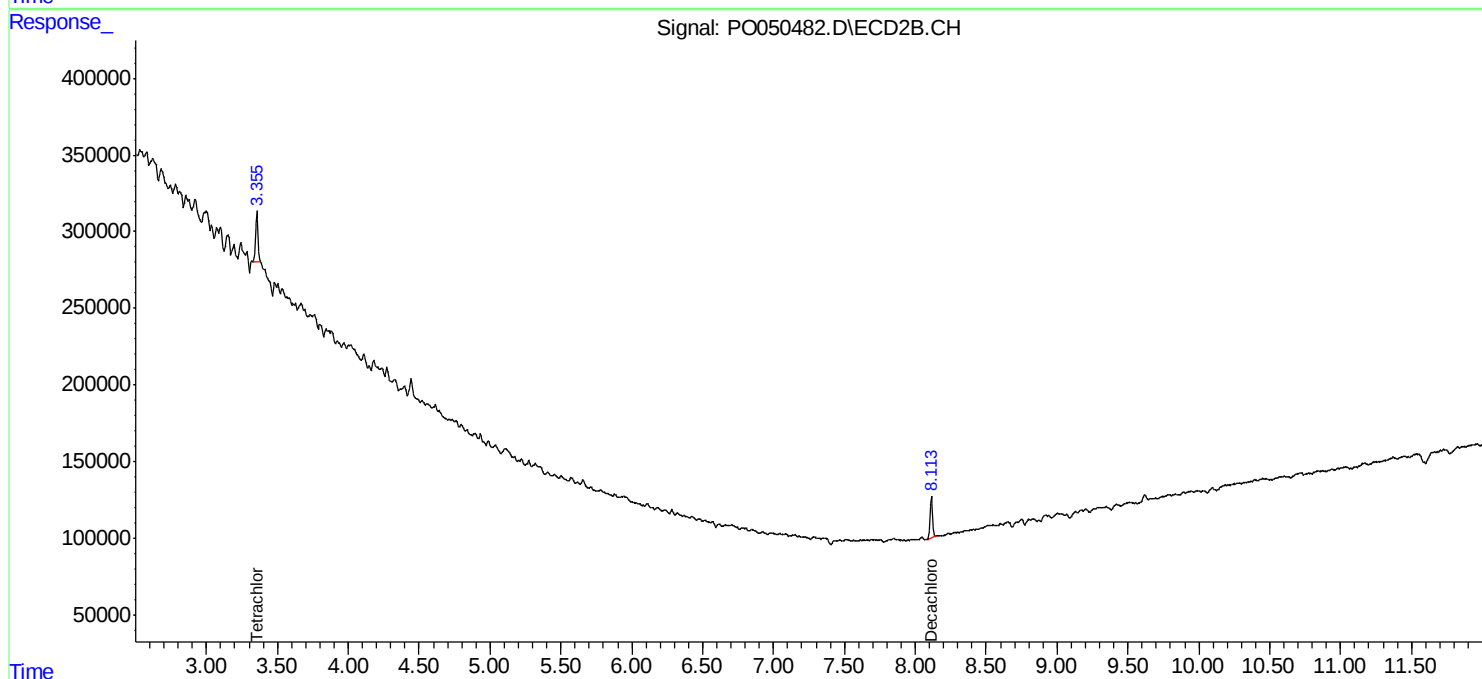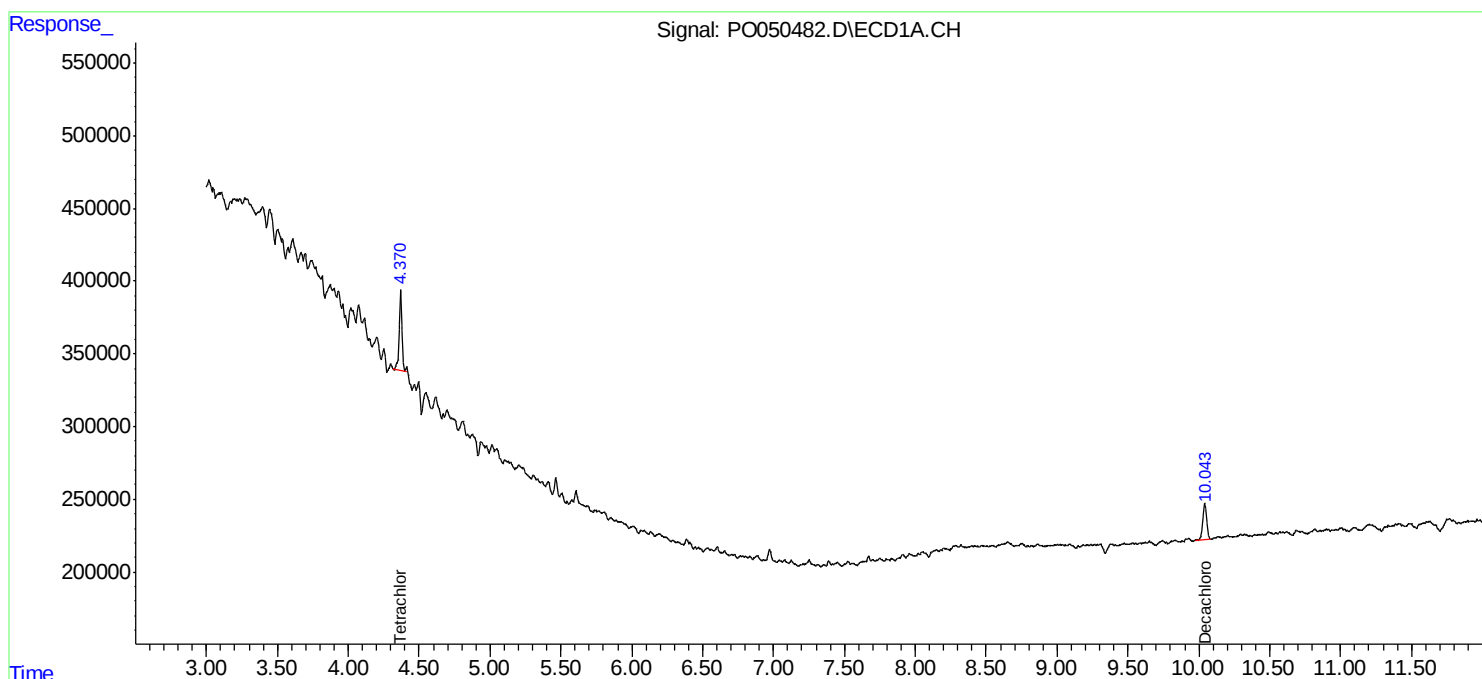

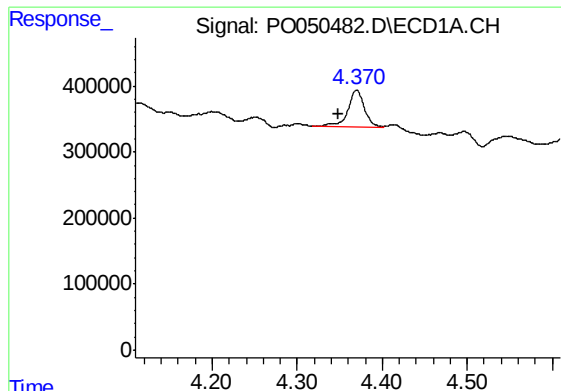


#1 Tetrachloro-m-xylene

R.T.: 4.370 min
Delta R.T.: 0.021 min
Response: 719723
Conc: 2.41 ng/ml

Instrument :
ECD_O
ClientSampleId :
SPRINGDALE-SV33366L


Manual Integrations
APPROVED

Sohil
10/25/2018 1:58:47 PM

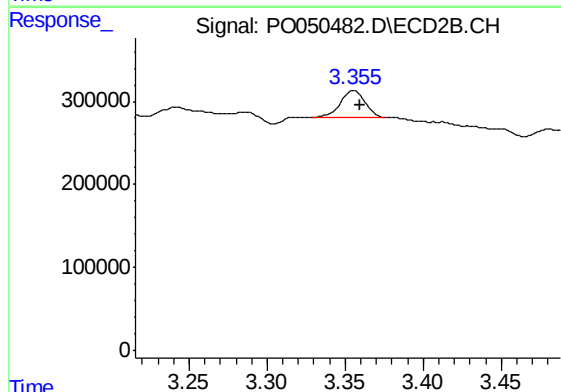


#1 Tetrachloro-m-xylene

R.T.: 3.355 min
Delta R.T.: -0.005 min
Response: 362857
Conc: 1.85 ng/ml m

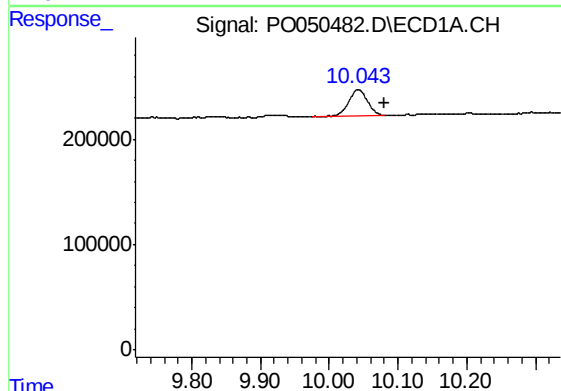

#2 Decachlorobiphenyl

R.T.: 10.043 min
Delta R.T.: -0.037 min
Response: 485203
Conc: 2.24 ng/ml m

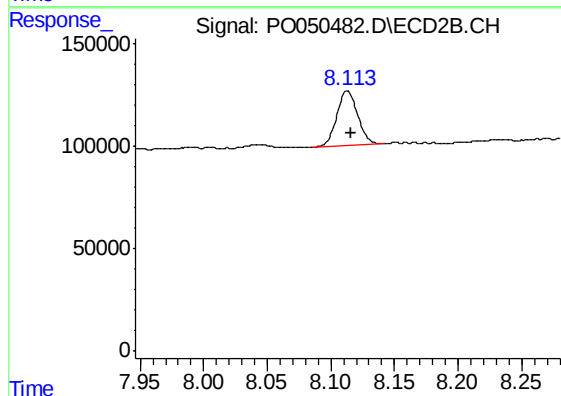

#2 Decachlorobiphenyl

R.T.: 8.113 min
Delta R.T.: -0.003 min
Response: 303754
Conc: 1.59 ng/ml